


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030817\
 Data File : BF093455.D
 Acq On : 9 Mar 2017 4:51
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 07 15:55:22 2017

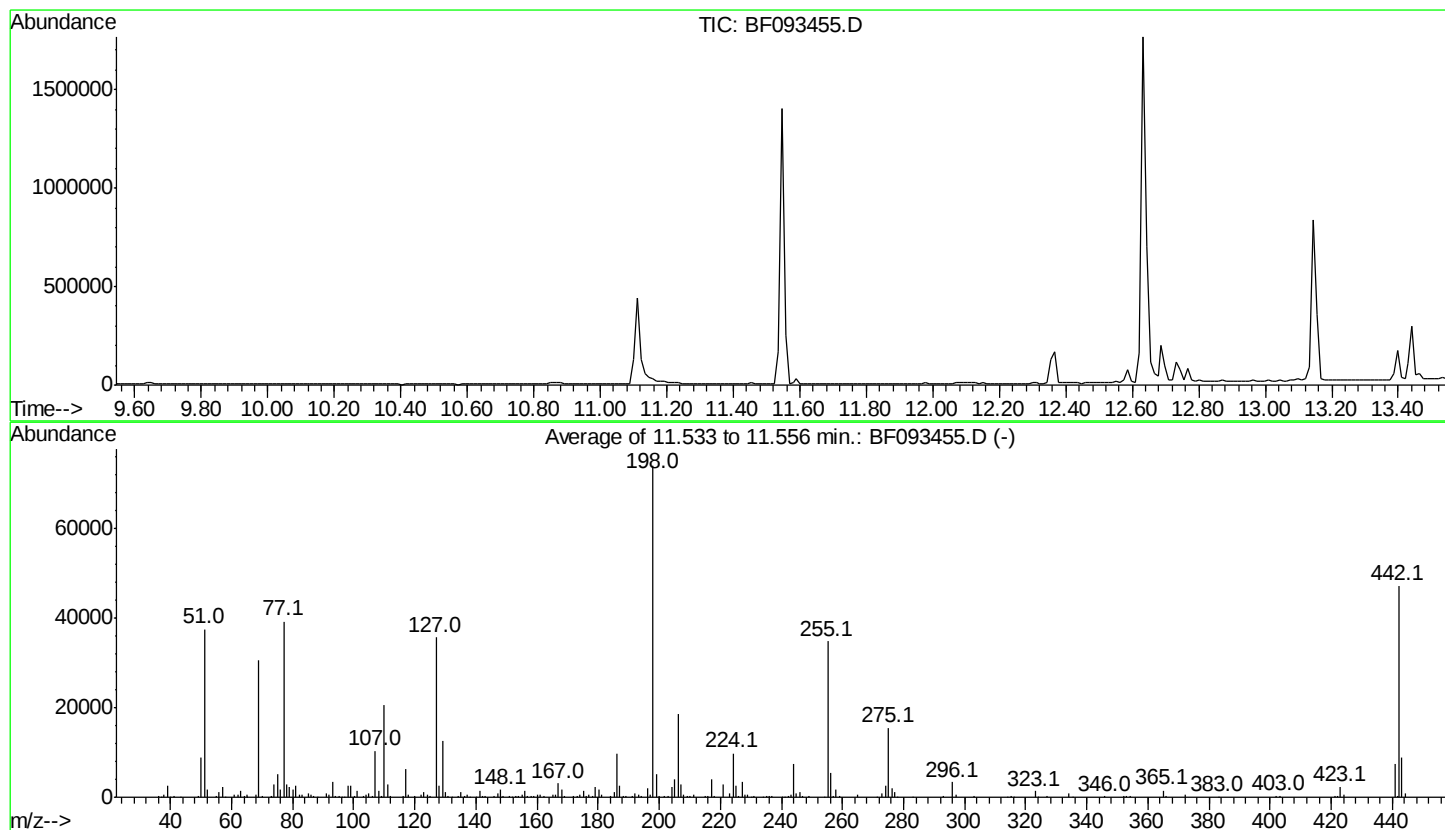

AutoFind: Scans 844, 845, 846; Background Corrected with Scan 841

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.7	37508	PASS
68	69	0.00	2	1.9	572	PASS
69	198	0.00	100	41.3	30536	PASS
70	69	0.00	2	0.7	203	PASS
127	198	10	80	48.3	35686	PASS
197	198	0.00	2	0.8	590	PASS
198	198	100	100	100.0	73959	PASS
199	198	5	9	6.8	5016	PASS
275	198	10	60	20.9	15437	PASS
365	198	1	100	2.0	1484	PASS
441	442	0.01	24	15.9	7498	PASS
442	198	50	100	63.8	47176	PASS
443	442	15	24	19.1	8995	PASS