

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF030818\
 Data File : BF103535.D
 Acq On : 8 Mar 2018 23:35
 Operator : SJ/JU
 Sample : J1826-10
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-3-B-COMP

Quant Time: Mar 09 01:33:33 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 08 14:20:19 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.86	152	123880	20.00	ng	0.00
21) Naphthalene-d8	8.15	136	489524	20.00	ng	0.00
38) Acenaphthene-d10	9.91	164	180612	20.00	ng	0.00
63) Phenanthrene-d10	11.40	188	294435	20.00	ng	0.00
75) Chrysene-d12	14.06	240	220820	20.00	ng	0.00
86) Perylene-d12	15.57	264	174806	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.49	112	1089049	132.96	ng	0.00
7) Phenol-d6	6.50	99	1329982	132.70	ng	0.00
23) Nitrobenzene-d5	7.43	82	819887	95.65	ng	0.00
41) 2,4,6-Tribromophenol	10.70	330	161423	105.59	ng	0.00
44) 2-Fluorobiphenyl	9.22	172	1040051	104.80	ng	0.00
78) Terphenyl-d14	12.99	244	723598	78.77	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.62	163	122993	8.489	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF030818\
Data File : BF103535.D
Acq On : 8 Mar 2018 23:35
Operator : SJ/JU
Sample : J1826-10
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-3-B-COMP

Quant Time: Mar 09 01:33:33 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 08 14:20:19 2018
Response via : Initial Calibration

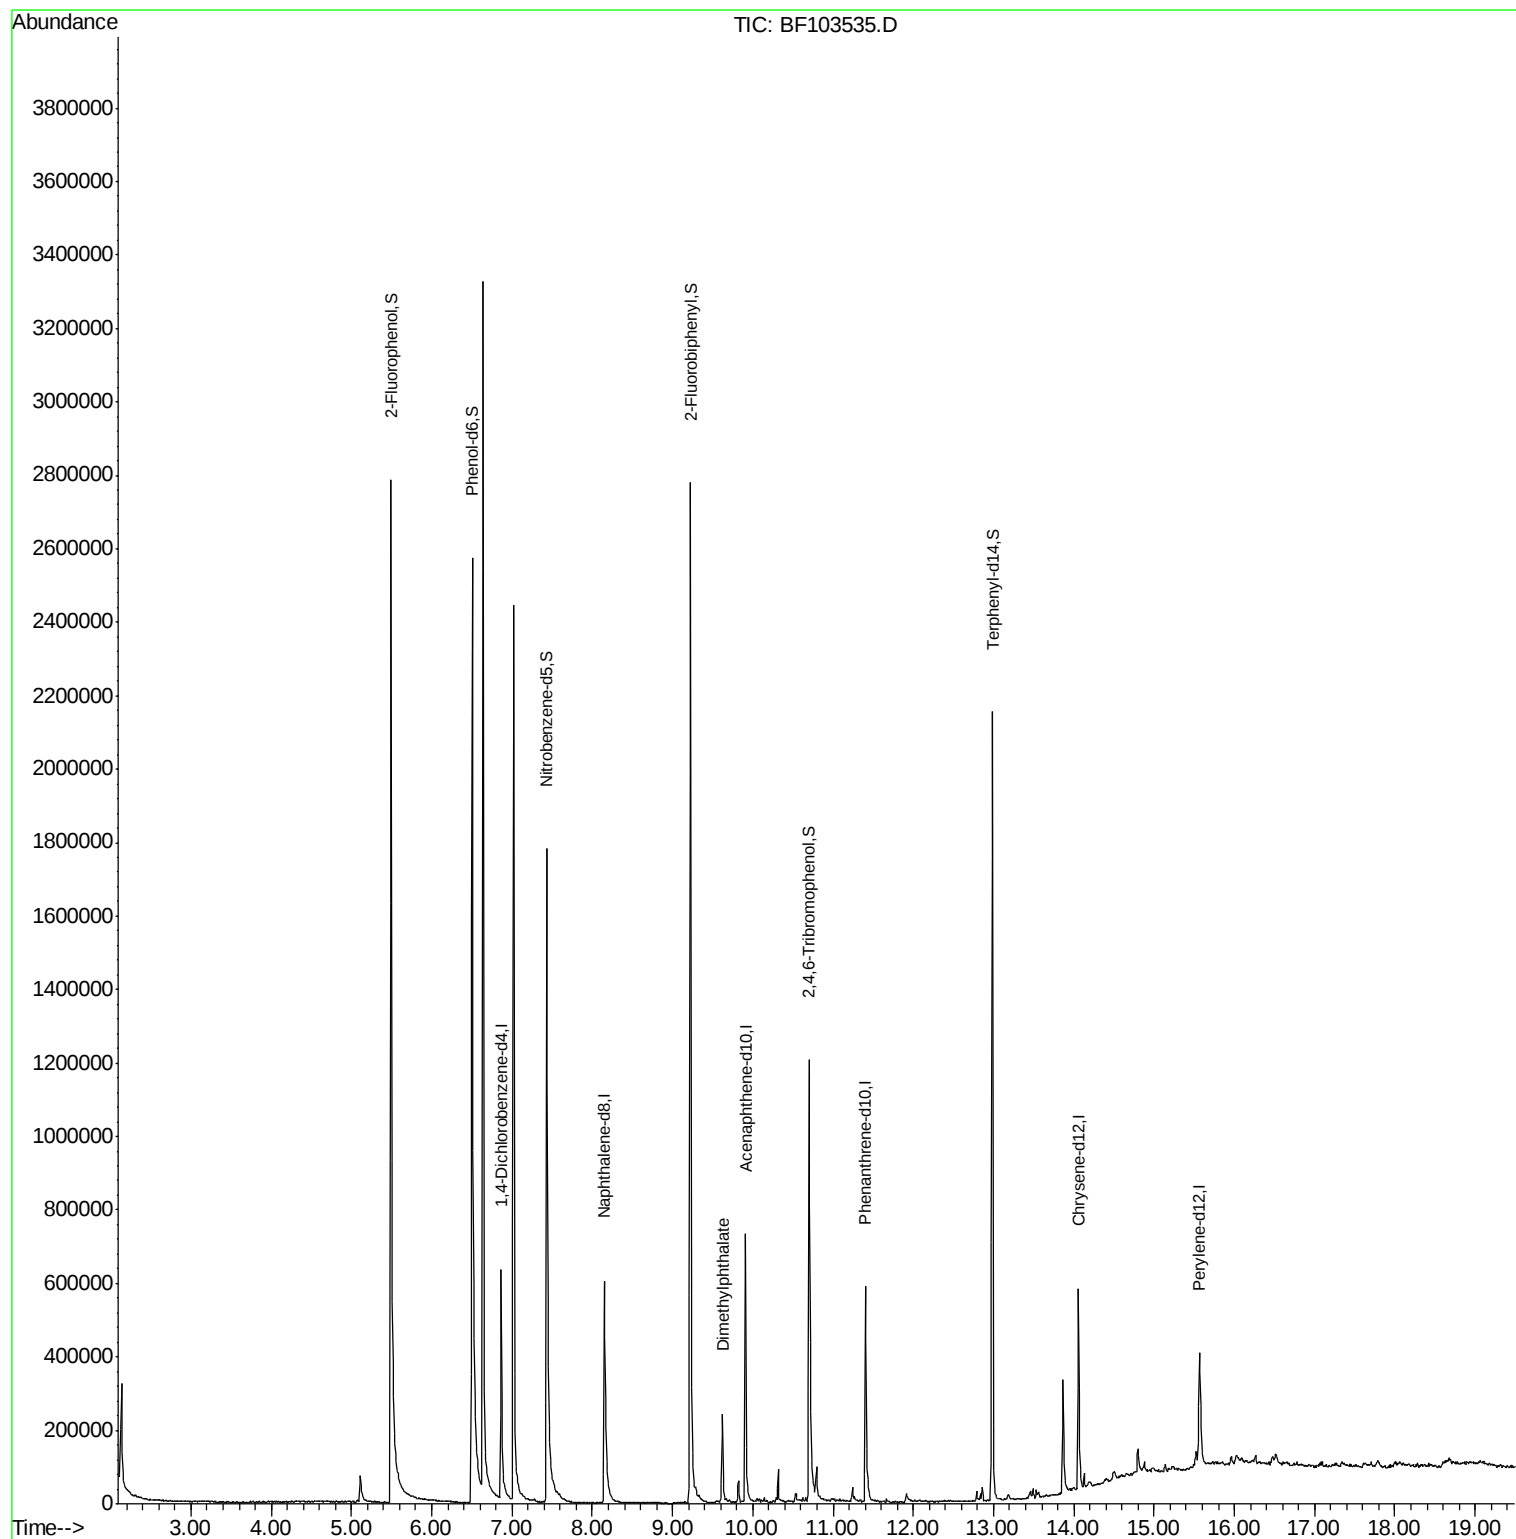







#1

1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.86 min Scan# 812
 Delta R.T. 0.00 min
 Lab File: BF103535.D
 Acq: 8 Mar 2018 23:35

Instrument :
 BNA_F
 ClientSampleId :
 TP-3-B-COMP




Tot Ion	Ratio	Lower	Upper
152	100		
150	159.0	124.6	186.8
115	67.5	50.1	75.1

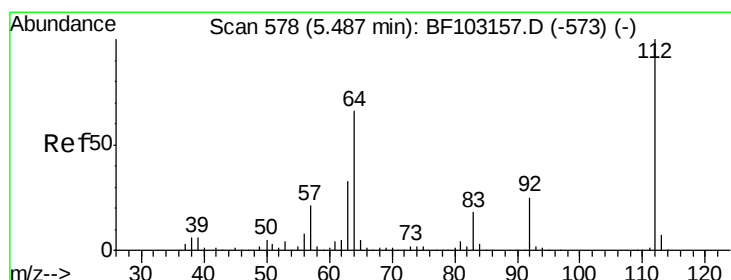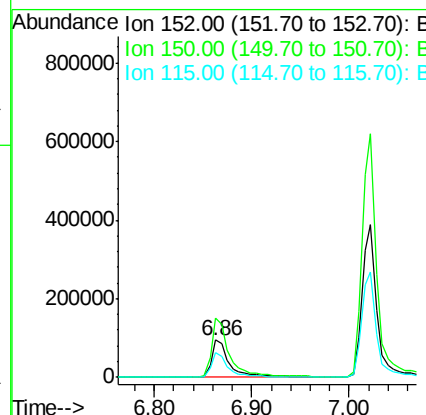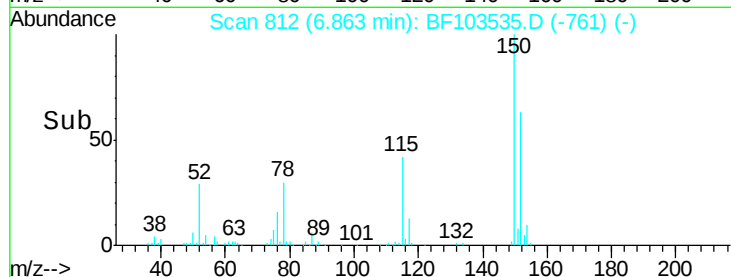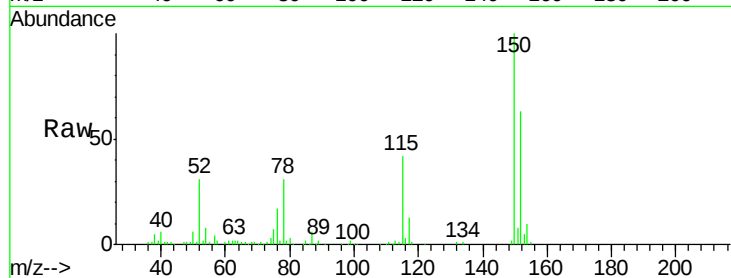


#5

2-Fluorophenol
 Concen: 132.960 ng
 RT: 5.49 min Scan# 579
 Delta R.T. 0.01 min
 Lab File: BF103535.D
 Acq: 8 Mar 2018 23:35

Tgt Ion	Ratio	Lower	Upper
112	100		
64	67.0	47.9	71.9
63	34.6	23.7	35.5

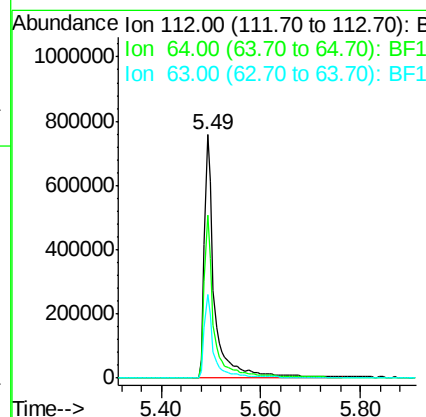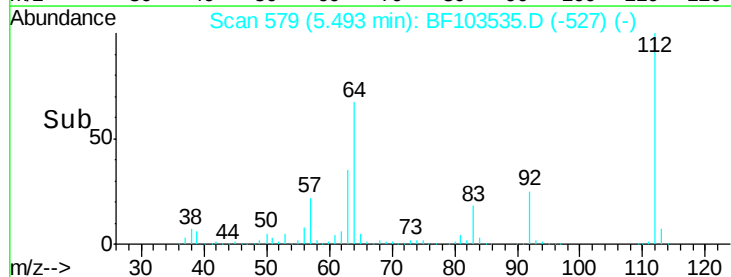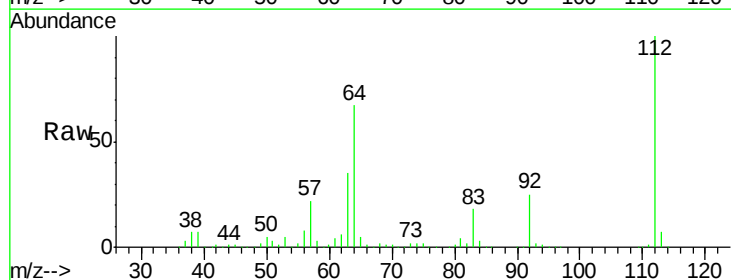

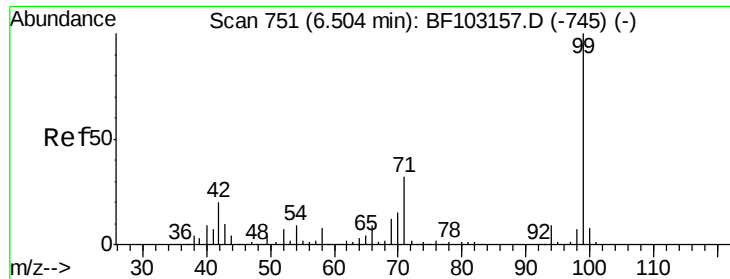

#7

Phenol-d6

Concen: 132.697 ng

RT: 6.50 min Scan# 751

Delta R.T. 0.00 min

Lab File: BF103535.D

Acq: 8 Mar 2018 23:35

Instrument :

BNA_F

ClientSampleId :

TP-3-B-COMP


Tot Ion: 99 Resp: 1329982

Ion Ratio Lower Upper




99 100

42 21.0 14.5 21.7

71 33.0 25.4 38.0

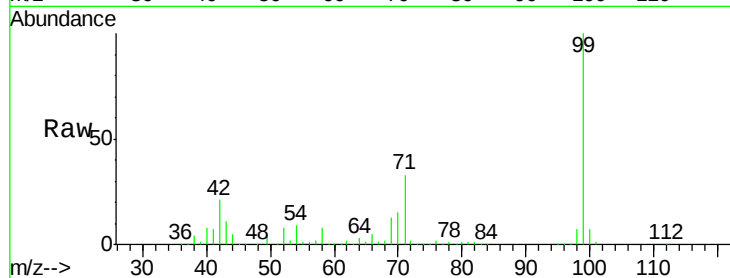

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

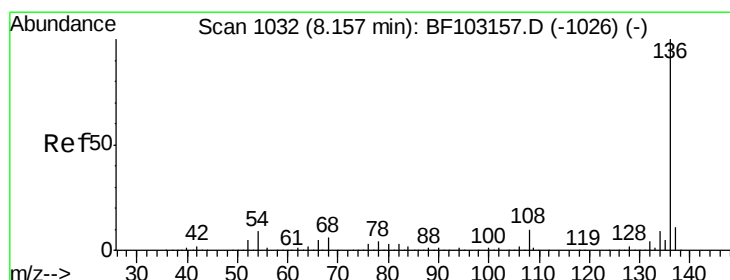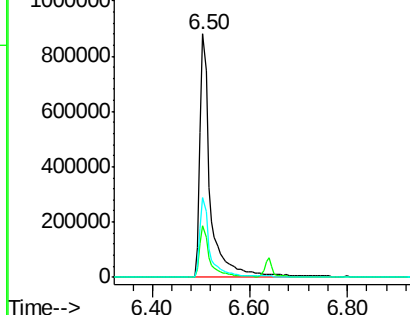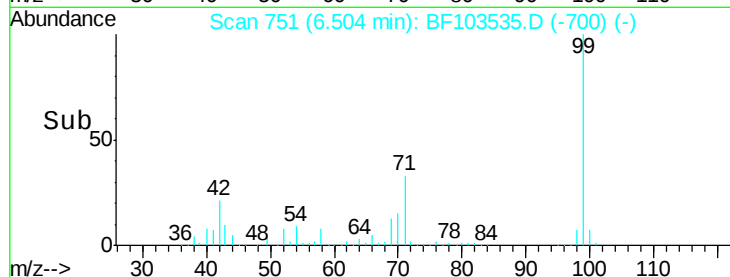

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.15 min Scan# 1031

Delta R.T. 0.00 min

Lab File: BF103535.D

Acq: 8 Mar 2018 23:35

Tgt Ion: 136 Resp: 489524


Ion Ratio Lower Upper

136 100



137 10.8 8.9 13.3


54 9.2 6.6 9.8

68 6.7 5.0 7.4

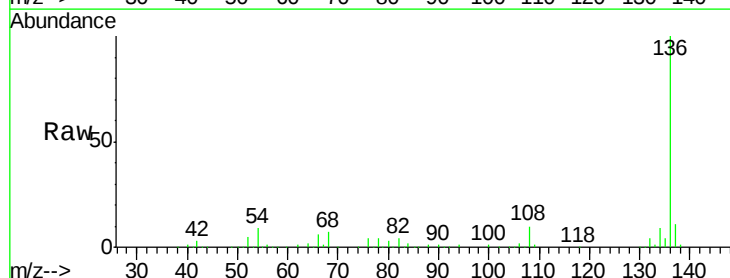

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1



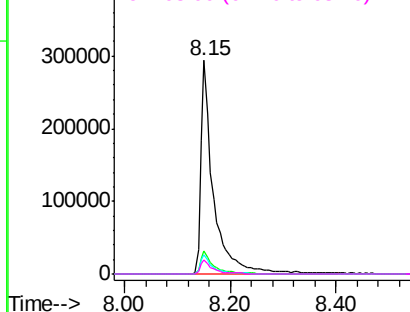
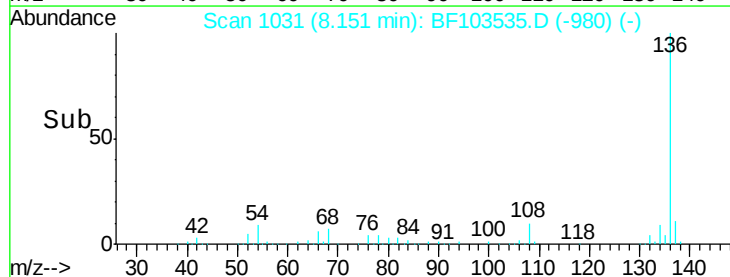


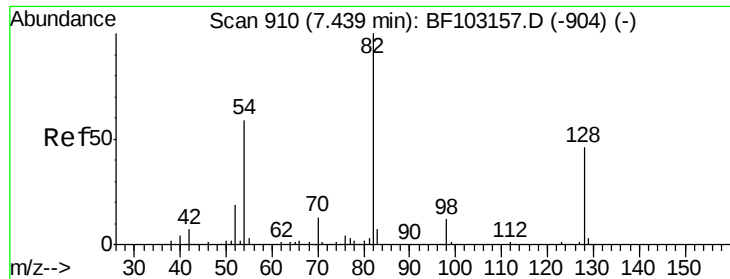

#23
Nitrobenzene-d5
Concen: 95.649 ng
RT: 7.43 min Scan# 909
Delta R.T. -0.01 min
Lab File: BF103535.D
Acq: 8 Mar 2018 23:35




Instrument :
BNA_F
ClientSampleId :
TP-3-B-COMP

Tot Ion: 82 Resp: 819887
Ion Ratio Lower Upper
82 100
128 42.8 36.1 54.1
54 60.3 41.4 62.2

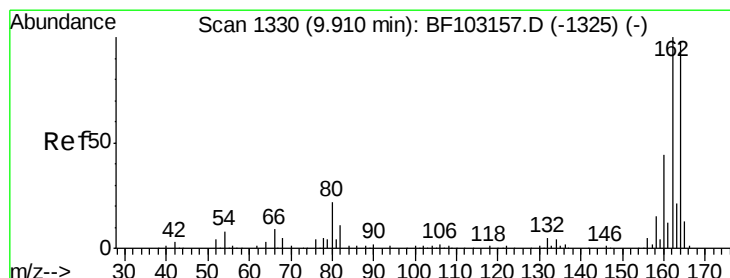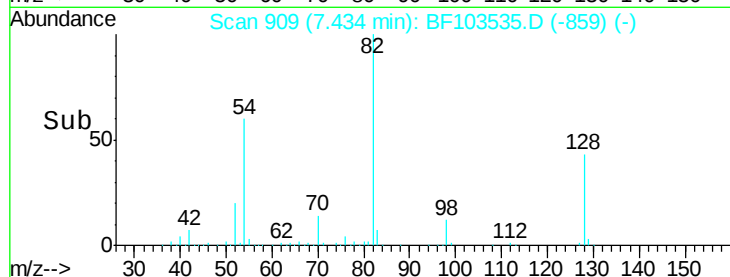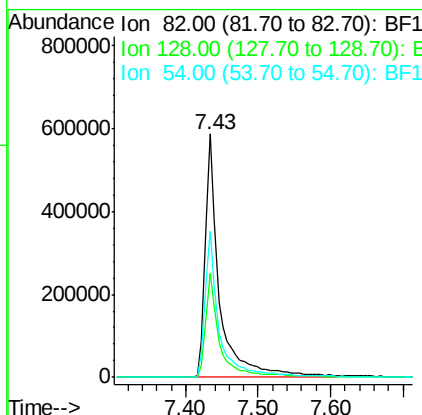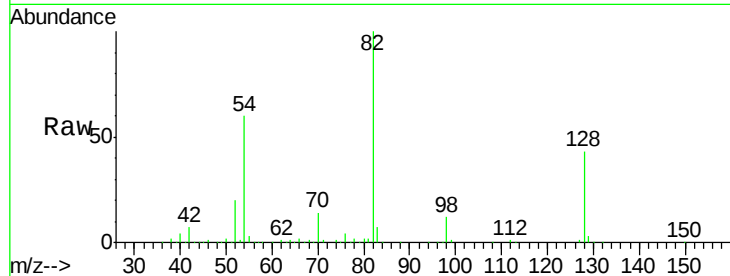

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.91 min Scan# 1330
Delta R.T. 0.00 min
Lab File: BF103535.D
Acq: 8 Mar 2018 23:35

Tgt Ion:164 Resp: 180612
Ion Ratio Lower Upper
164 100
162 100.7 86.1 129.1
160 45.5 38.3 57.5

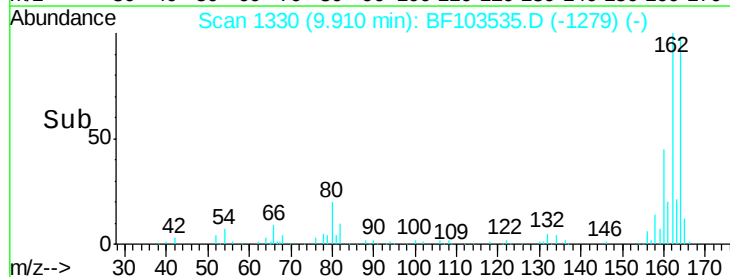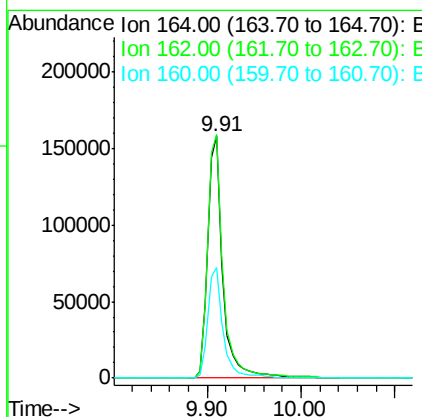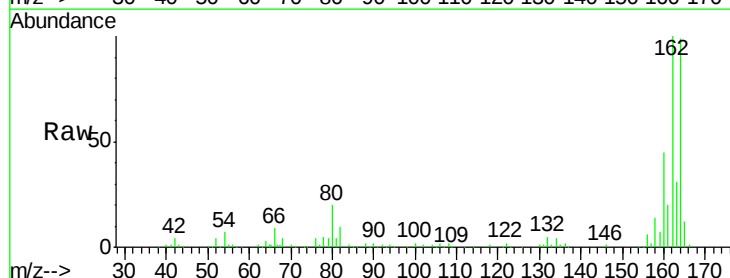







#41
 2,4,6-Tribromophenol
 Concen: 105.589 ng
 RT: 10.70 min Scan# 1465
 Delta R.T. 0.00 min
 Lab File: BF103535.D
 Acq: 8 Mar 2018 23:35

Instrument :
 BNA_F
 ClientSampleId :
 TP-3-B-COMP

Tot Ion:330 Resp: 161423
 Ion Ratio Lower Upper
 330 100
 332 103.1 77.0 115.6
 141 50.8 29.9 44.9#

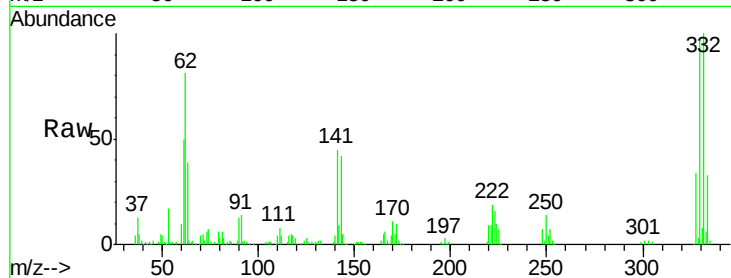


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

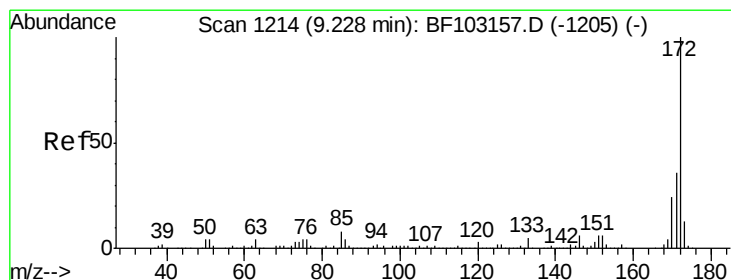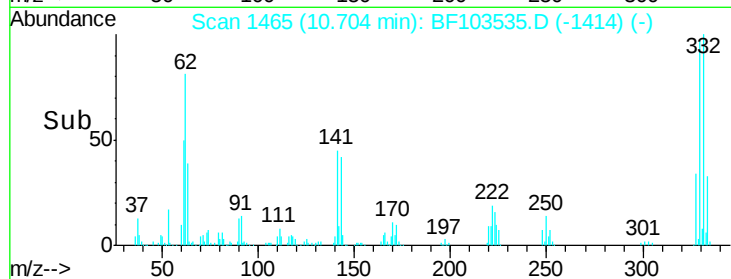
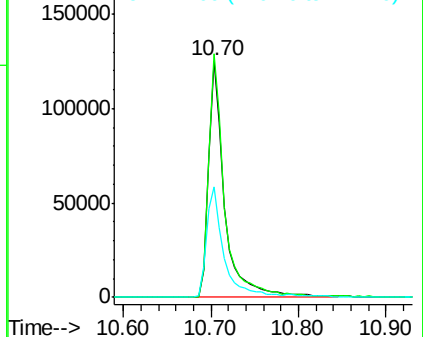



#44
 2-Fluorobiphenyl
 Concen: 104.795 ng
 RT: 9.22 min Scan# 1213
 Delta R.T. 0.00 min
 Lab File: BF103535.D
 Acq: 8 Mar 2018 23:35

Tgt Ion:172 Resp: 1040051
 Ion Ratio Lower Upper
 172 100
 171 35.9 29.7 44.5
 170 24.4 19.6 29.4

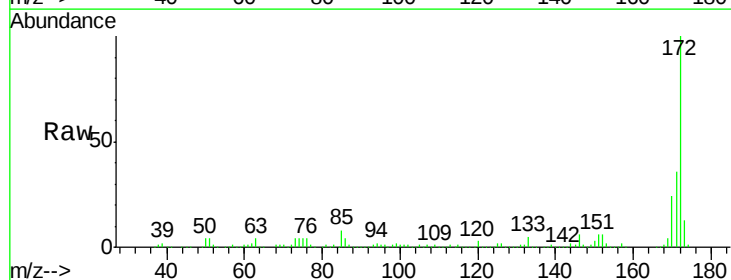

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

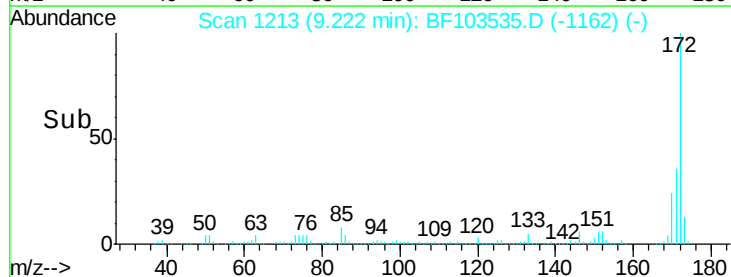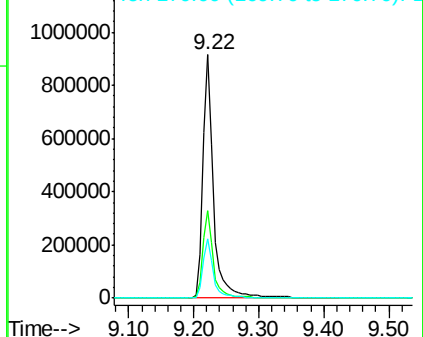


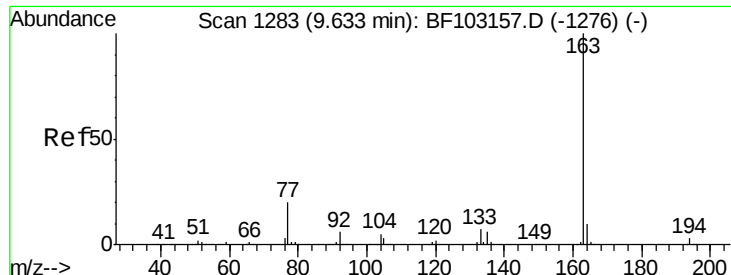




#49
Dimethylphthalate
Concen: 8.489 ng
RT: 9.62 min Scan# 1281
Delta R.T. -0.01 min
Lab File: BF103535.D
Acq: 8 Mar 2018 23:35

Instrument :
BNA_F
ClientSampleId :
TP-3-B-COMP

Tot Ion:163 Resp: 122993
Ion Ratio Lower Upper
163 100
194 3.1 2.7 4.1
164 9.7 8.2 12.2

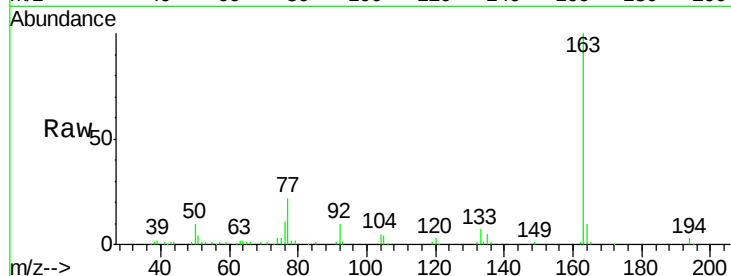


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

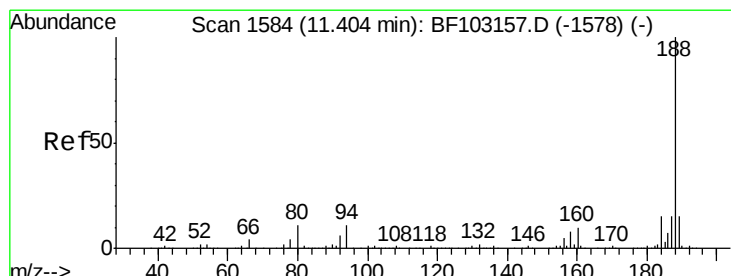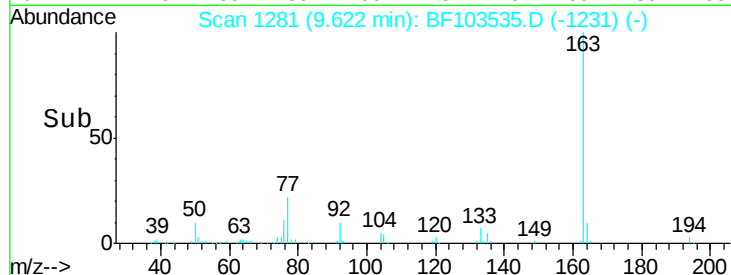
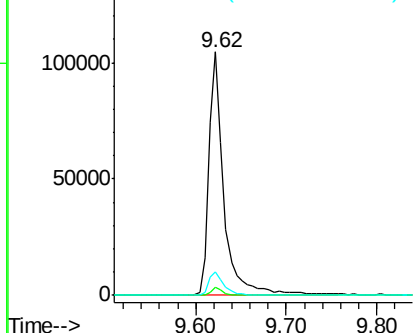



#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.40 min Scan# 1584
Delta R.T. 0.00 min
Lab File: BF103535.D
Acq: 8 Mar 2018 23:35

Tgt Ion:188 Resp: 294435
Ion Ratio Lower Upper
188 100
94 11.9 8.5 12.7
80 12.4 9.2 13.8

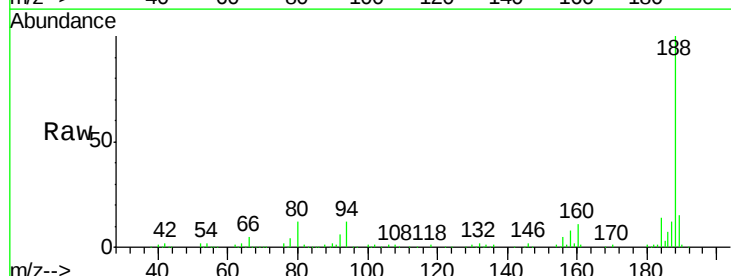

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

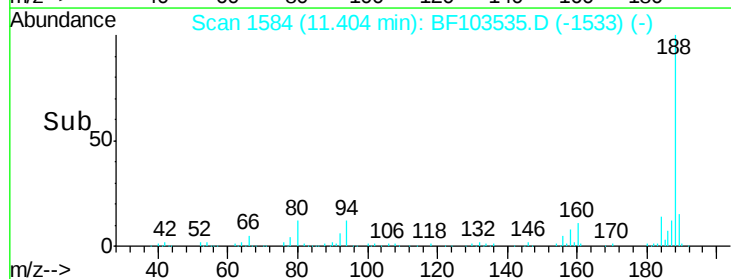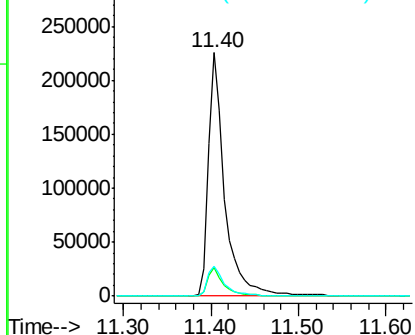

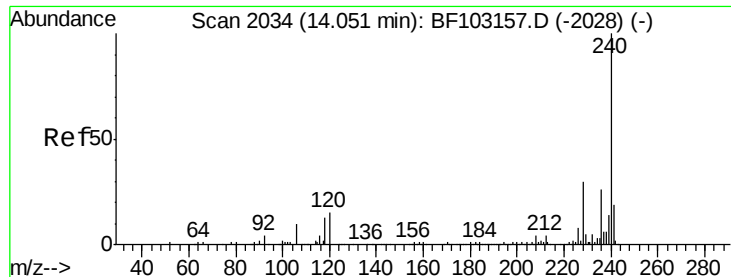

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.06 min Scan# 2035

Delta R.T. -0.01 min

Lab File: BF103535.D

Acq: 8 Mar 2018 23:35

Instrument :

BNA_F

ClientSampleId :

TP-3-B-COMP


Tot Ion:240 Resp: 220820

Ion Ratio Lower Upper

240 100

120 16.5 9.5 14.3#




236 27.6 20.7 31.1

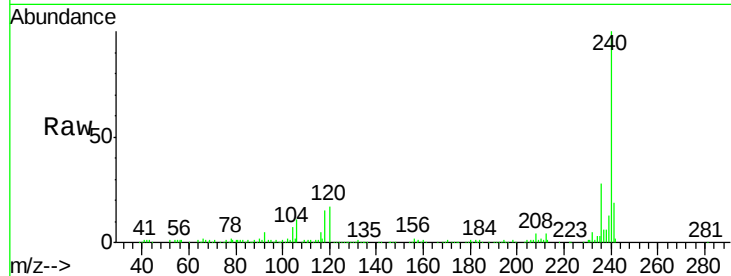

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

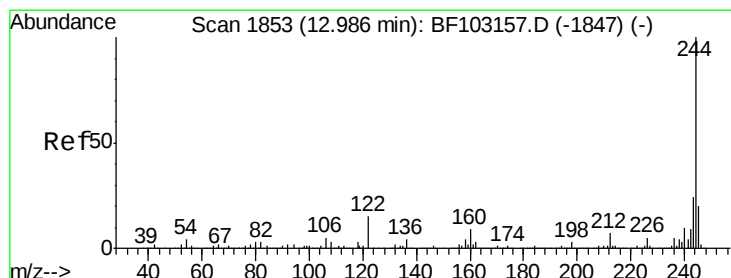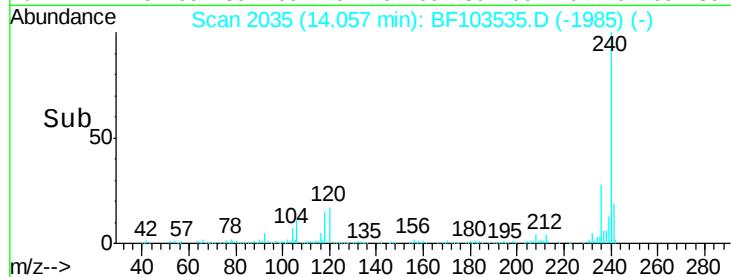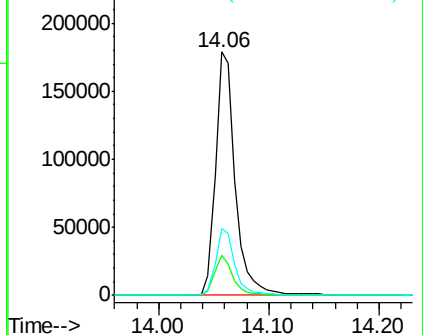

#78

Terphenyl-d14

Concen: 78.772 ng

RT: 12.99 min Scan# 1853

Delta R.T. 0.00 min

Lab File: BF103535.D

Acq: 8 Mar 2018 23:35


Tgt Ion:244 Resp: 723598

Ion Ratio Lower Upper

244 100

212 7.0 5.4 8.0



122 14.2 11.0 16.4

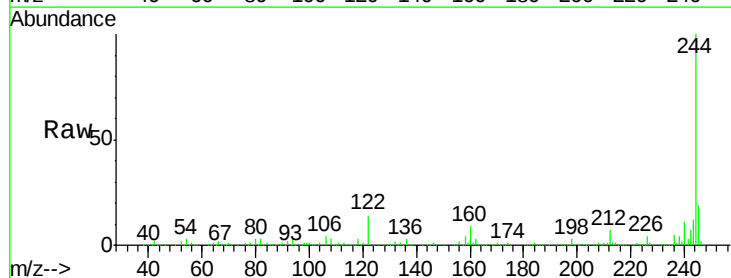


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

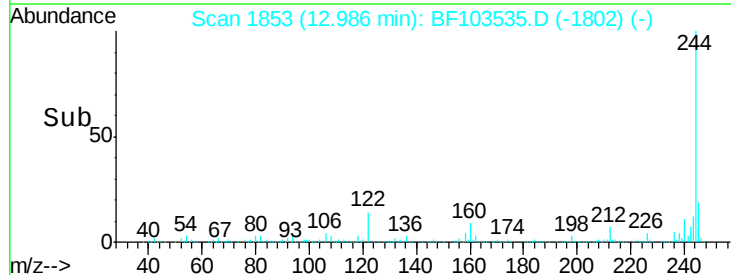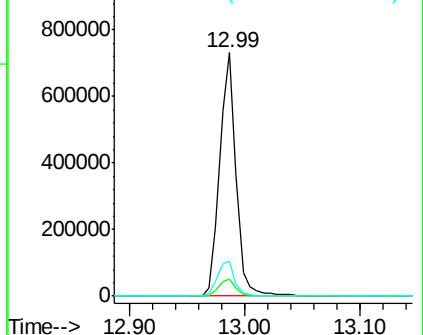


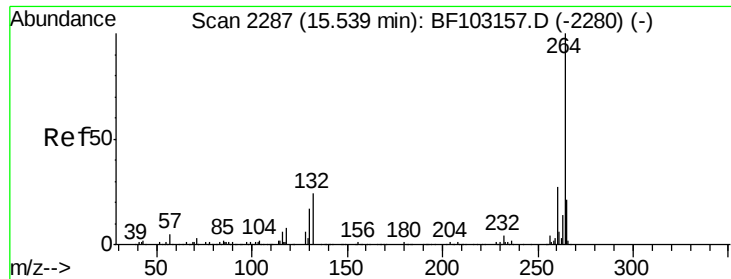

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.57 min Scan# 2292
Delta R.T. 0.00 min
Lab File: BF103535.D
Acq: 8 Mar 2018 23:35

Instrument :
BNA_F
ClientSampleId :
TP-3-B-COMP

Tot Ion	Ratio	Lower	Upper
264	100		
260	25.3	19.2	28.8
265	21.9	17.5	26.3

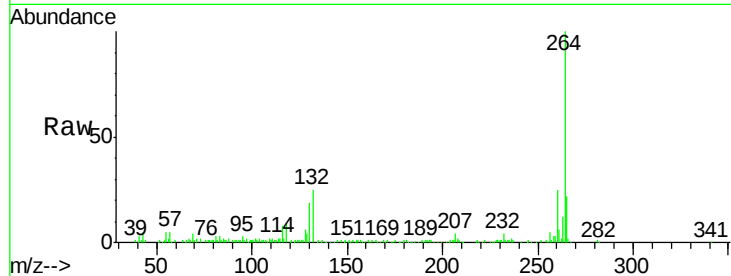

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

