


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF030818\
Data File : BF103511.D
Acq On : 8 Mar 2018 12:39
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 08 14:20:19 2018

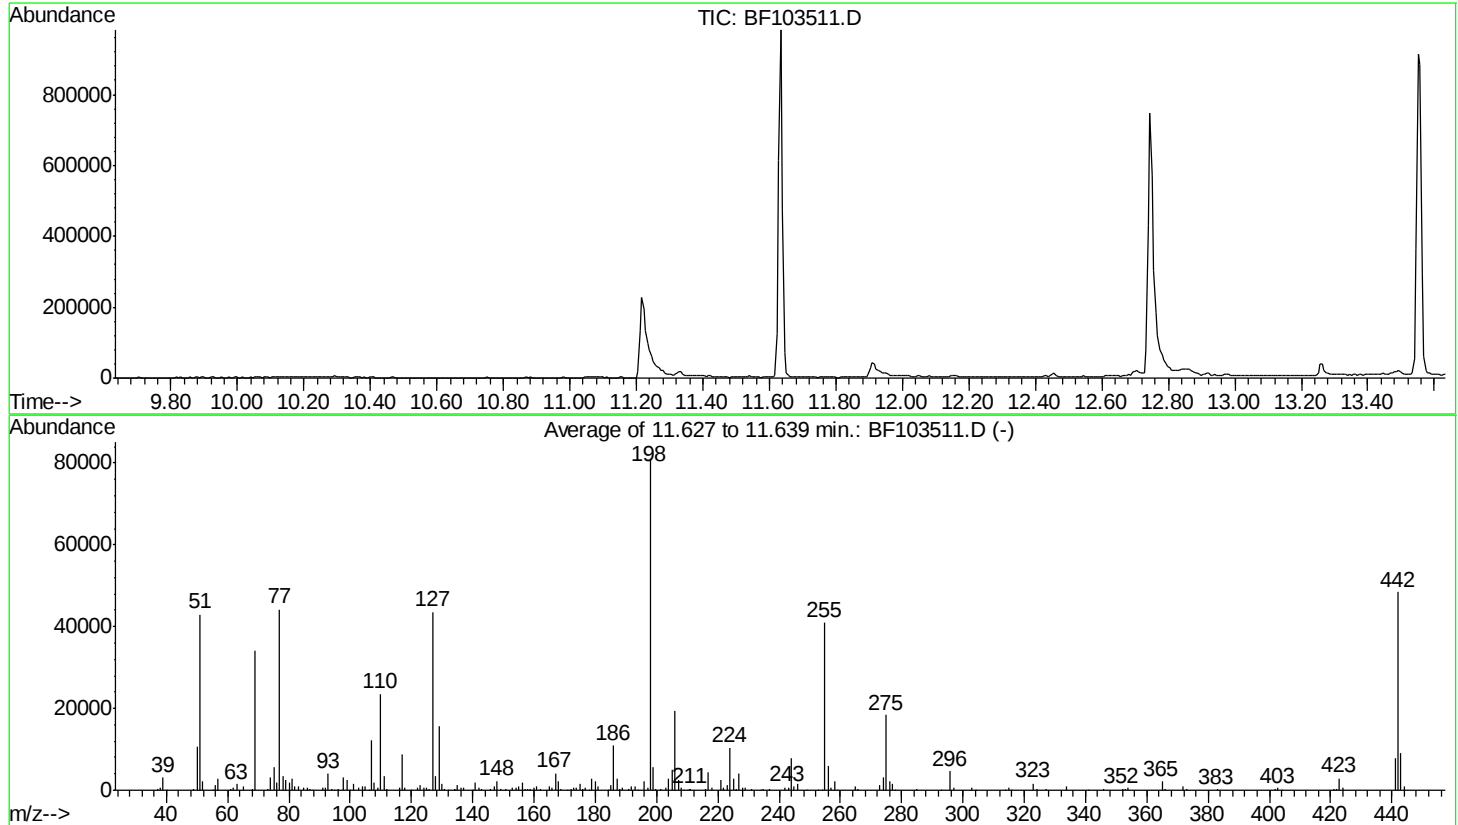

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.0	42925	PASS
68	69	0.00	2	1.3	440	PASS
69	198	0.00	100	42.2	34214	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.7	43536	PASS
197	198	0.00	2	0.8	647	PASS
198	198	100	100	100.0	81064	PASS
199	198	5	9	6.8	5531	PASS
275	198	10	60	22.7	18366	PASS
365	198	1	100	2.5	2051	PASS
441	443	0.01	100	88.7	7940	PASS
442	198	50	100	59.7	48373	PASS
443	442	15	24	18.5	8948	PASS