


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF030818\
 Data File : BF103536.D
 Acq On : 9 Mar 2018 00:54
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 08 14:20:19 2018

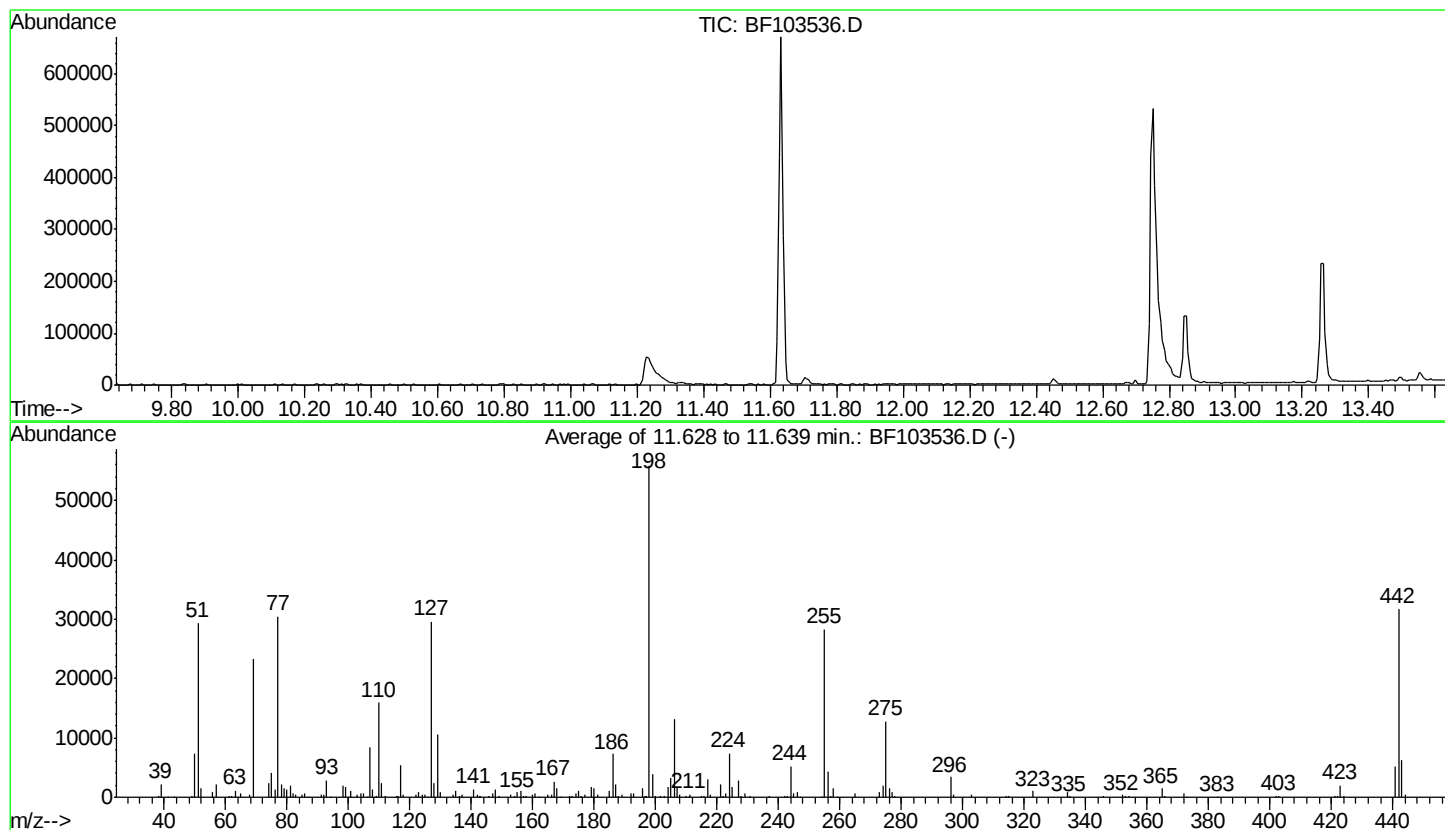

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.6	29426	PASS
68	69	0.00	2	1.9	439	PASS
69	198	0.00	100	41.8	23387	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.0	29613	PASS
197	198	0.00	2	0.4	207	PASS
198	198	100	100	100.0	55896	PASS
199	198	5	9	7.0	3885	PASS
275	198	10	60	22.8	12761	PASS
365	198	1	100	2.6	1438	PASS
441	443	0.01	100	82.9	5254	PASS
442	198	50	100	56.9	31825	PASS
443	442	15	24	19.9	6334	PASS