
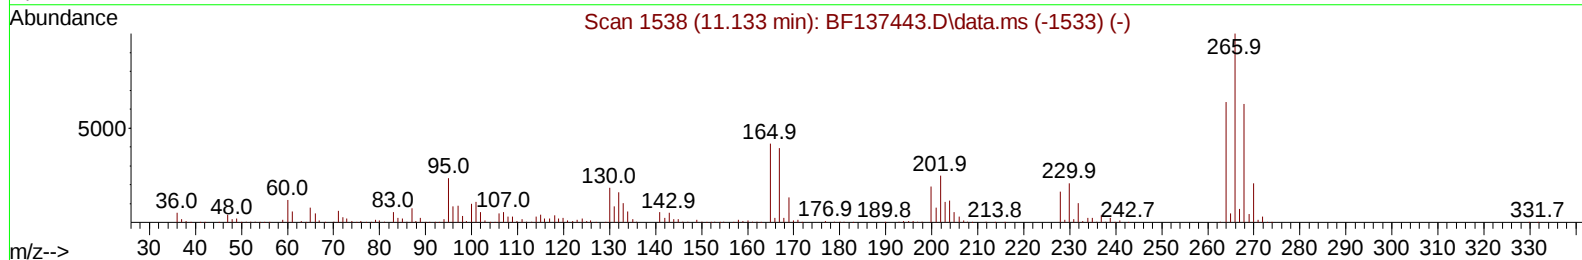
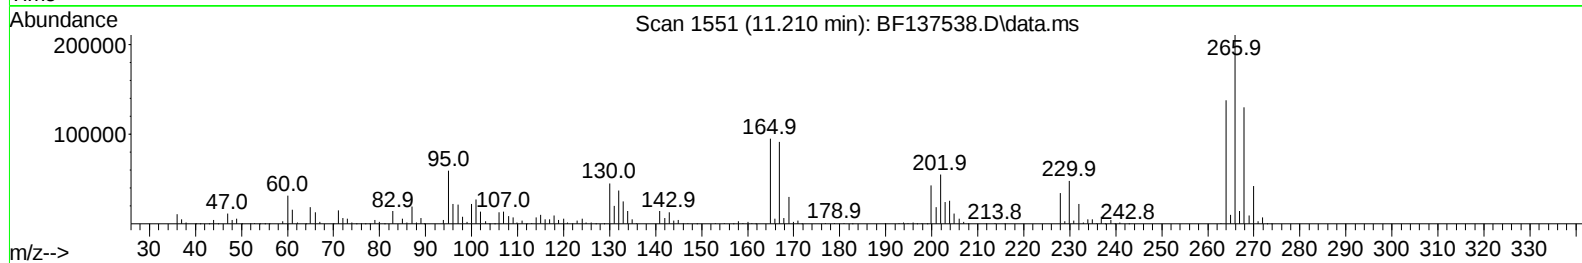


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030824\
Data File : BF137538.D
Acq On : 08 Mar 2024 12:35
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 08 14:33:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 08 00:31:33 2024
Response via : Initial Calibration

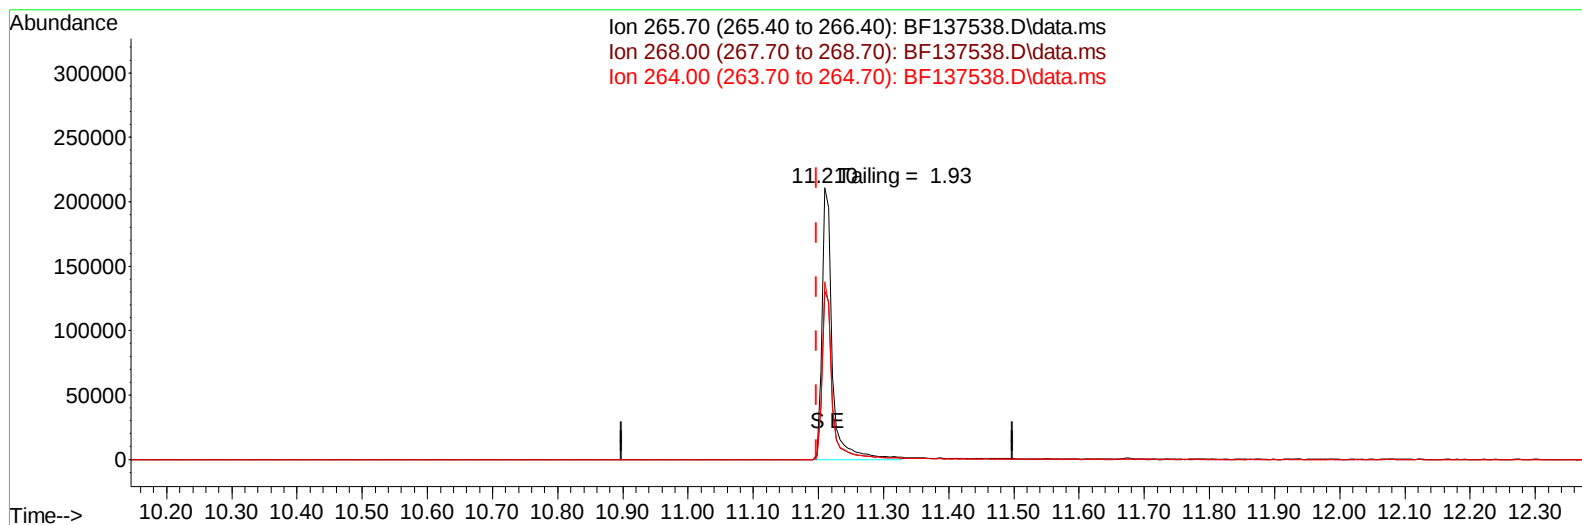

TIC: BF137538.D\data.ms

(70) Pentachlorophenol (C)




11.210min (+ 0.012) 0.00 ng

response 233210

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	61.83
264.00	63.60	65.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030824\
Data File : BF137538.D
Acq On : 08 Mar 2024 12:35
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 08 14:33:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 08 00:31:33 2024
Response via : Initial Calibration

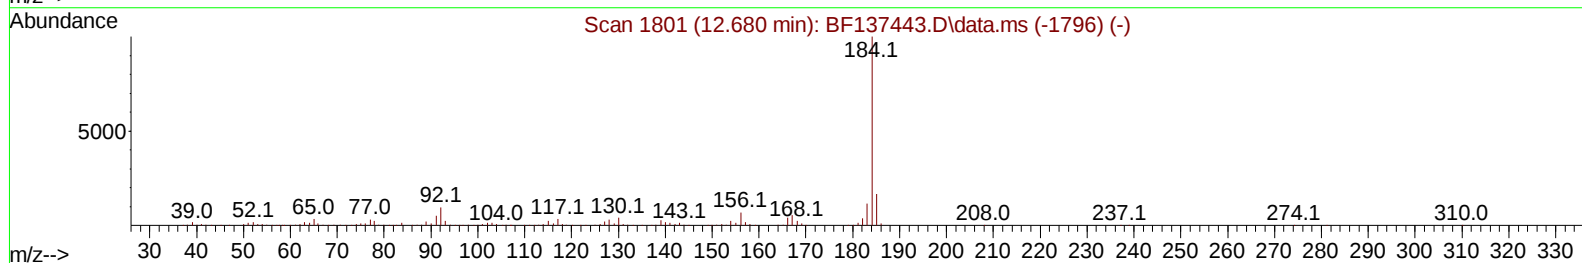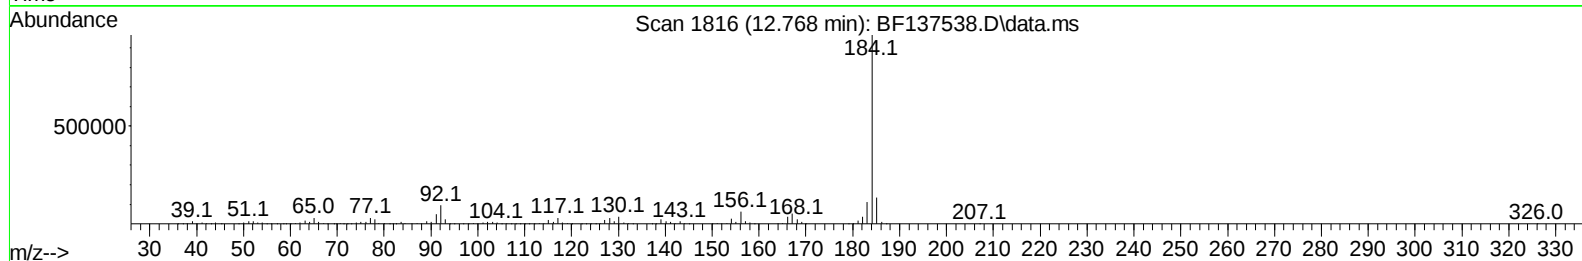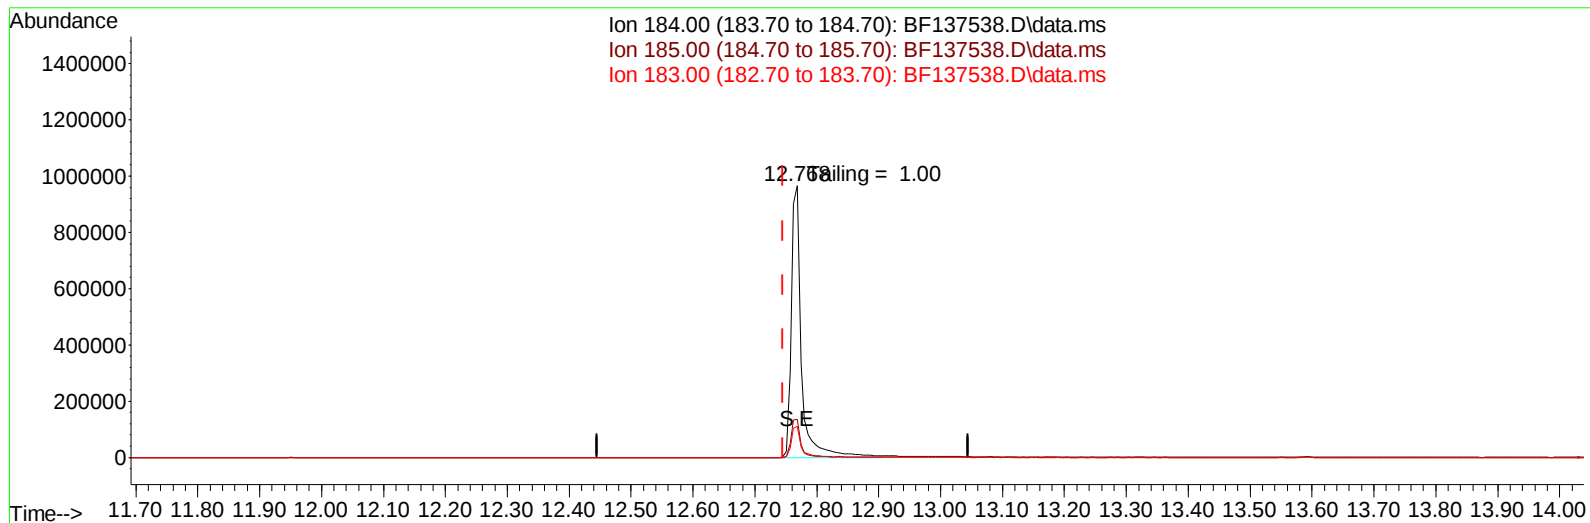

TIC: BF137538.D\data.ms

(77) Benzidine**12.768min (+ 0.024) 873190.65 ng****response 1132554**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.50	14.06
183.00	11.60	11.52
0.00	0.00	0.00