

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030824\
 Data File : BF137540.D
 Acq On : 08 Mar 2024 13:35
 Operator : CG\JU
 Sample : PB159511BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB159511BL

Quant Time: Mar 08 22:15:19 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 08 22:10:14 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.887	152	240702	20.000	ng	0.00
21) Naphthalene-d8	8.157	136	944930	20.000	ng	0.00
39) Acenaphthene-d10	9.916	164	526592	20.000	ng	0.00
64) Phenanthrene-d10	11.410	188	970195	20.000	ng	0.00
76) Chrysene-d12	14.068	240	605851	20.000	ng	0.00
86) Perylene-d12	15.615	264	491195	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.557	112	1815976	114.264	ng	0.01
7) Phenol-d6	6.534	99	2497855	108.883	ng	0.00
23) Nitrobenzene-d5	7.445	82	1556041	76.514	ng	0.00
42) 2,4,6-Tribromophenol	10.710	330	602433	130.273	ng	0.00
45) 2-Fluorobiphenyl	9.239	172	2499159	74.291	ng	0.00
79) Terphenyl-d14	13.016	244	3099564	70.351	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030824\
Data File : BF137540.D
Acq On : 08 Mar 2024 13:35
Operator : CG\JU
Sample : PB159511BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB159511BL


Quant Time: Mar 08 22:15:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 08 22:10:14 2024
Response via : Initial Calibration

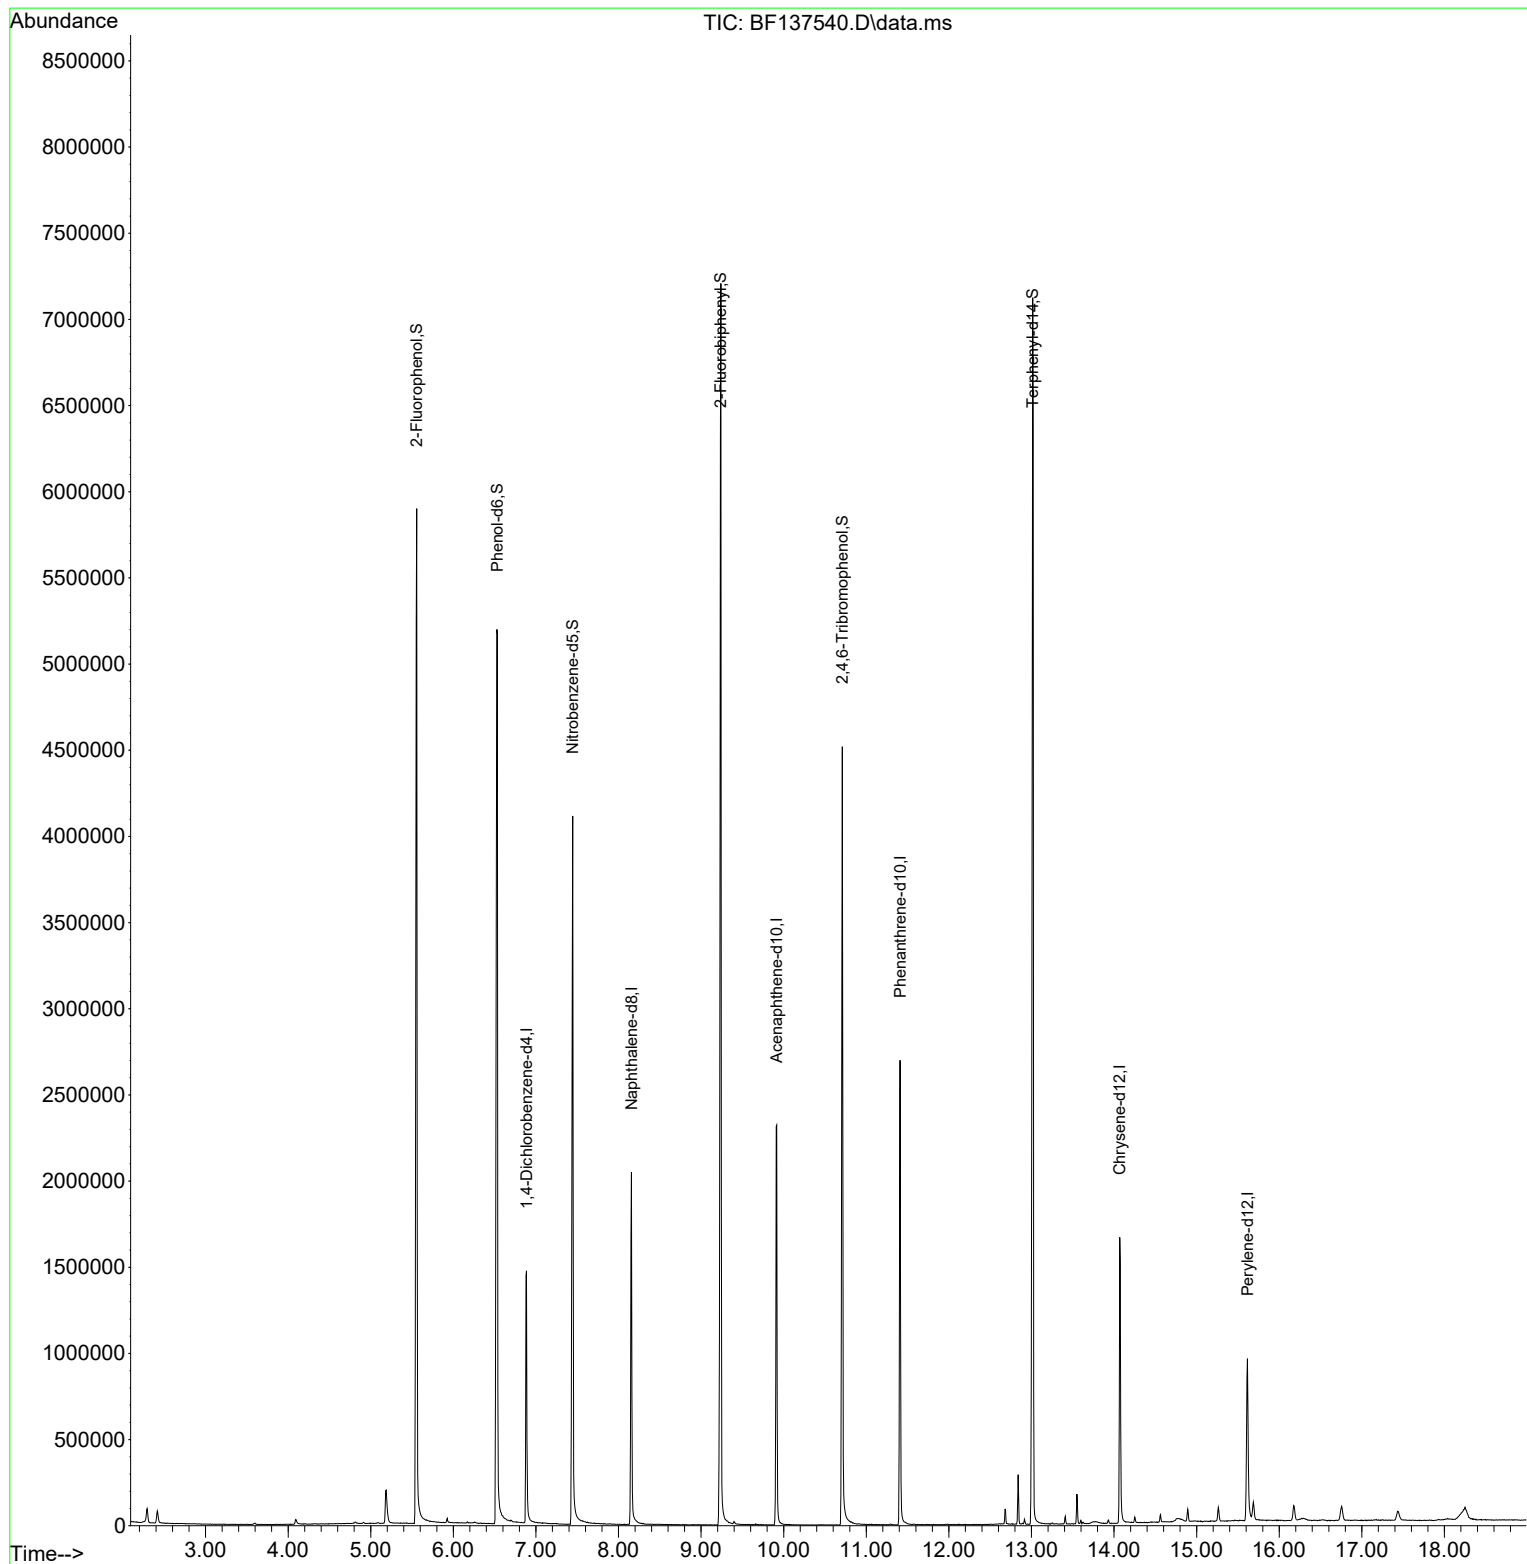






#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.887 min Scan# 816
Delta R.T. -0.000 min
Lab File: BF137540.D
Acq: 08 Mar 2024 13:35

Instrument :
BNA_F
ClientSampleId :
PB159511BL



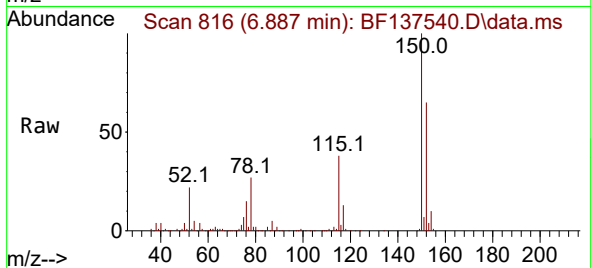



Tgt Ion:152 Resp: 240702
Ion Ratio Lower Upper
152 100
150 154.0 125.8 188.6
115 58.5 48.8 73.2

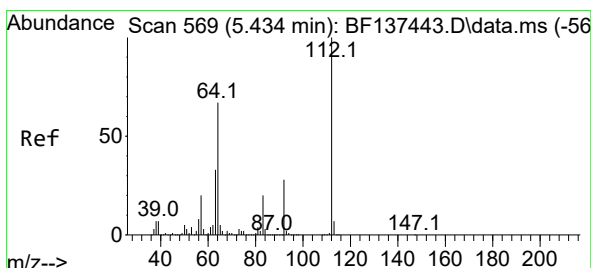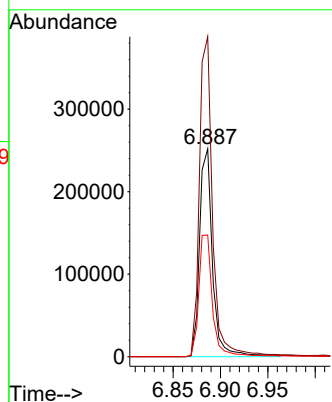

#5
2-Fluorophenol
Concen: 114.264 ng
RT: 5.557 min Scan# 590
Delta R.T. 0.012 min
Lab File: BF137540.D
Acq: 08 Mar 2024 13:35

Tgt Ion:112 Resp: 1815976
Ion Ratio Lower Upper
112 100
64 64.6 53.4 80.2
63 31.6 26.2 39.2


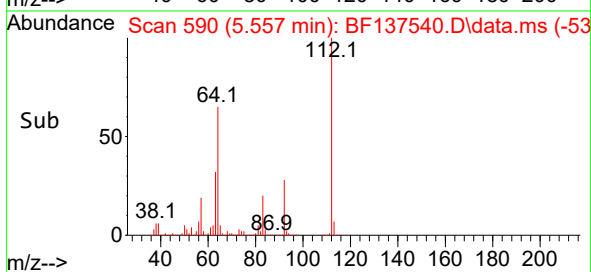
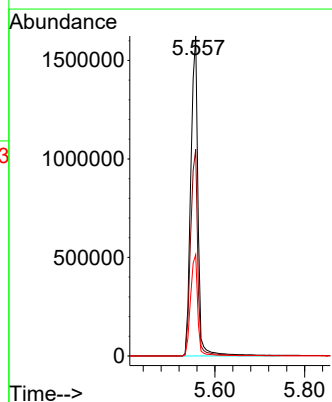





#7
Phenol-d6
Concen: 108.883 ng
RT: 6.534 min Scan# 71
Delta R.T. 0.000 min
Lab File: BF137540.D
Acq: 08 Mar 2024 13:35




Instrument :
BNA_F
ClientSampleId :
PB159511BL


Tgt Ion: 99 Resp: 2497855
Ion Ratio Lower Upper
99 100
42 17.4 14.6 21.8
71 31.7 25.3 37.9

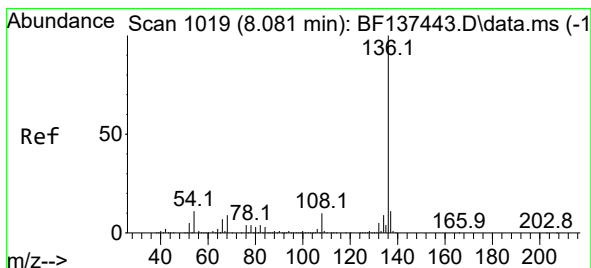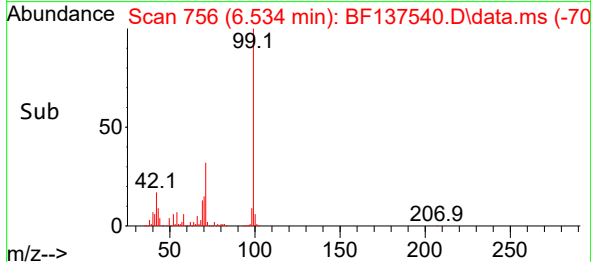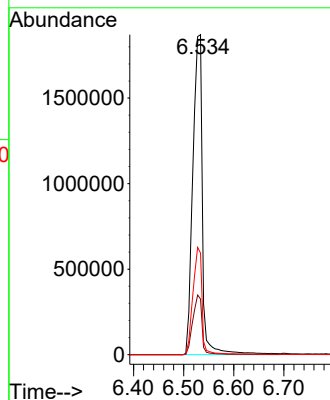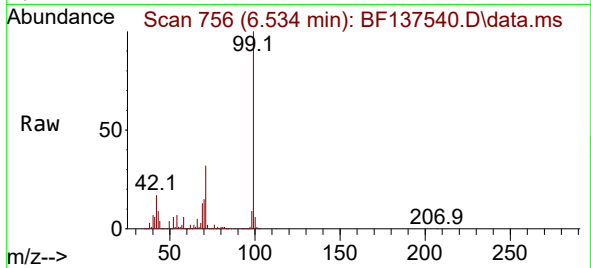

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.157 min Scan# 1032
Delta R.T. 0.000 min
Lab File: BF137540.D
Acq: 08 Mar 2024 13:35

Tgt Ion: 136 Resp: 944930
Ion Ratio Lower Upper
136 100
137 10.8 9.1 13.7
54 9.5 8.5 12.7
68 8.6 7.4 11.2

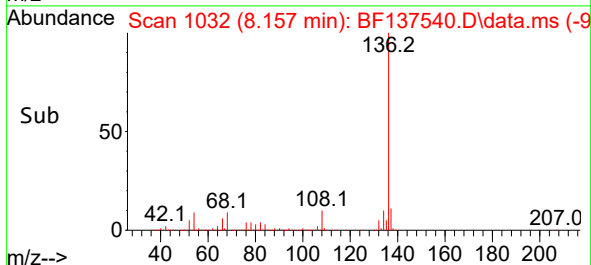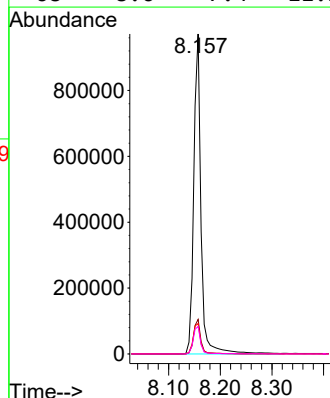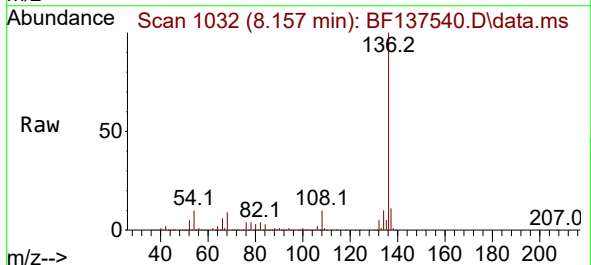



#23

Nitrobenzene-d5

Concen: 76.514 ng

RT: 7.445 min Scan# 911

Delta R.T. -0.006 min

Lab File: BF137540.D

Acq: 08 Mar 2024 13:35

Instrument :

BNA_F

ClientSampleId :

PB159511BL





Tgt Ion: 82 Resp: 1556041

Ion Ratio Lower Upper

82 100

128 41.8 32.5 48.7

54 51.0 41.5 62.3

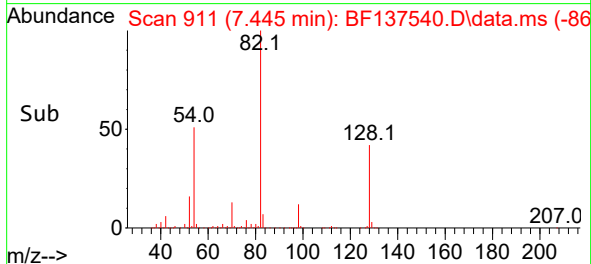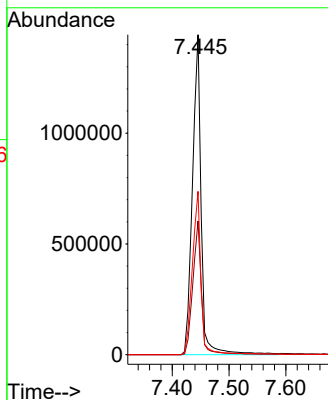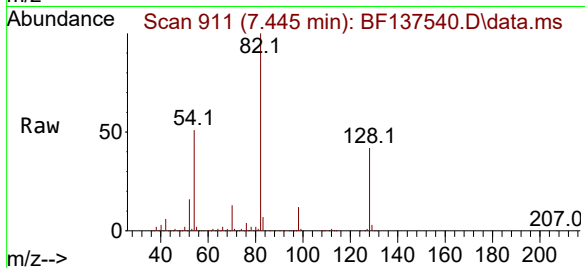

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.916 min Scan# 1331

Delta R.T. 0.000 min

Lab File: BF137540.D

Acq: 08 Mar 2024 13:35




Tgt Ion:164 Resp: 526592


Ion Ratio Lower Upper

164 100

162 101.5 79.8 119.8

160 44.3 34.4 51.6


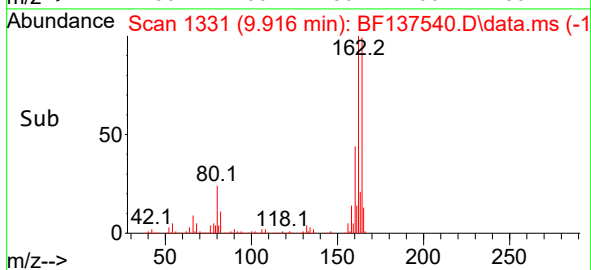
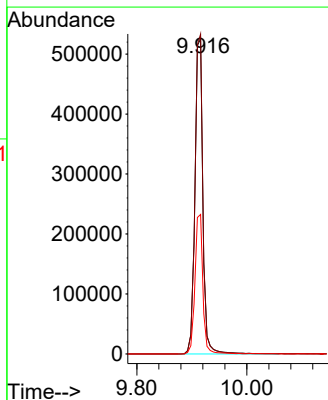
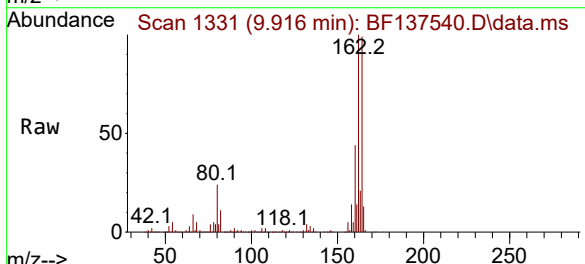




#42
2,4,6-Tribromophenol
Concen: 130.273 ng
RT: 10.710 min Scan# 1453
Delta R.T. -0.006 min
Lab File: BF137540.D
Acq: 08 Mar 2024 13:35




Instrument :
BNA_F
ClientSampleId :
PB159511BL


Tgt Ion:330 Resp: 602433
Ion Ratio Lower Upper
330 100
332 95.2 78.0 117.0
141 28.5 27.3 40.9

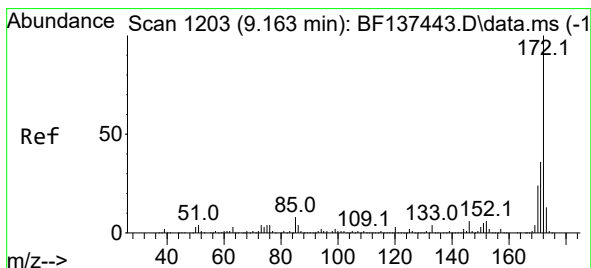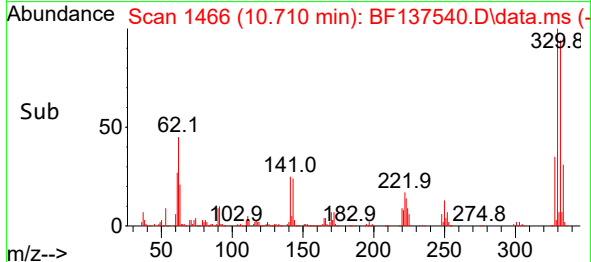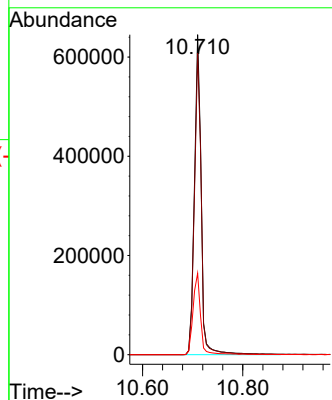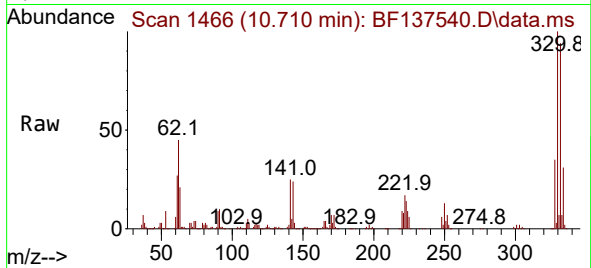

#45
2-Fluorobiphenyl
Concen: 74.291 ng
RT: 9.239 min Scan# 1216
Delta R.T. 0.000 min
Lab File: BF137540.D
Acq: 08 Mar 2024 13:35

Tgt Ion:172 Resp: 2499159
Ion Ratio Lower Upper
172 100
171 36.6 28.5 42.7
170 24.2 19.0 28.6

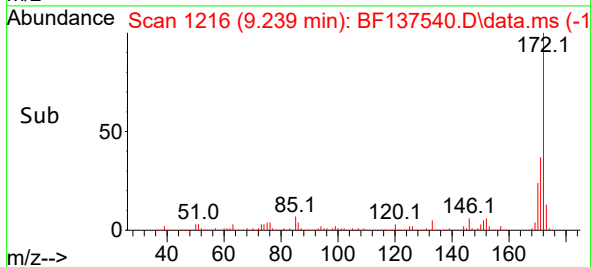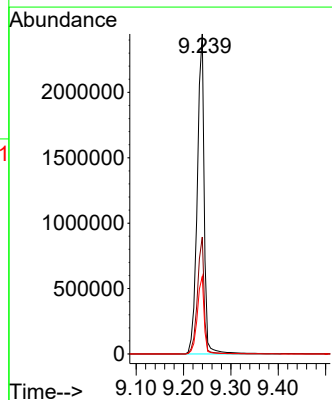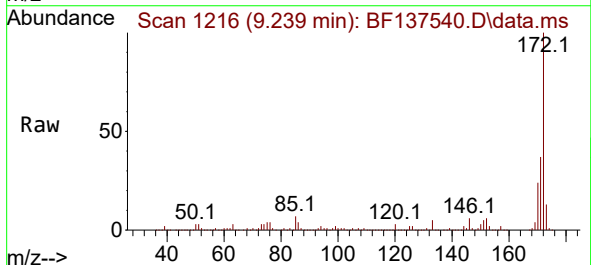

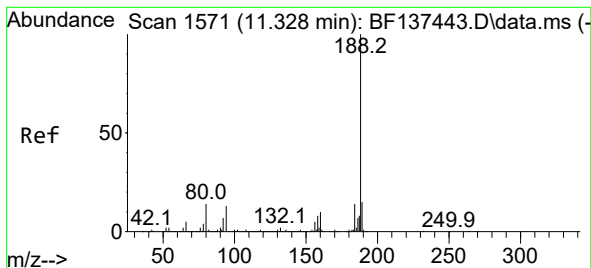

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.410 min Scan# 11

Delta R.T. 0.000 min

Lab File: BF137540.D

Acq: 08 Mar 2024 13:35

Instrument :

BNA_F

ClientSampleId :

PB159511BL





Tgt Ion:188 Resp: 970195

Ion Ratio Lower Upper

188 100

94 12.8 10.6 15.8

80 13.3 11.5 17.3

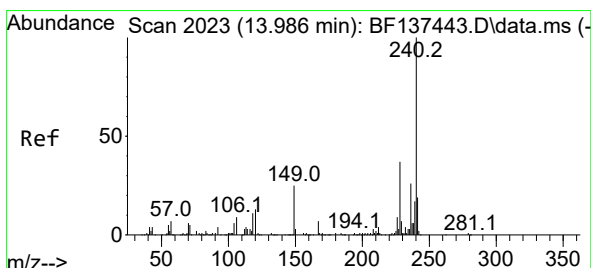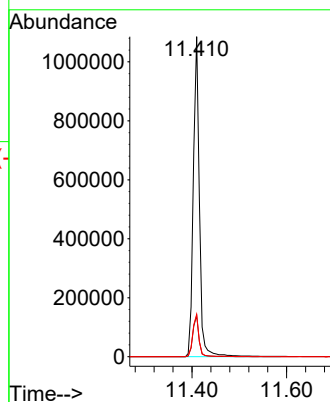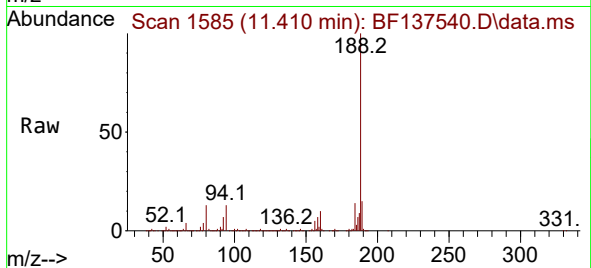

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.068 min Scan# 2037

Delta R.T. -0.006 min

Lab File: BF137540.D

Acq: 08 Mar 2024 13:35




Tgt Ion:240 Resp: 605851


Ion Ratio Lower Upper

240 100

120 14.6 10.4 15.6


236 26.6 20.9 31.3

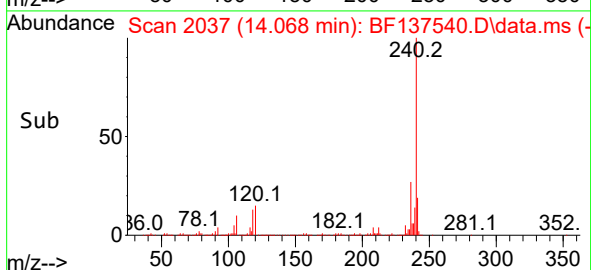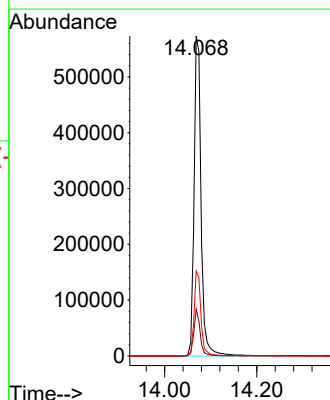






#79
Terphenyl-d14
Concen: 70.351 ng
RT: 13.016 min Scan# 11
Delta R.T. 0.000 min
Lab File: BF137540.D
Acq: 08 Mar 2024 13:35

Instrument :
BNA_F
ClientSampleId :
PB159511BL

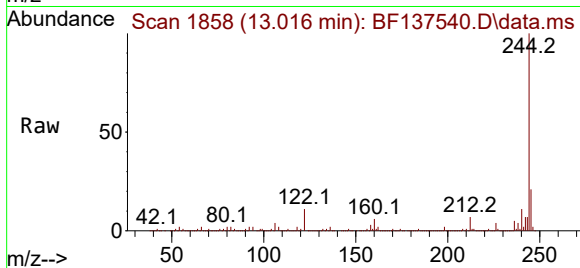

Tgt Ion:244 Resp: 3099564
Ion Ratio Lower Upper
244 100
212 6.8 5.4 8.2
122 10.8 9.1 13.7

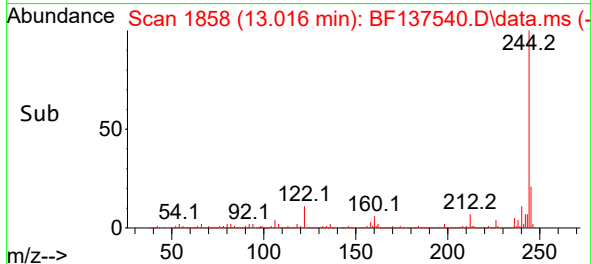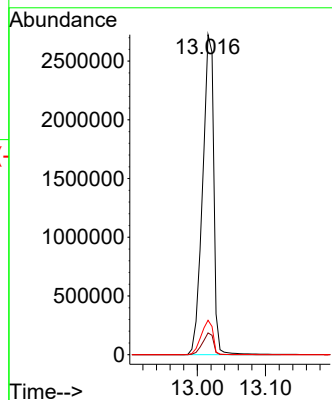

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.615 min Scan# 2300
Delta R.T. 0.000 min
Lab File: BF137540.D
Acq: 08 Mar 2024 13:35

Tgt Ion:264 Resp: 491195
Ion Ratio Lower Upper
264 100
260 23.9 19.3 28.9
265 21.5 17.4 26.0

