


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030824\
Data File : BF137538.D
Acq On : 08 Mar 2024 12:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Mar 08 22:10:14 2024

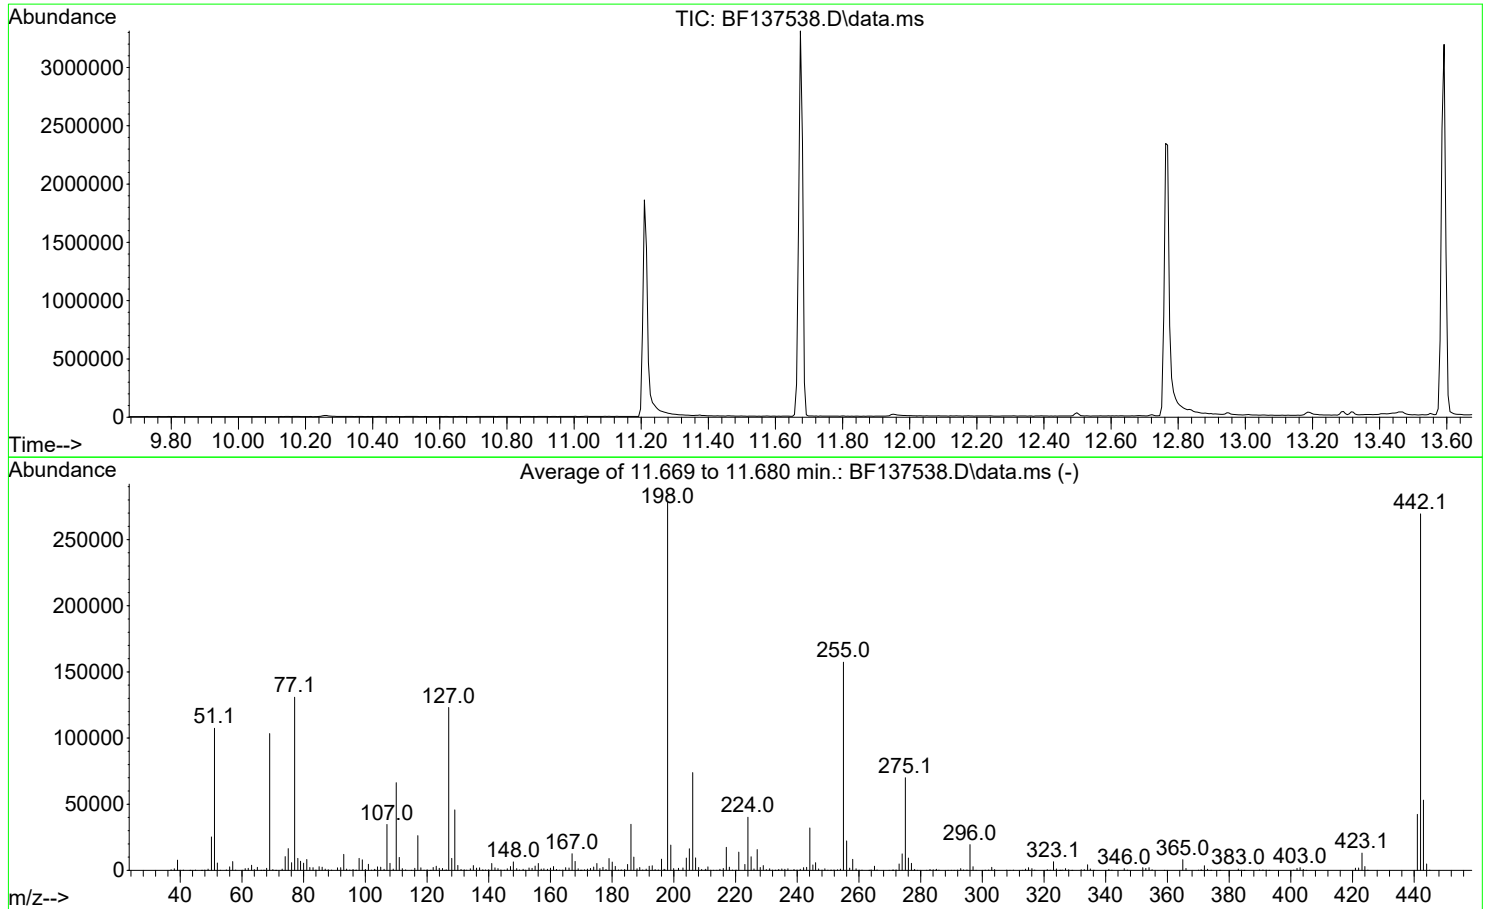

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	107376	PASS
68	69	0.00	2	1.5	1562	PASS
69	198	0.00	100	37.2	103384	PASS
70	69	0.00	2	0.5	564	PASS
127	198	10	80	44.3	123139	PASS
197	198	0.00	2	0.3	903	PASS
198	198	100	100	100.0	278037	PASS
199	198	5	9	6.9	19070	PASS
275	198	10	60	25.2	69989	PASS
365	198	1	100	2.9	8115	PASS
441	198	0.01	100	15.2	42363	PASS
442	442	50	100	100.0	269485	PASS
443	442	15	24	19.7	53141	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/8/2024	BNA_F	<u>BF137538.D</u>
Compound Name	Response	Retention Time
DDT	552469	13.592
DDD	10588	13.292
DDE	2469	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13057	565526	2.31

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030824\
Data File : BF137538.D
Acq On : 08 Mar 2024 12:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 08 14:33:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 08 00:31:33 2024
Response via : Initial Calibration

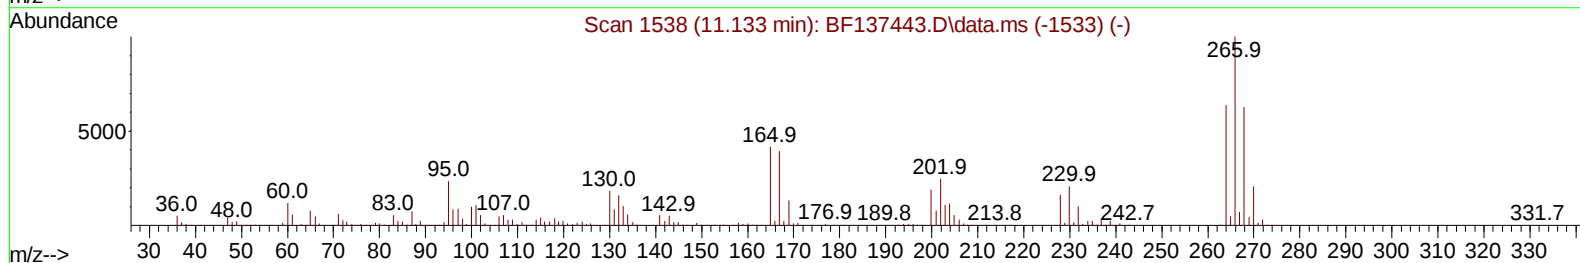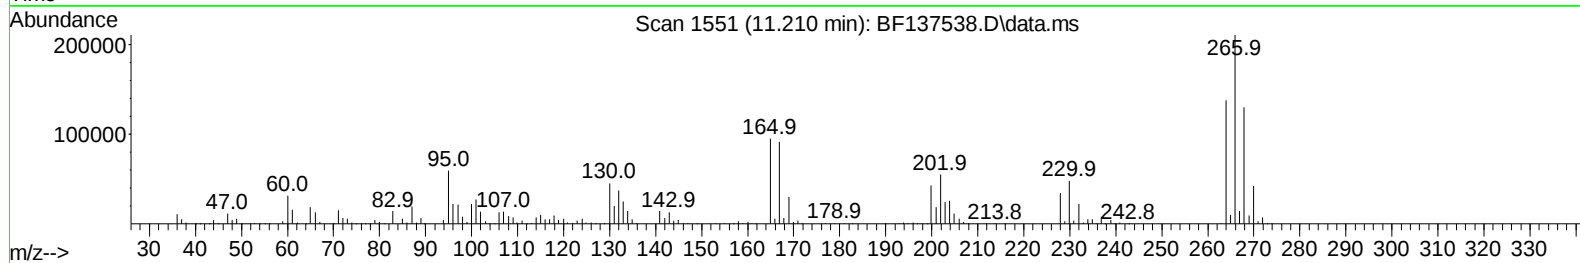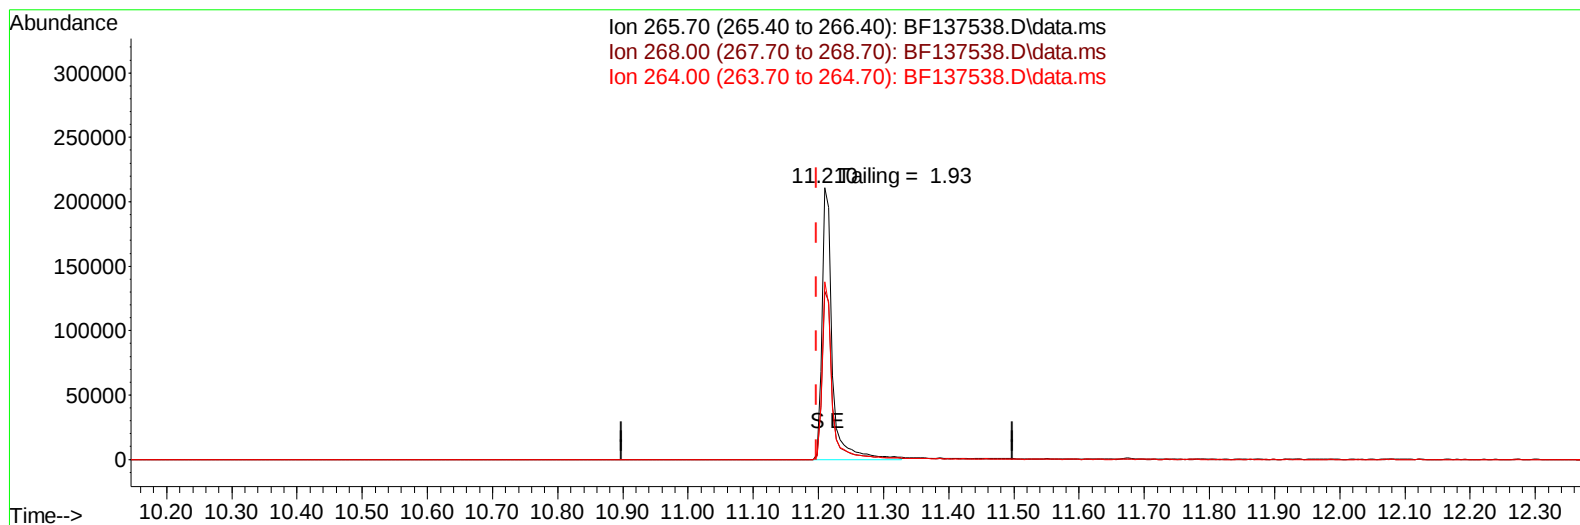

TIC: BF137538.D\data.ms

(70) Pentachlorophenol (C)

11.210min (+ 0.012) 0.00 ng




response 233210

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	61.83
264.00	63.60	65.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030824\
Data File : BF137538.D
Acq On : 08 Mar 2024 12:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 08 14:33:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 08 00:31:33 2024
Response via : Initial Calibration

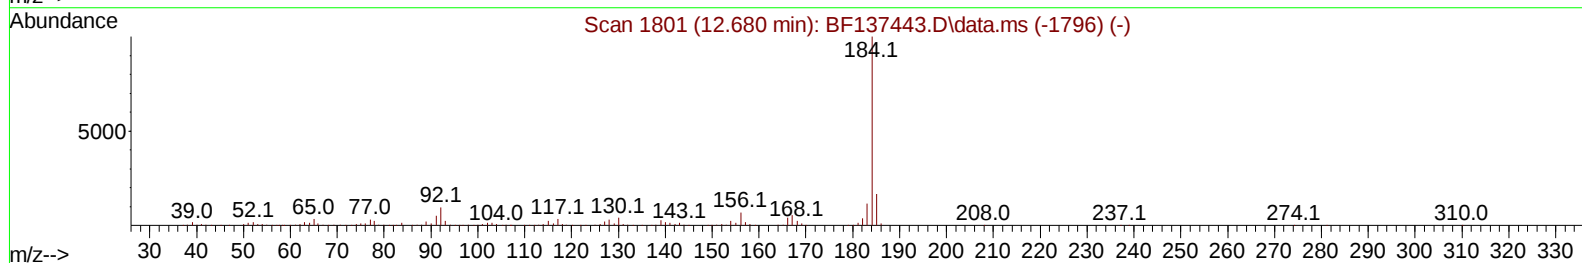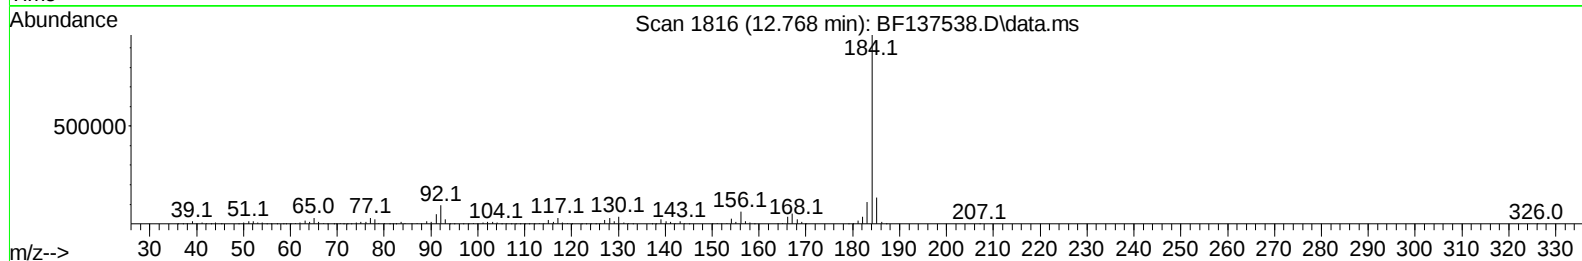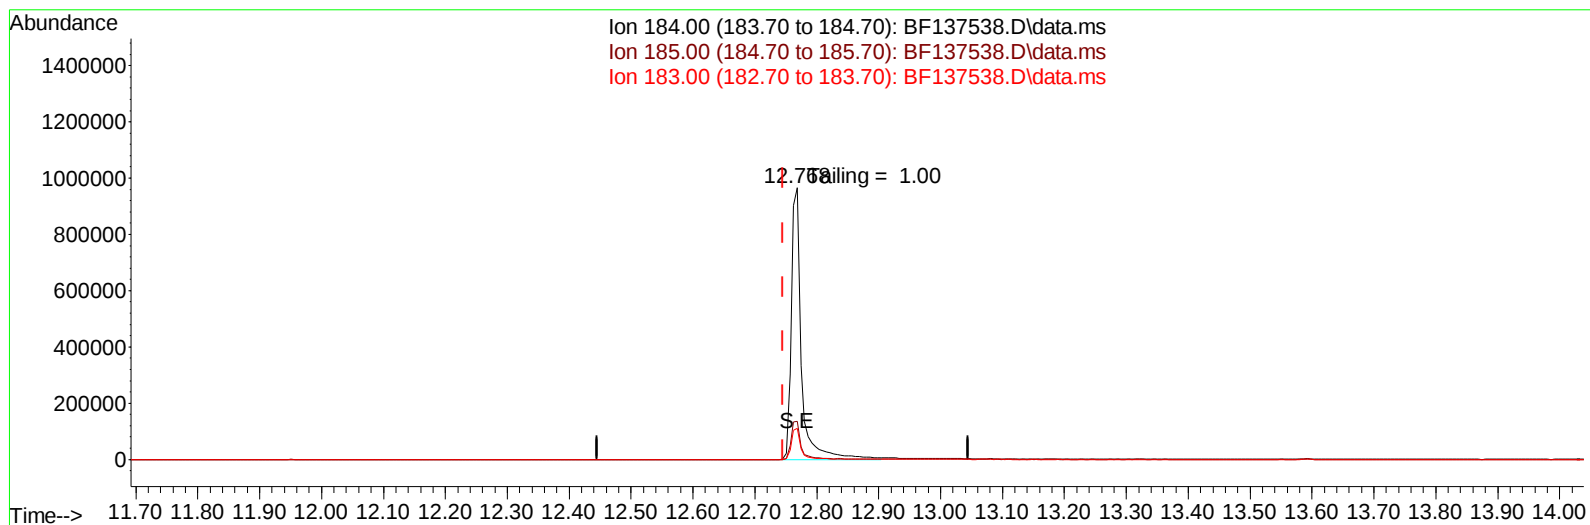

TIC: BF137538.D\data.ms

(77) Benzidine

12.768min (+ 0.024) 873190.65 ng

response 1132554

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.50	14.06
183.00	11.60	11.52
0.00	0.00	0.00