


Data Path : Z:\HPCHEM1\BNA_F\Data\BF030915\
 Data File : BF077637.D
 Acq On : 9 Mar 2015 10:02
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 04 13:27:09 2015

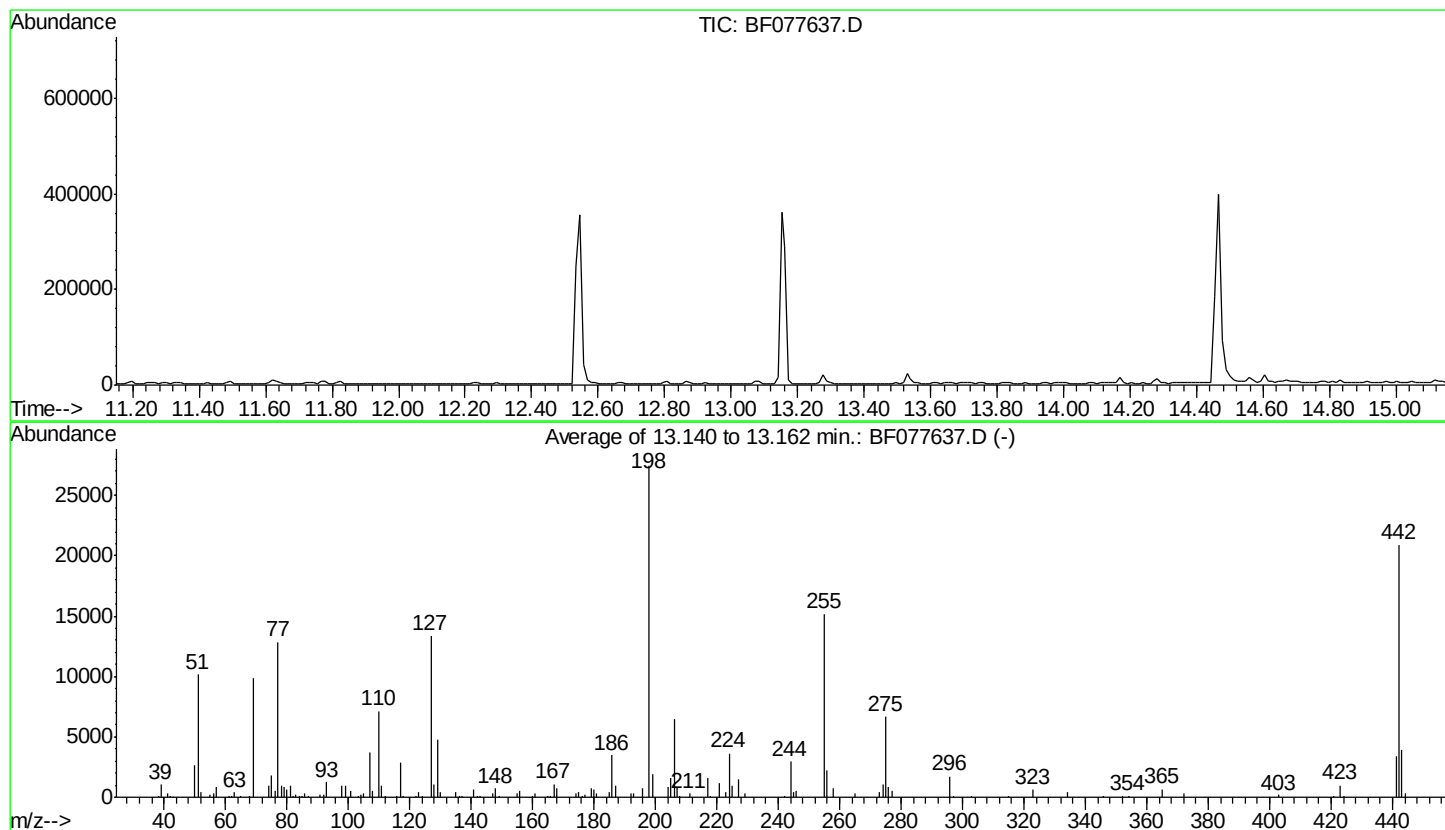

AutoFind: Scans 1072, 1073, 1074; Background Corrected with Scan 1069

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	10132	PASS
68	69	0.00	2	1.3	132	PASS
69	198	0.00	100	36.0	9888	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.7	13384	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	27471	PASS
199	198	5	9	6.9	1886	PASS
275	198	10	60	24.2	6638	PASS
365	198	1	100	2.5	689	PASS
441	442	0.01	24	16.4	3430	PASS
442	198	50	100	76.2	20939	PASS
443	442	15	24	18.7	3906	PASS