

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030915\
 Data File : BF077639.D
 Acq On : 9 Mar 2015 15:42
 Operator : TP/IZ
 Sample : G1442-01DL 5X
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DCW-WW-073-3515DL

Quant Time: Mar 10 01:11:32 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF021915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 10 00:35:08 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.19	152	14382	20.00	ng	0.00
21) Naphthalene-d8	8.77	136	56956	20.00	ng	0.00
38) Acenaphthene-d10	10.94	164	28222	20.00	ng	0.00
63) Phenanthrene-d10	12.78	188	53463	20.00	ng	0.00
75) Chrysene-d12	16.05	240	57067	20.00	ng	0.00
86) Perylene-d12	17.75	264	55839	20.00	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.48	112	45338	52.63	ng	0.00
7) Phenol-d6	6.75	99	35193	31.77	ng	0.00
23) Nitrobenzene-d5	7.88	82	84396	92.14	ng	0.00
41) 2,4,6-Tribromophenol	11.92	330	33205	122.19	ng	0.00
44) 2-Fluorobiphenyl	10.11	172	180370	99.65	ng	0.00
78) Terphenyl-d14	14.77	244	181852	74.50	ng	0.00
Target Compounds						Qvalue
13) 1,4-Dichlorobenzene	7.21	146	8799	7.82	ng	97
14) 1,2-Dichlorobenzene	7.40	146	152815	142.70	ng	96
30) 1,2,4-Trichlorobenzene	8.70	180	60795	66.67	ng	96
31) Naphthalene	8.80	128	420738	147.72	ng	99
33) 4-Chloroaniline	8.85	127	48601	38.38	ng	97
37) 2-Methylnaphthalene	9.65	142	79424	39.27	ng	98
45) 1,1'-Biphenyl	10.24	154	6346	2.97	ng	93
51) Acenaphthene	10.98	154	16171	10.21	ng	96
54) Dibenzofuran	11.19	168	7762	3.17	ng	# 97
56) 2,4-Dinitrotoluene	11.19	165	4854	9.03	ng	# 59
57) Fluorene	11.62	166	17701	9.05	ng	99
70) Phenanthrene	12.81	178	17360	5.60	ng	98
72) Carbazole	13.08	167	10764	3.68	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030915\
Data File : BF077639.D
Acq On : 9 Mar 2015 15:42
Operator : TP/IZ
Sample : G1442-01DL 5X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DCW-WW-073-3515DL

Quant Time: Mar 10 01:11:32 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF021915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 10 00:35:08 2015
Response via : Initial Calibration

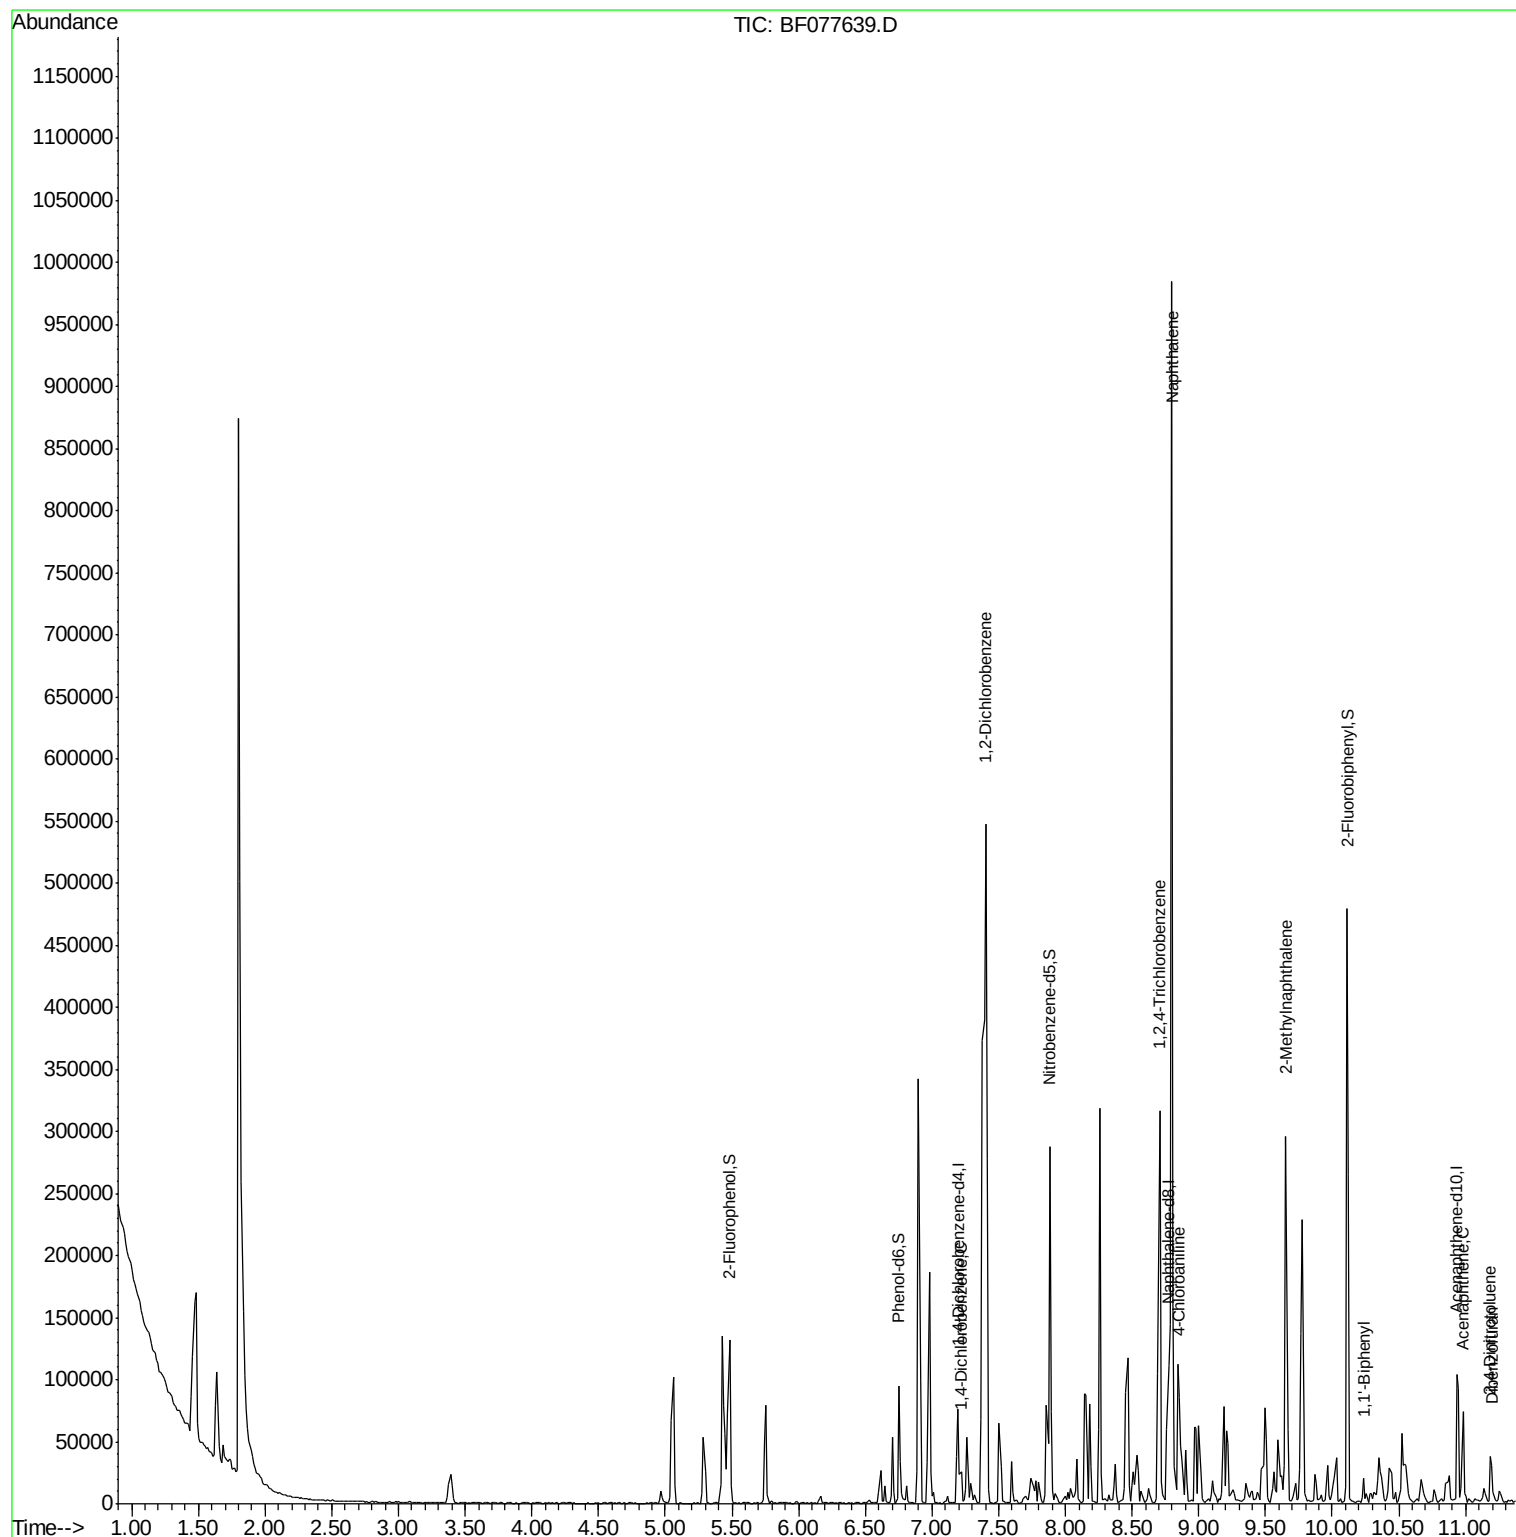

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030915\
Data File : BF077639.D
Acq On : 9 Mar 2015 15:42
Operator : TP/IZ
Sample : G1442-01DL 5X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DCW-WW-073-3515DL

Quant Time: Mar 10 01:11:32 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF021915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 10 00:35:08 2015
Response via : Initial Calibration

