

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030915\
 Data File : BF077640.D
 Acq On : 9 Mar 2015 16:11
 Operator : TP/IZ
 Sample : G1442-04DL 5X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DCW-WW-076-3515DL

Quant Time: Mar 10 01:15:54 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF021915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 10 00:35:08 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.19	152	14184	20.00	ng	0.00
21) Naphthalene-d8	8.77	136	56773	20.00	ng	0.00
38) Acenaphthene-d10	10.94	164	27036	20.00	ng	0.00
63) Phenanthrene-d10	12.78	188	51272	20.00	ng	0.00
75) Chrysene-d12	16.06	240	54688	20.00	ng	0.00
86) Perylene-d12	17.77	264	56518	20.00	ng	0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.48	112	41323	48.64	ng	0.00
7) Phenol-d6	6.75	99	30567	27.98	ng	0.00
23) Nitrobenzene-d5	7.88	82	79485	87.06	ng	0.00
41) 2,4,6-Tribromophenol	11.92	330	31193	119.82	ng	0.00
44) 2-Fluorobiphenyl	10.11	172	168819	97.36	ng	0.00
78) Terphenyl-d14	14.77	244	187444	80.13	ng	0.00
Target Compounds						Qvalue
13) 1,4-Dichlorobenzene	7.21	146	9148	8.24	ng	95
14) 1,2-Dichlorobenzene	7.40	146	165309	156.52	ng	95
30) 1,2,4-Trichlorobenzene	8.70	180	69906	76.90	ng	97
31) Naphthalene	8.80	128	428904	151.07	ng	99
33) 4-Chloroaniline	8.85	127	61023	48.34	ng	98
37) 2-Methylnaphthalene	9.65	142	83059	41.20	ng	98
45) 1,1'-Biphenyl	10.24	154	6225	3.04	ng	97
51) Acenaphthene	10.98	154	17258	11.37	ng	98
54) Dibenzofuran	11.19	168	8958	3.82	ng	96
56) 2,4-Dinitrotoluene	11.19	165	5972	11.60	ng	# 68
57) Fluorene	11.62	166	18678	9.97	ng	97
70) Phenanthrene	12.81	178	15852	5.33	ng	96
71) Anthracene	12.87	178	6146	2.08	ng	97
72) Carbazole	13.08	167	10611	3.78	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030915\
Data File : BF077640.D
Acq On : 9 Mar 2015 16:11
Operator : TP/IZ
Sample : G1442-04DL 5X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DCW-WW-076-3515DL

Quant Time: Mar 10 01:15:54 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF021915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 10 00:35:08 2015
Response via : Initial Calibration

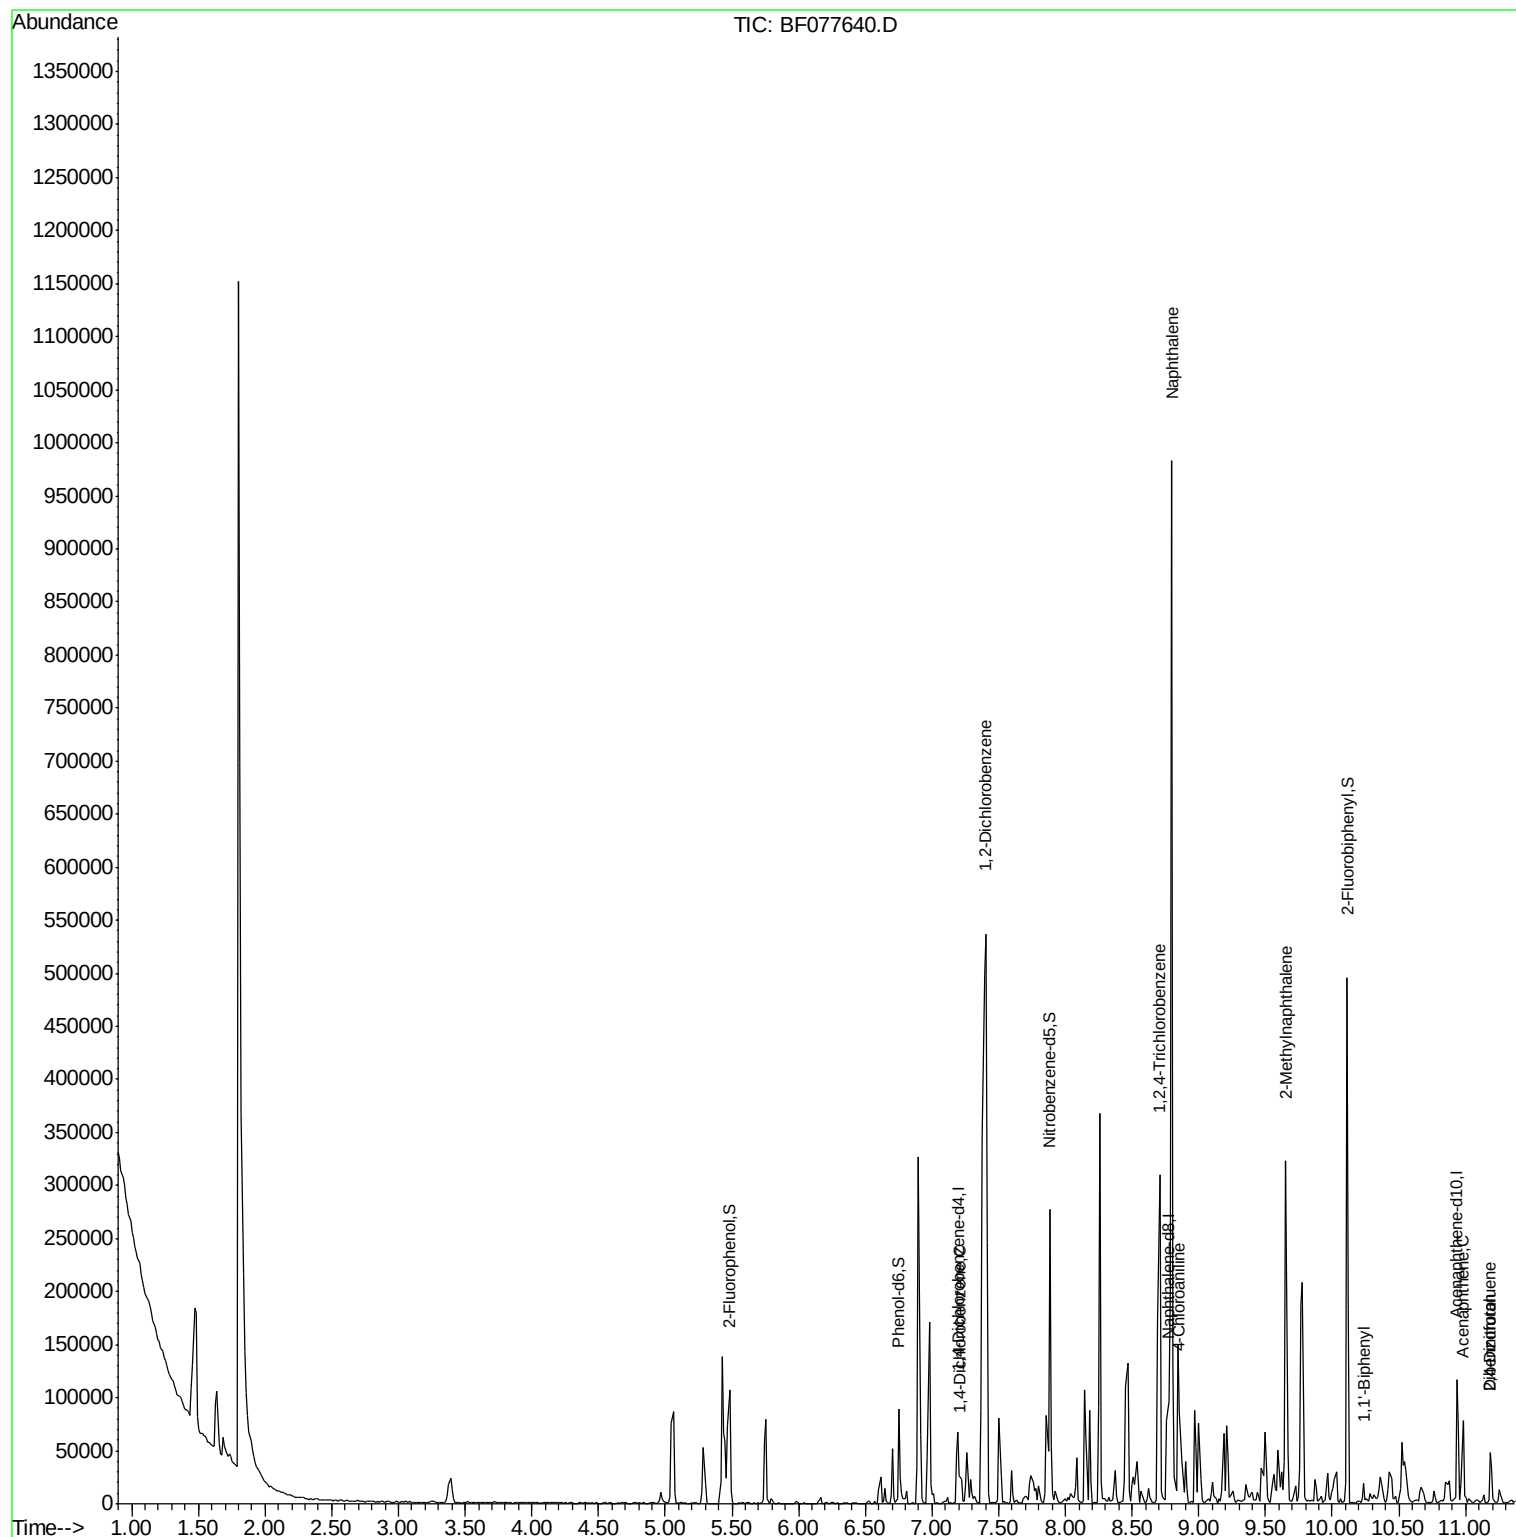

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030915\
Data File : BF077640.D
Acq On : 9 Mar 2015 16:11
Operator : TP/IZ
Sample : G1442-04DL 5X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DCW-WW-076-3515DL

Quant Time: Mar 10 01:15:54 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF021915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 10 00:35:08 2015
Response via : Initial Calibration

