

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030915\
 Data File : BF077641.D
 Acq On : 9 Mar 2015 16:40
 Operator : TP/IZ
 Sample : PB82019BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB82019BL

Quant Time: Mar 10 01:01:19 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF021915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 10 00:35:08 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.19	152	57743	20.00	ng	0.00
21) Naphthalene-d8	8.77	136	231674	20.00	ng	0.00
38) Acenaphthene-d10	10.94	164	112967	20.00	ng	0.00
63) Phenanthrene-d10	12.78	188	213052	20.00	ng	0.00
75) Chrysene-d12	16.06	240	221992	20.00	ng	0.00
86) Perylene-d12	17.76	264	231805	20.00	ng	0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.48	112	257161	74.35	ng	0.00
7) Phenol-d6	6.75	99	302662	68.06	ng	0.00
23) Nitrobenzene-d5	7.88	82	236414	63.46	ng	0.00
41) 2,4,6-Tribromophenol	11.92	330	72491	66.64	ng	0.00
44) 2-Fluorobiphenyl	10.11	172	490035	67.64	ng	0.00
78) Terphenyl-d14	14.77	244	561314	59.11	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030915\
Data File : BF077641.D
Acq On : 9 Mar 2015 16:40
Operator : TP/IZ
Sample : PB82019BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB82019BL

Quant Time: Mar 10 01:01:19 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF021915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 10 00:35:08 2015
Response via : Initial Calibration

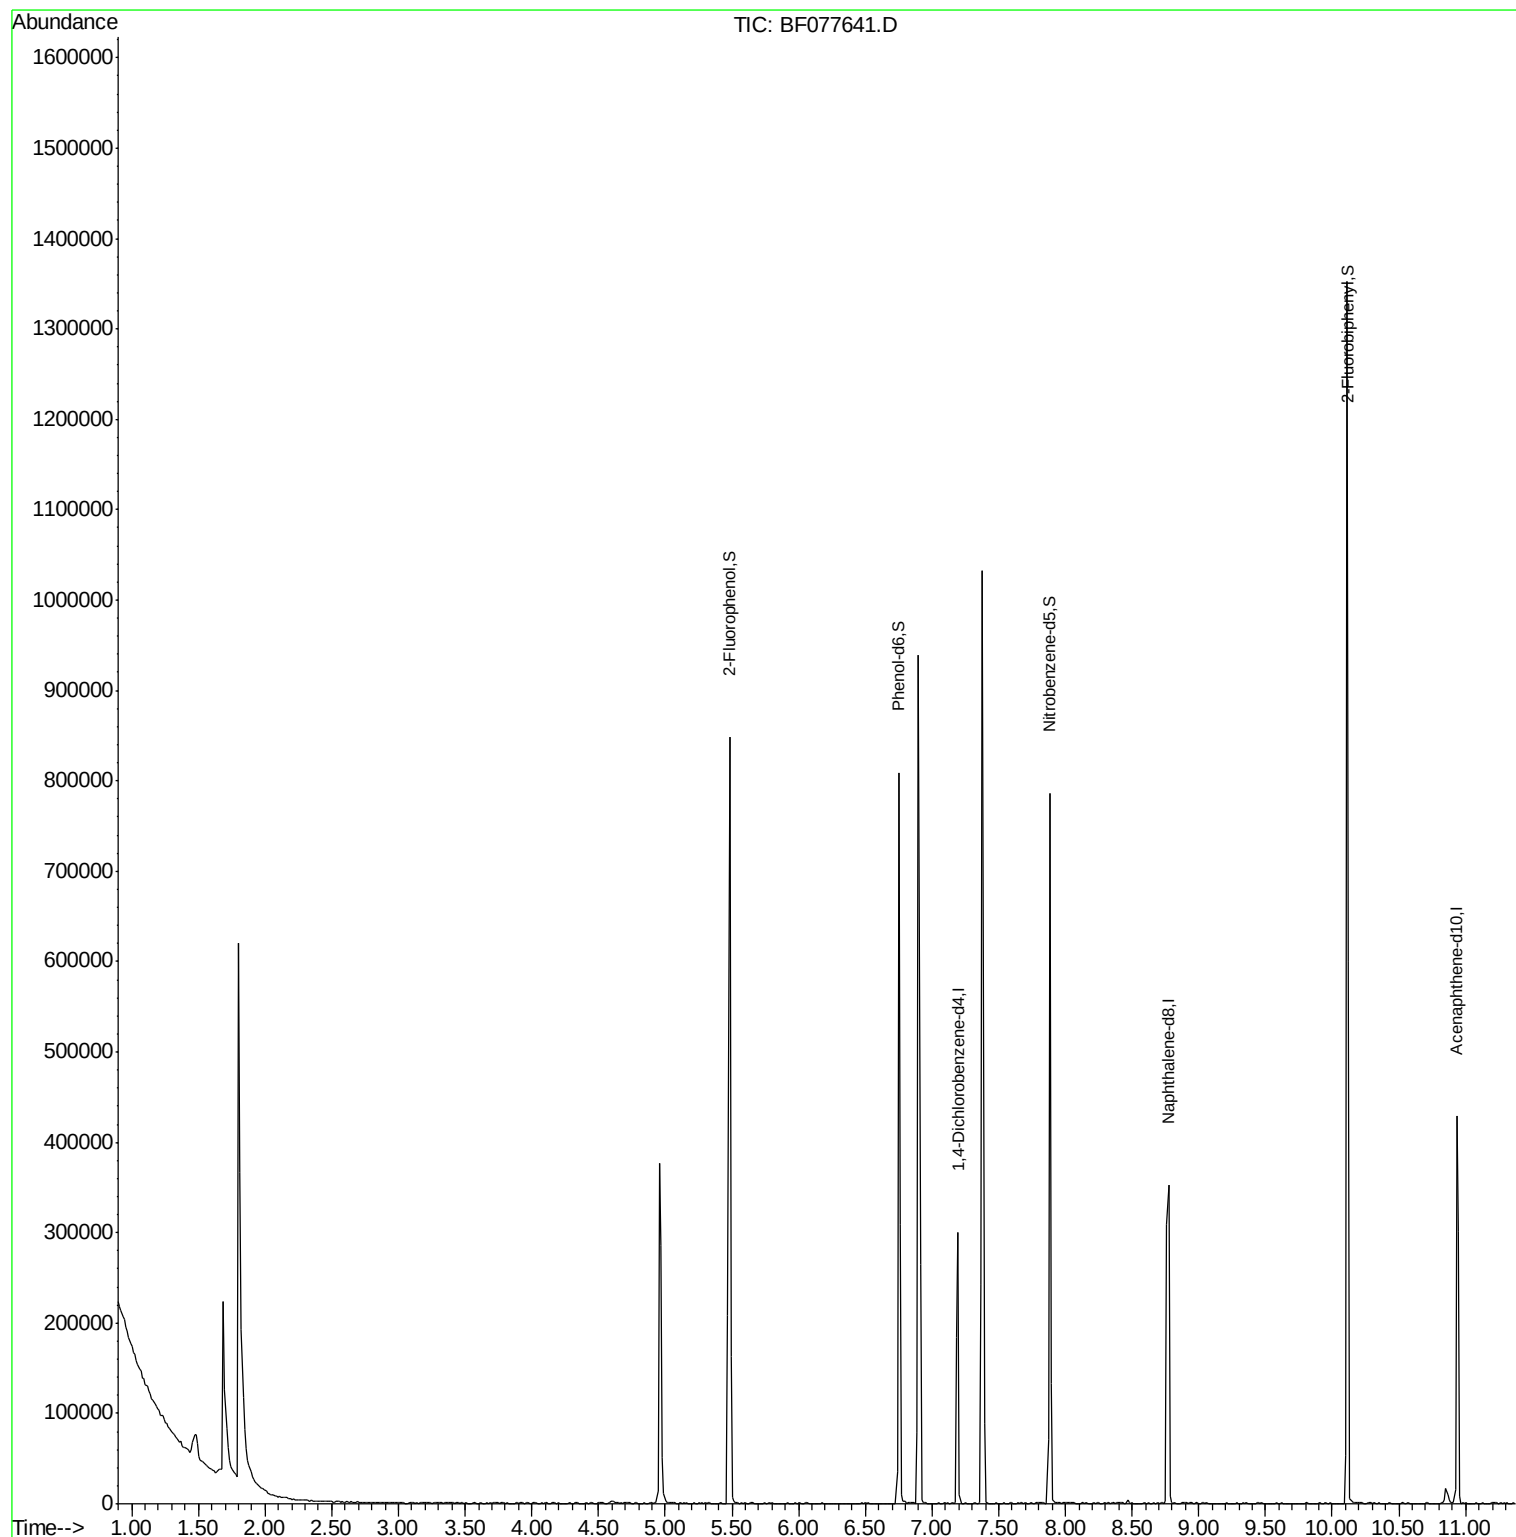

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030915\
Data File : BF077641.D
Acq On : 9 Mar 2015 16:40
Operator : TP/IZ
Sample : PB82019BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB82019BL

Quant Time: Mar 10 01:01:19 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF021915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 10 00:35:08 2015
Response via : Initial Calibration

