

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030915\
 Data File : BF077649.D
 Acq On : 9 Mar 2015 20:30
 Operator : TP/IZ
 Sample : G1453-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SEP3

Quant Time: Mar 10 02:29:39 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF021915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 10 00:35:08 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.19	152	52909	20.00	ng	0.00
21) Naphthalene-d8	8.77	136	210020	20.00	ng	0.00
38) Acenaphthene-d10	10.94	164	104278	20.00	ng	0.00
63) Phenanthrene-d10	12.78	188	210581	20.00	ng	0.00
75) Chrysene-d12	16.06	240	262202	20.00	ng	0.00
86) Perylene-d12	17.82	264	242810	20.00	ng	0.09

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.48	112	326143	102.91	ng	0.00
7) Phenol-d6	6.76	99	370787	90.99	ng	0.00
23) Nitrobenzene-d5	7.88	82	200658	59.41	ng	0.00
41) 2,4,6-Tribromophenol	11.92	330	96772	96.38	ng	0.00
44) 2-Fluorobiphenyl	10.11	172	401080	59.97	ng	0.00
78) Terphenyl-d14	14.77	244	494067	44.05	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
10) Phenol	6.77	94	10091	2.09	ng	95
70) Phenanthrene	12.81	178	56984	4.67	ng	97
74) Fluoranthene	14.28	202	84767	6.36	ng	98
77) Pyrene	14.56	202	78293	4.88	ng	98
80) Benzo(a)anthracene	16.05	228	43705	2.84	ng	97
82) Chrysene	16.09	228	42339	2.93	ng	97
83) Bis(2-ethylhexyl)phthalate	16.12	149	142105	13.43	ng	98
87) Benzo(b)fluoranthene	17.37	252	51881m	3.67	ng	
89) Benzo(a)pyrene	17.76	252	32811	2.44	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030915\
Data File : BF077649.D
Acq On : 9 Mar 2015 20:30
Operator : TP/IZ
Sample : G1453-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SEP3

Quant Time: Mar 10 02:29:39 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF021915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 10 00:35:08 2015
Response via : Initial Calibration

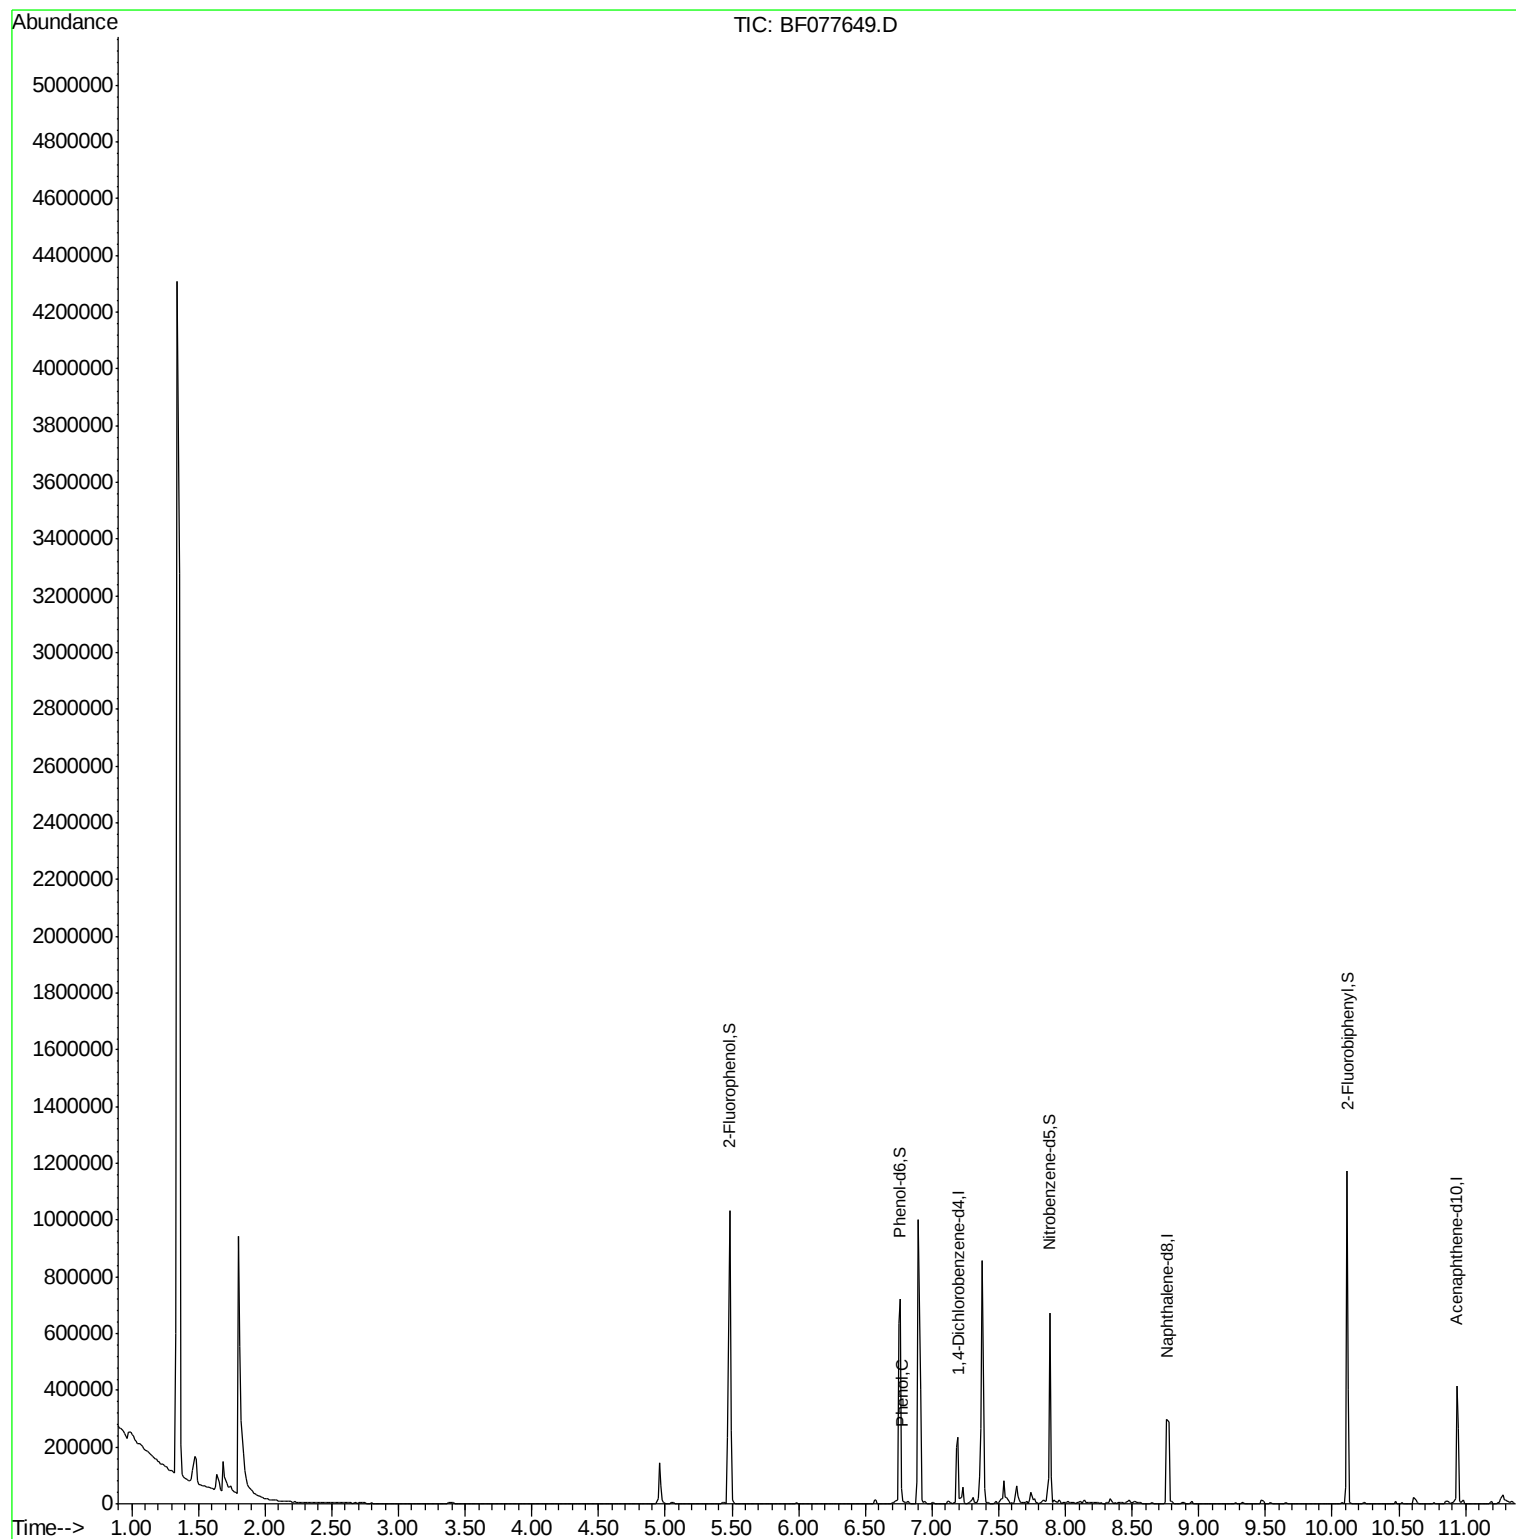

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030915\
Data File : BF077649.D
Acq On : 9 Mar 2015 20:30
Operator : TP/IZ
Sample : G1453-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SEP3

Quant Time: Mar 10 02:29:39 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF021915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 10 00:35:08 2015
Response via : Initial Calibration

