

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030915\
 Data File : BF077650.D
 Acq On : 9 Mar 2015 20:58
 Operator : TP/IZ
 Sample : G1453-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SEP4

Quant Time: Mar 10 02:39:56 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF021915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 10 00:35:08 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.19	152	54552	20.00	ng	0.00
21) Naphthalene-d8	8.77	136	219030	20.00	ng	0.00
38) Acenaphthene-d10	10.94	164	113136	20.00	ng	0.00
63) Phenanthrene-d10	12.78	188	242496	20.00	ng	0.00
75) Chrysene-d12	16.06	240	249614	20.00	ng	0.00
86) Perylene-d12	17.81	264	246397	20.00	ng	0.08
System Monitoring Compounds						
5) 2-Fluorophenol	5.48	112	241068	73.77	ng	0.00
7) Phenol-d6	6.76	99	298155	70.97	ng	0.00
23) Nitrobenzene-d5	7.88	82	178818	50.77	ng	0.00
41) 2,4,6-Tribromophenol	11.92	330	91085	83.61	ng	0.00
44) 2-Fluorobiphenyl	10.11	172	358687	49.43	ng	0.00
78) Terphenyl-d14	14.77	244	427934	40.08	ng	0.00
Target Compounds						Qvalue
70) Phenanthrene	12.80	178	118917	8.46	ng	99
74) Fluoranthene	14.28	202	82634	5.38	ng	99
77) Pyrene	14.56	202	137186	8.98	ng	96
80) Benzo(a)anthracene	16.05	228	57868	3.96	ng	96
82) Chrysene	16.09	228	58855	4.28	ng	97
87) Benzo(b)fluoranthene	17.37	252	48170m	3.36	ng	
89) Benzo(a)pyrene	17.74	252	45046	3.30	ng	# 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030915\
Data File : BF077650.D
Acq On : 9 Mar 2015 20:58
Operator : TP/IZ
Sample : G1453-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SEP4

Quant Time: Mar 10 02:39:56 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF021915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 10 00:35:08 2015
Response via : Initial Calibration

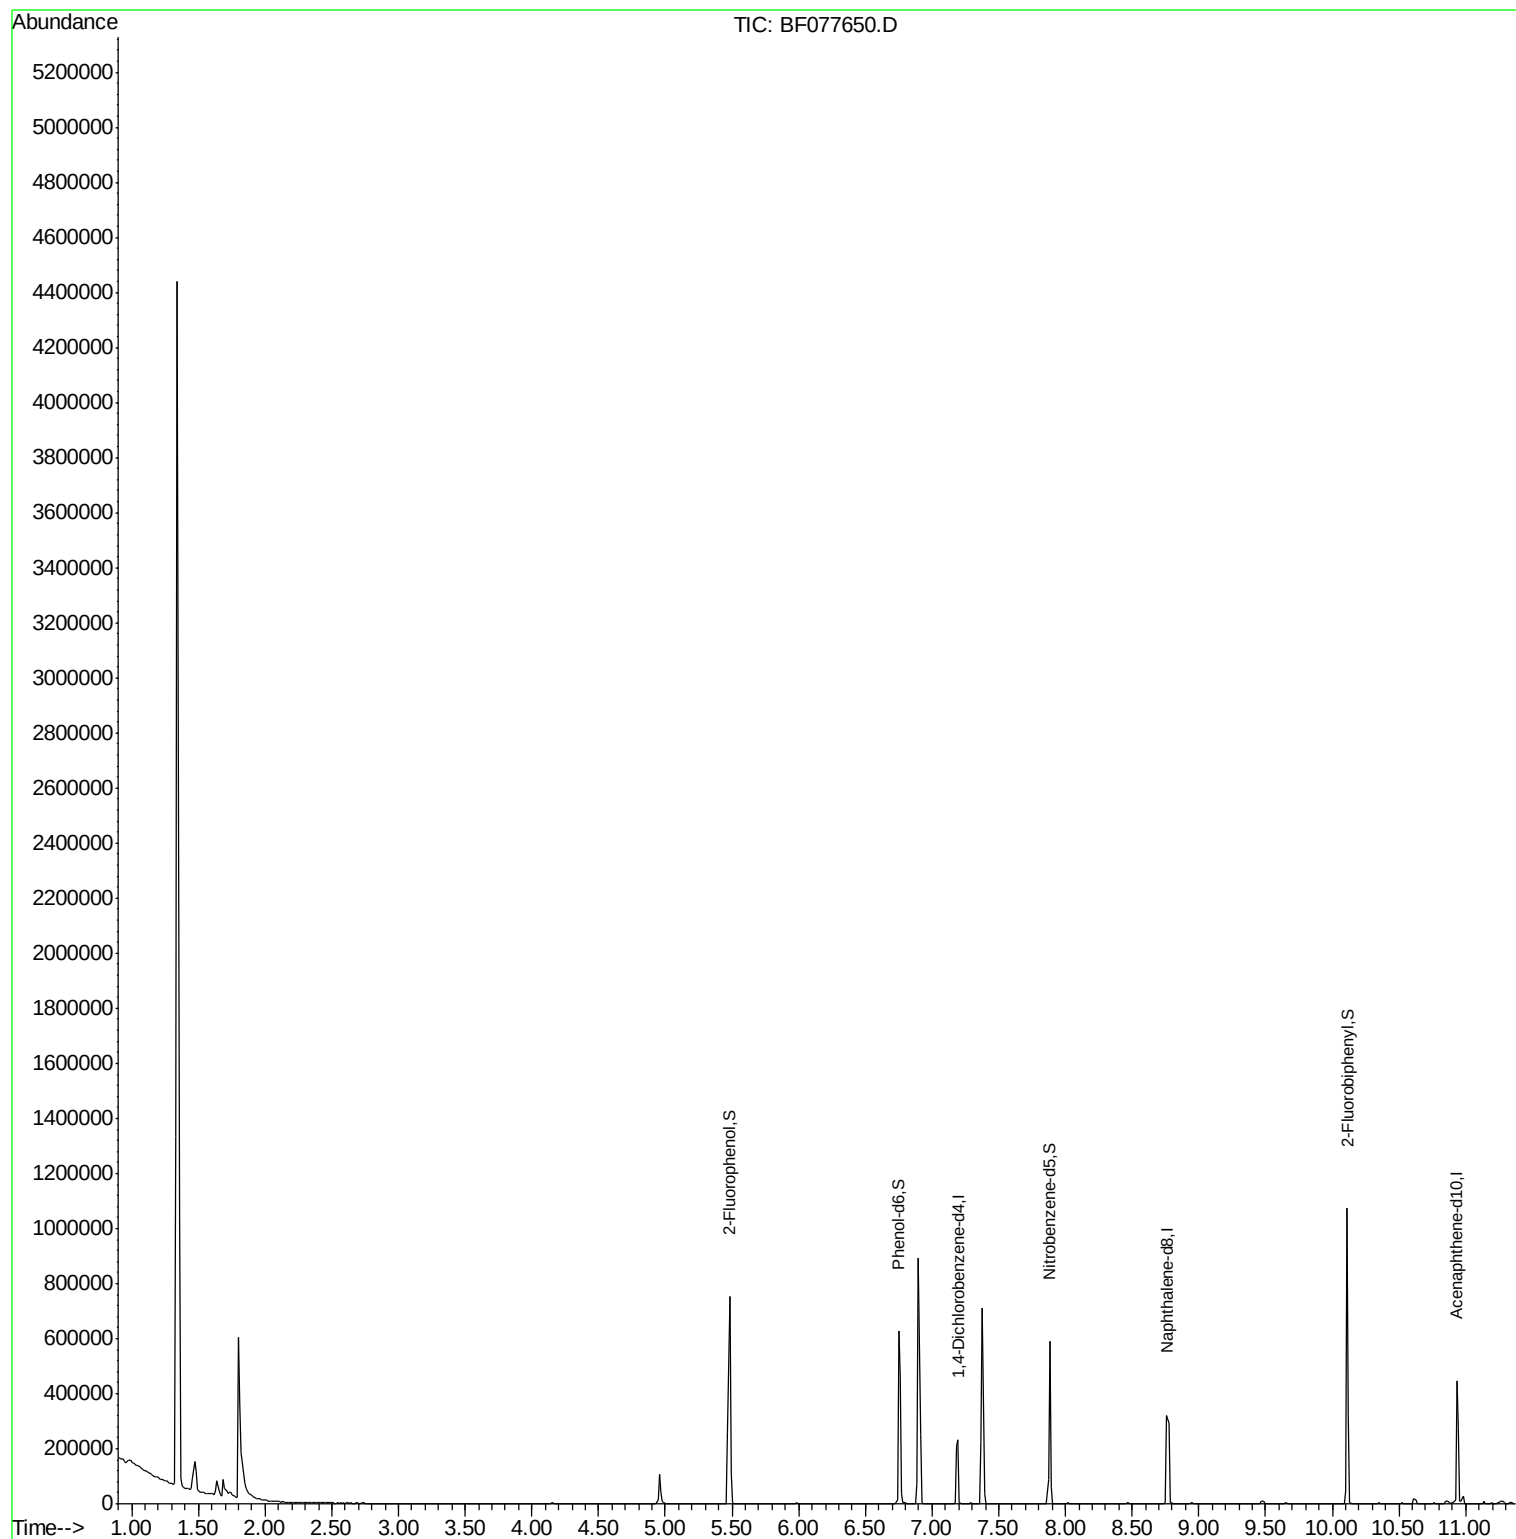

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030915\
Data File : BF077650.D
Acq On : 9 Mar 2015 20:58
Operator : TP/IZ
Sample : G1453-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SEP4

Quant Time: Mar 10 02:39:56 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF021915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 10 00:35:08 2015
Response via : Initial Calibration

