

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030915\
 Data File : BF077654.D
 Acq On : 9 Mar 2015 22:53
 Operator : TP/IZ
 Sample : G1453-01DL 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SEP2DL

Quant Time: Mar 10 03:40:04 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF021915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 10 00:35:08 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.19	152	50697	20.00	ng	0.00
21) Naphthalene-d8	8.77	136	209128	20.00	ng	0.00
38) Acenaphthene-d10	10.94	164	108184	20.00	ng	0.00
63) Phenanthrene-d10	12.78	188	225045	20.00	ng	0.00
75) Chrysene-d12	16.06	240	288822	20.00	ng	0.00
86) Perylene-d12	17.75	264	246104	20.00	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.50	112	46262	15.23	ng	0.02
7) Phenol-d6	6.76	99	57000	14.60	ng	0.00
23) Nitrobenzene-d5	7.88	82	27634	8.22	ng	0.00
41) 2,4,6-Tribromophenol	11.92	330	1248	1.20	ng	0.00
44) 2-Fluorobiphenyl	10.12	172	66659	9.61	ng	0.00
78) Terphenyl-d14	14.77	244	92253	7.47	ng	0.00
Target Compounds						
74) Fluoranthene	14.28	202	46990	3.30	ng	98
77) Pyrene	14.56	202	42552	2.41	ng	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030915\
Data File : BF077654.D
Acq On : 9 Mar 2015 22:53
Operator : TP/IZ
Sample : G1453-01DL 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SEP2DL

Quant Time: Mar 10 03:40:04 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF021915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 10 00:35:08 2015
Response via : Initial Calibration

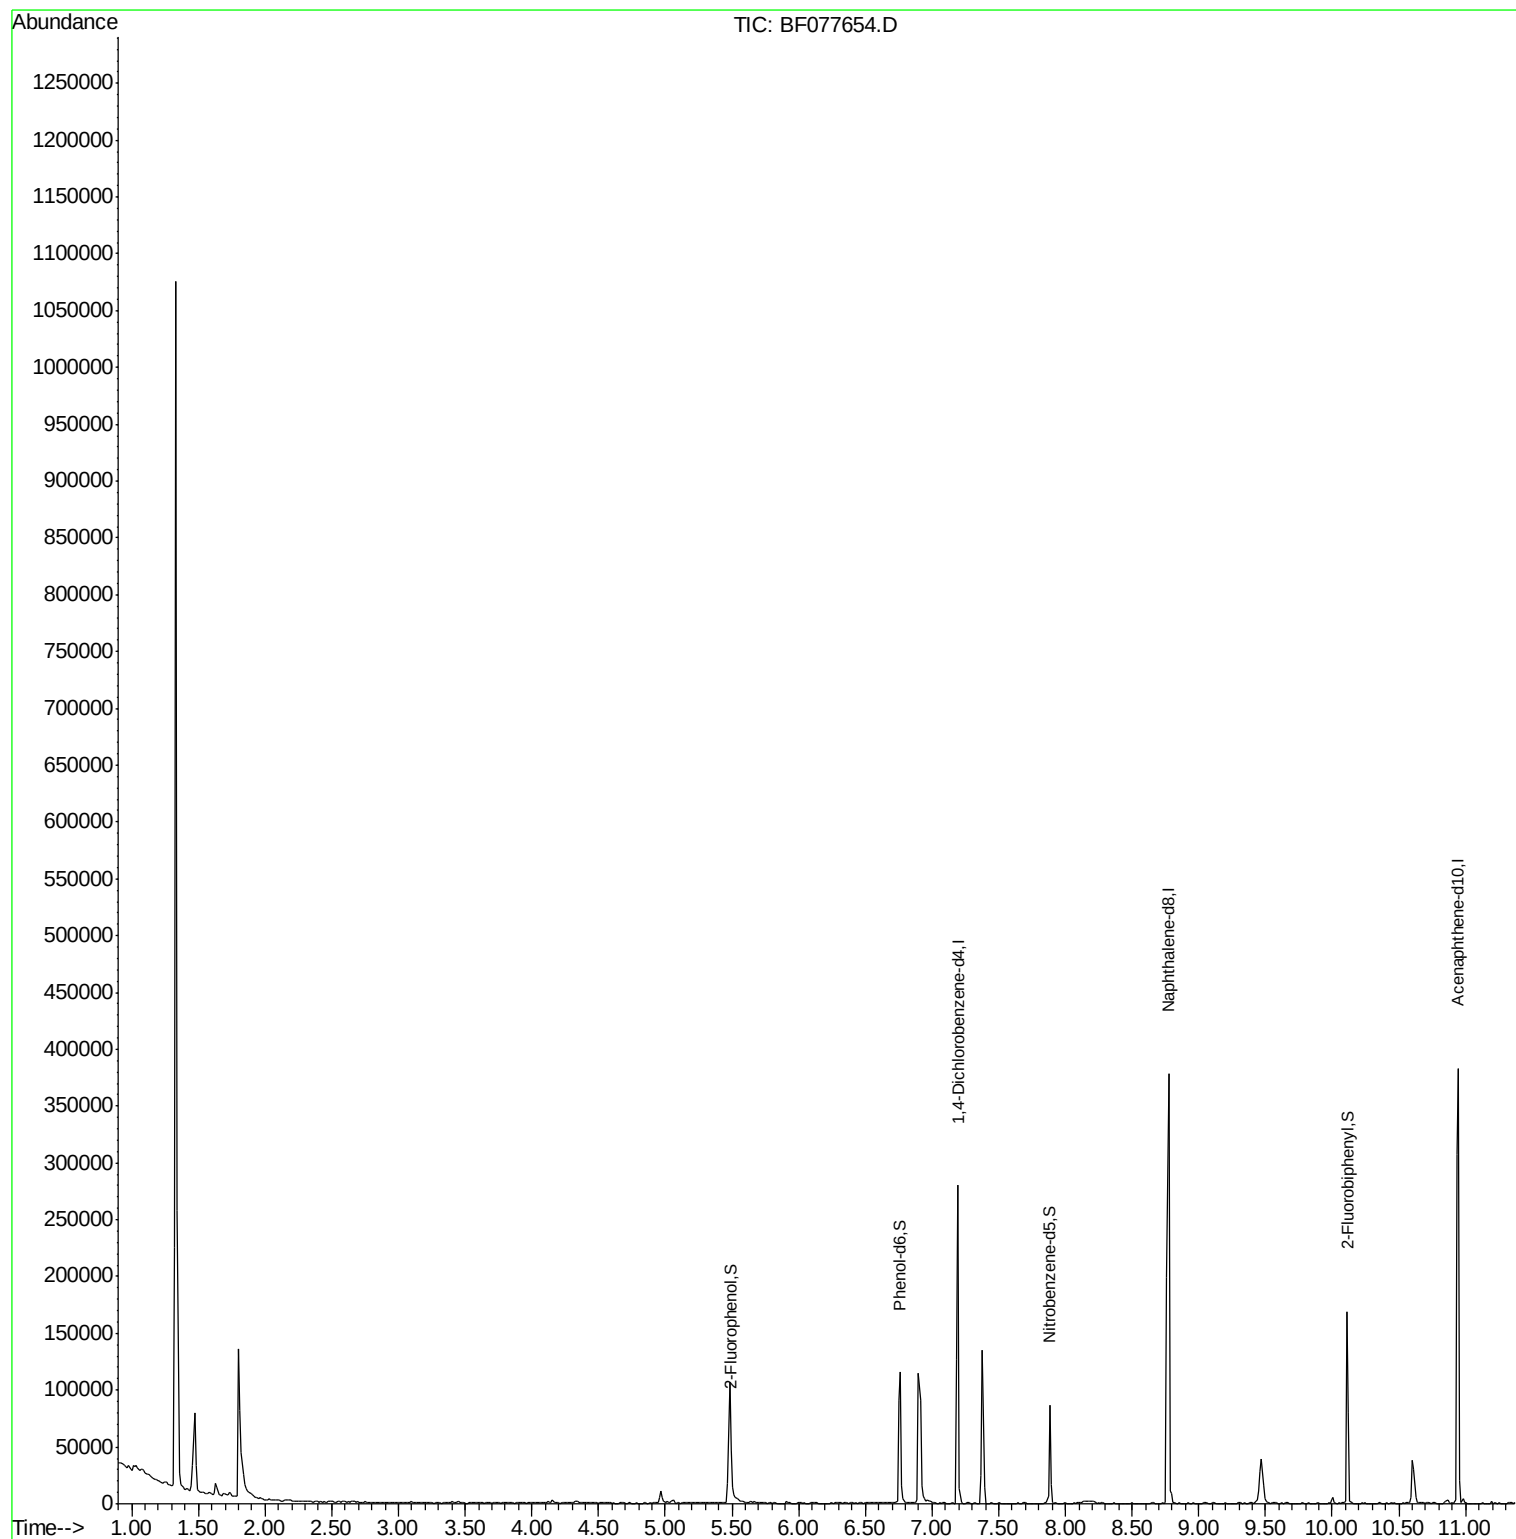

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030915\
Data File : BF077654.D
Acq On : 9 Mar 2015 22:53
Operator : TP/IZ
Sample : G1453-01DL 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SEP2DL

Quant Time: Mar 10 03:40:04 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF021915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 10 00:35:08 2015
Response via : Initial Calibration

