

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030915\
 Data File : BF077655.D
 Acq On : 9 Mar 2015 23:22
 Operator : TP/IZ
 Sample : G1453-03DL 5X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SEP4DL

Quant Time: Mar 10 01:08:39 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF021915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 10 00:35:08 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.19	152	47157	20.00	ng	0.00
21) Naphthalene-d8	8.77	136	197580	20.00	ng	0.00
38) Acenaphthene-d10	10.94	164	101264	20.00	ng	0.00
63) Phenanthrene-d10	12.78	188	210352	20.00	ng	0.00
75) Chrysene-d12	16.06	240	267528	20.00	ng	0.00
86) Perylene-d12	17.73	264	267796	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.49	112	43623	15.44	ng	0.00
7) Phenol-d6	6.76	99	53322	14.68	ng	0.00
23) Nitrobenzene-d5	7.88	82	25366	7.98	ng	0.00
41) 2,4,6-Tribromophenol	11.92	330	2406	2.47	ng	0.00
44) 2-Fluorobiphenyl	10.12	172	60157	9.26	ng	0.00
78) Terphenyl-d14	14.77	244	79887	6.98	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030915\
Data File : BF077655.D
Acq On : 9 Mar 2015 23:22
Operator : TP/IZ
Sample : G1453-03DL 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SEP4DL

Quant Time: Mar 10 01:08:39 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF021915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 10 00:35:08 2015
Response via : Initial Calibration

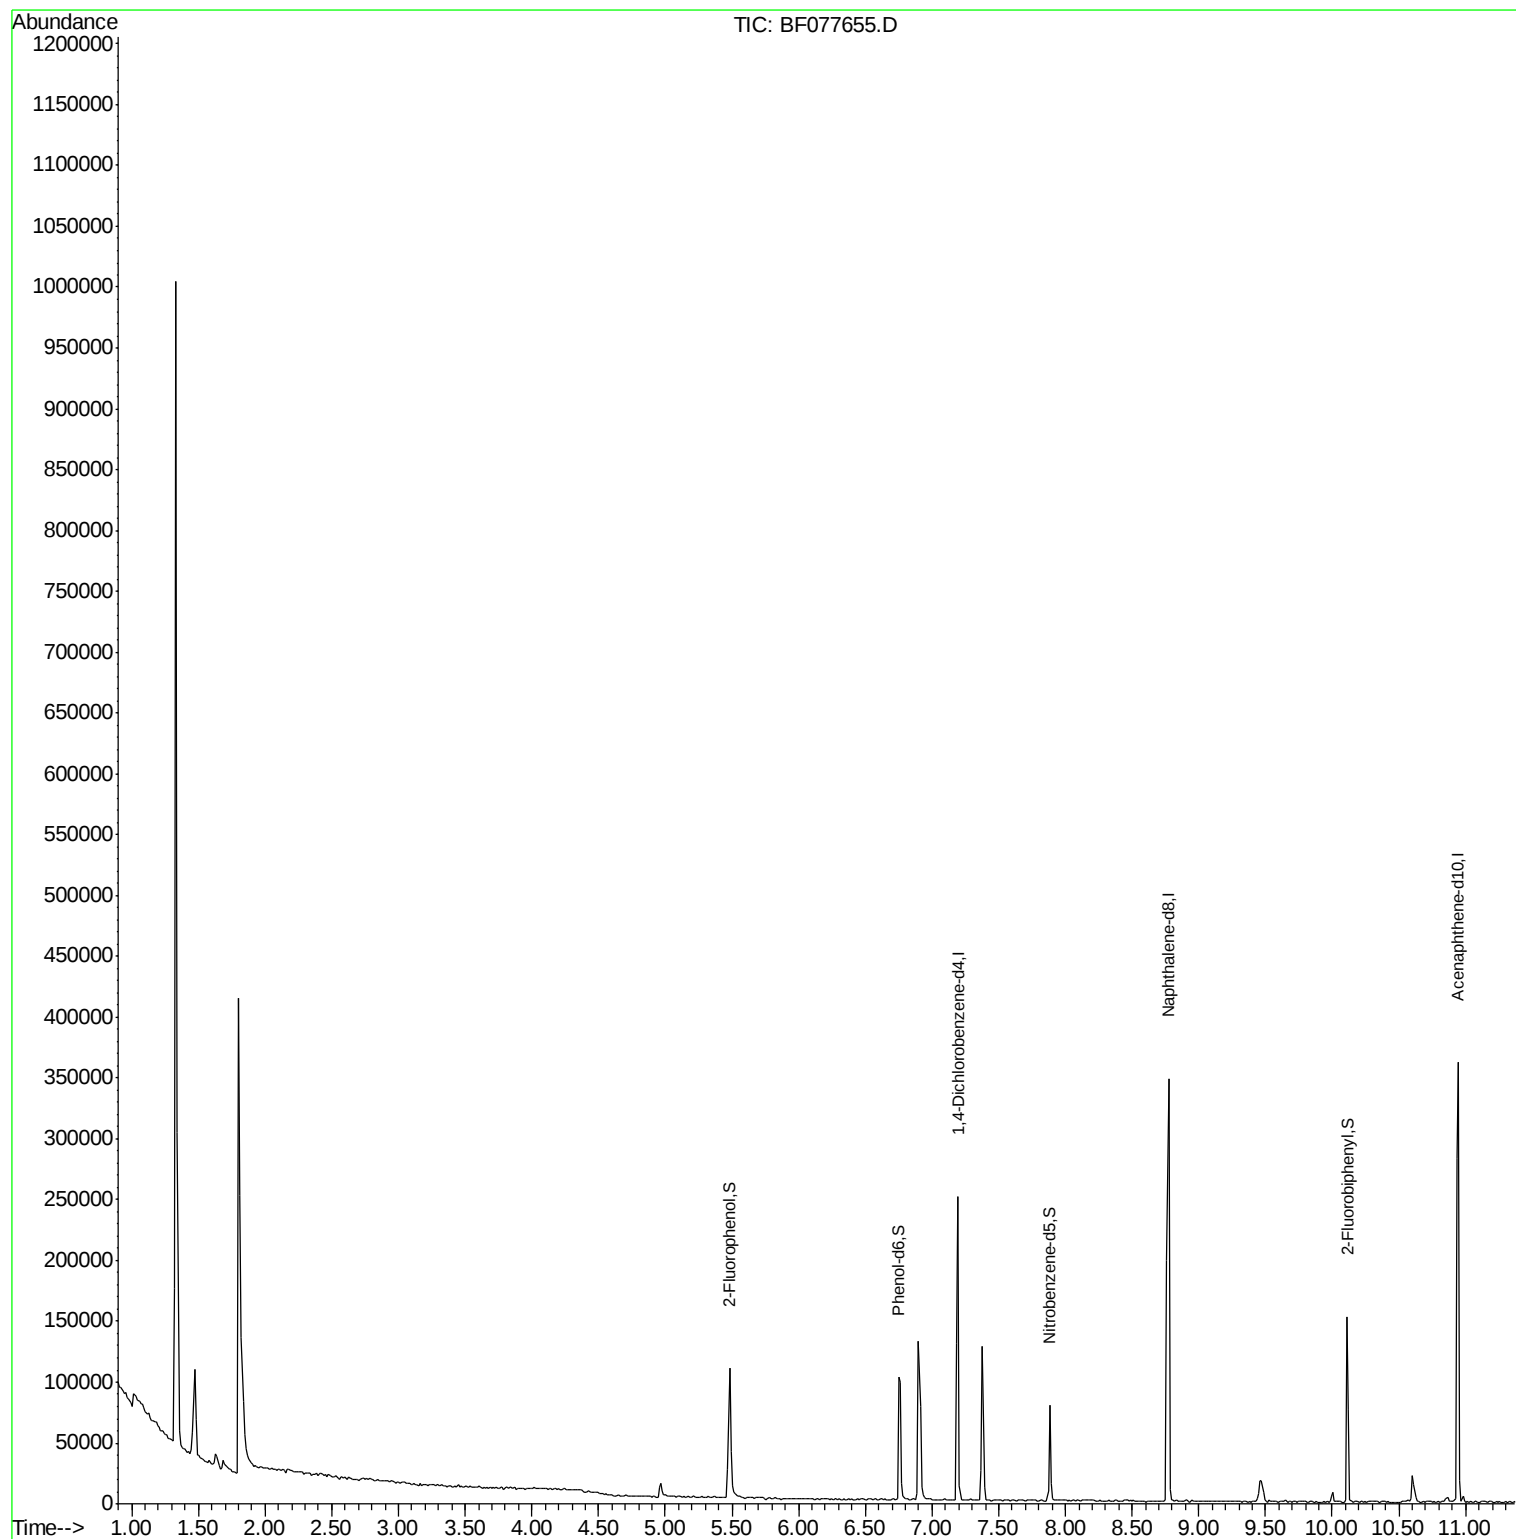

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030915\
Data File : BF077655.D
Acq On : 9 Mar 2015 23:22
Operator : TP/IZ
Sample : G1453-03DL 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SEP4DL

Quant Time: Mar 10 01:08:39 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF021915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 10 00:35:08 2015
Response via : Initial Calibration

