
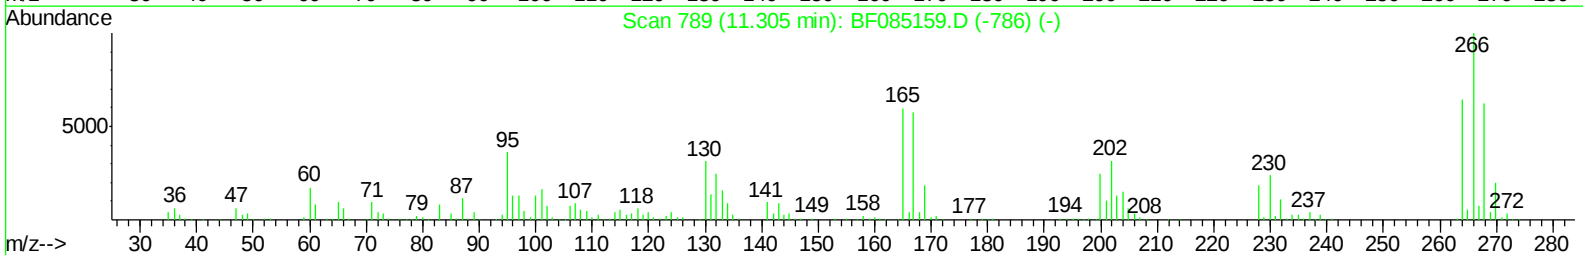
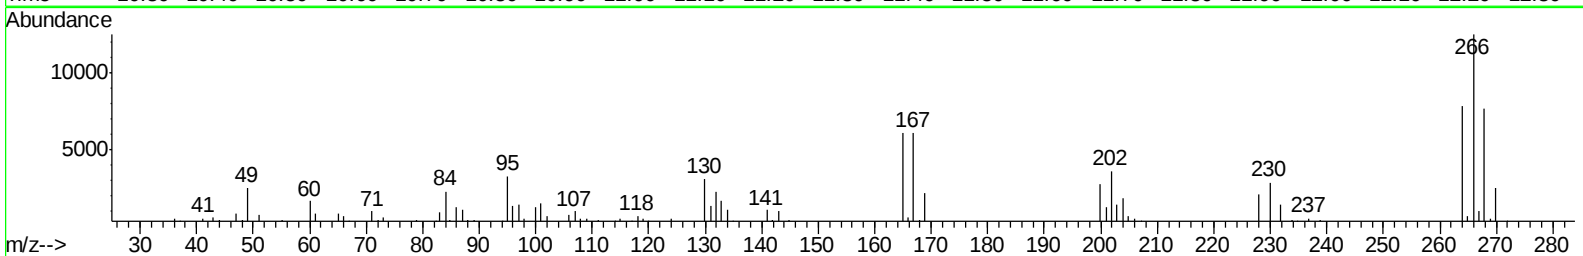


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030916\
Data File : BF085299.D
Acq On : 9 Mar 2016 14:06
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 02:19:51 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 04 00:54:58 2016
Response via : Initial Calibration

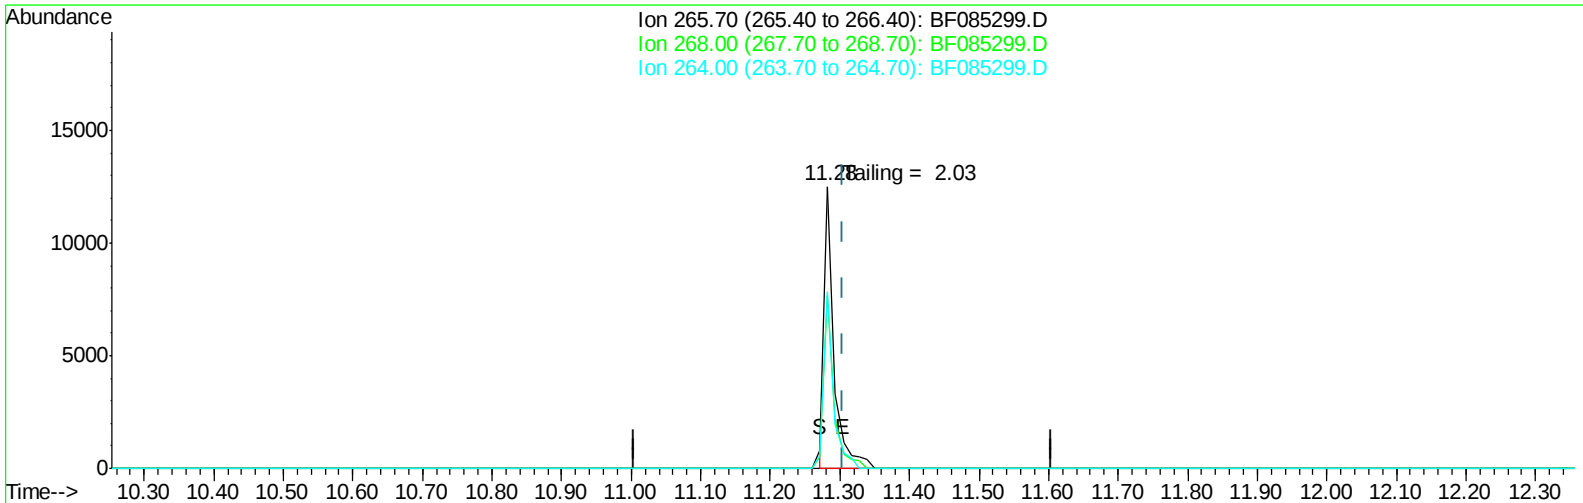

TIC: BF085299.D

(69) Pentachlorophenol (C)




11.282min (-0.023) 10642.25ng

response 13095

Ion	Exp%	Act%
265.70	100	100
268.00	62.50	61.33
264.00	64.30	62.69
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030916\  
Data File : BF085299.D  
Acq On    : 9 Mar 2016 14:06  
Operator  : UM/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Quant Time: Mar 10 02:19:51 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 04 00:54:58 2016
Response via : Initial Calibration

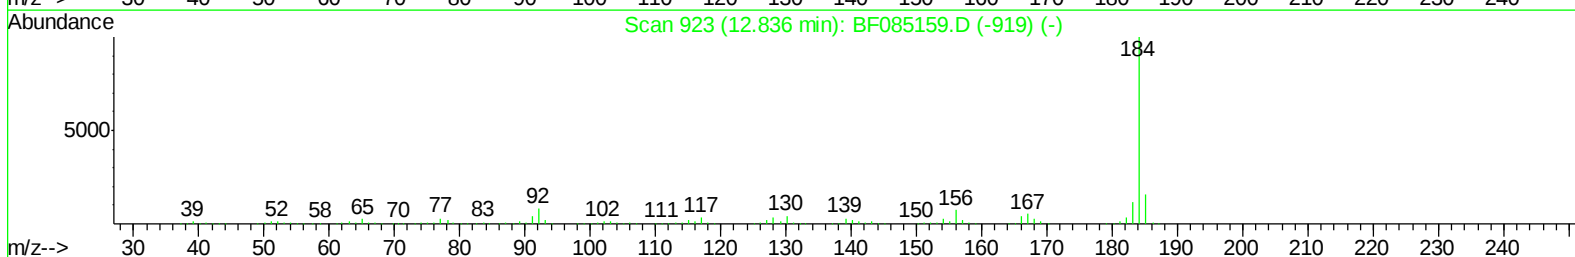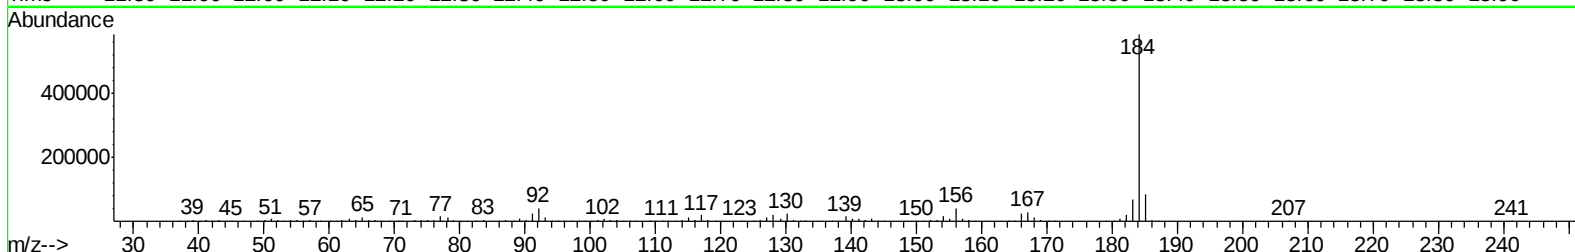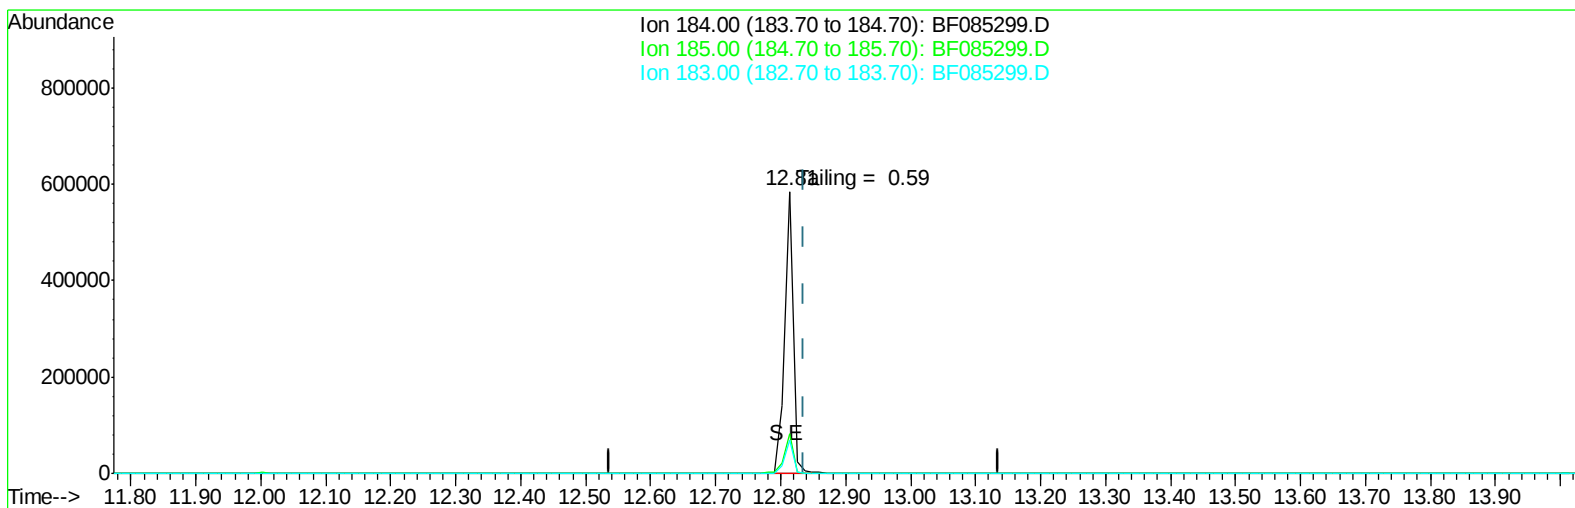

TIC: BF085299.D

(76) Benzidine

12.814min (-0.023) 0.00ng

response 527075

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.15
183.00	11.80	11.78
0.00	0.00	0.00