
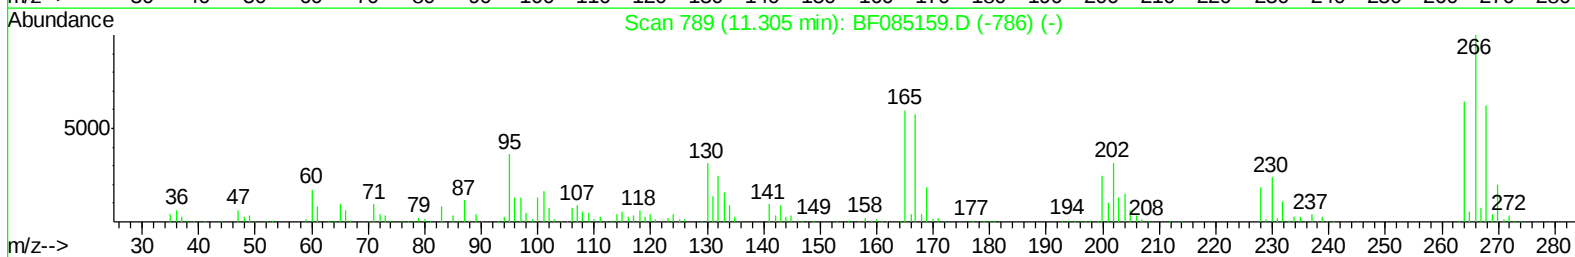
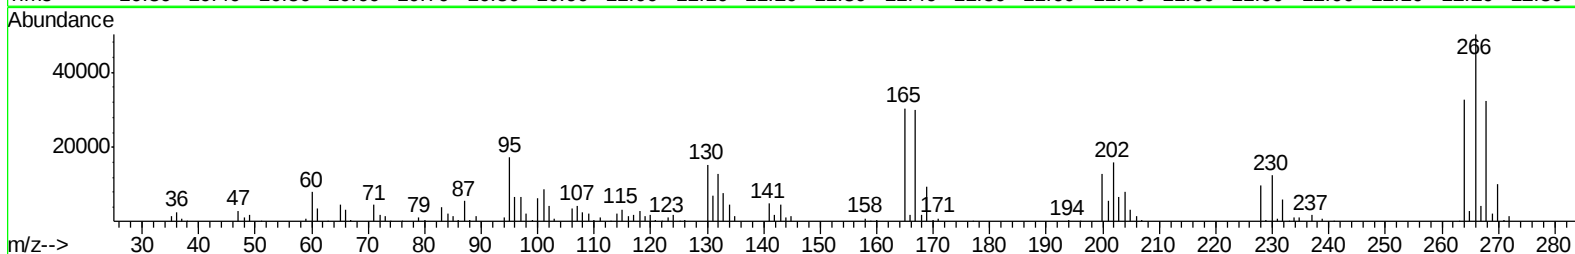


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030916\
Data File : BF085319.D
Acq On : 10 Mar 2016 00:55
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 02:22:59 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 04 00:54:58 2016
Response via : Initial Calibration

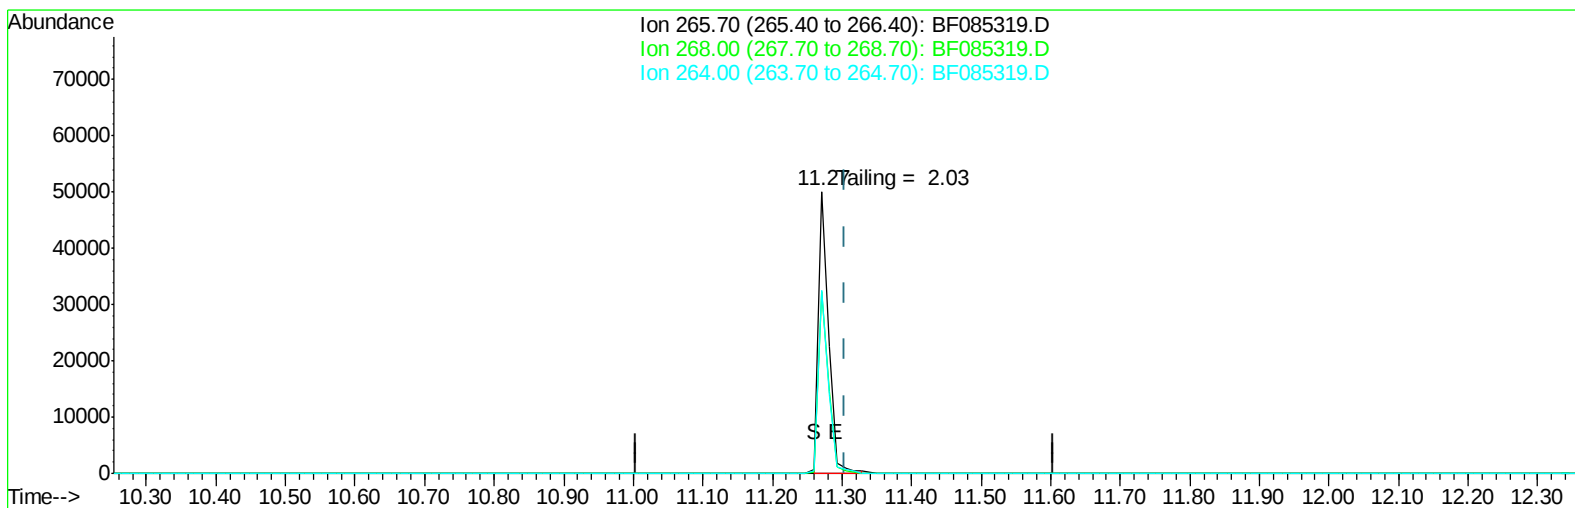

TIC: BF085319.D

(69) Pentachlorophenol (C)




11.270min (-0.034) 23719.93ng

response 52918

Ion	Exp%	Act%
265.70	100	100
268.00	62.50	64.76
264.00	64.30	64.99
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030916\
Data File : BF085319.D
Acq On : 10 Mar 2016 00:55
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 02:22:59 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 04 00:54:58 2016
Response via : Initial Calibration

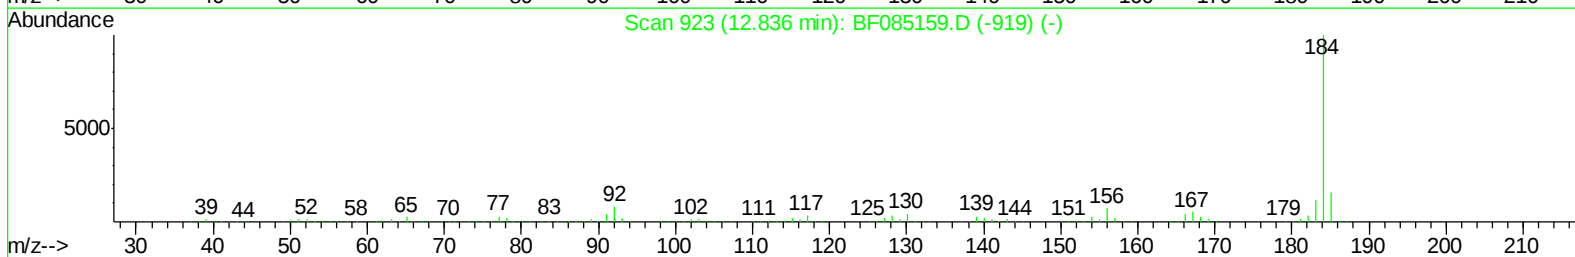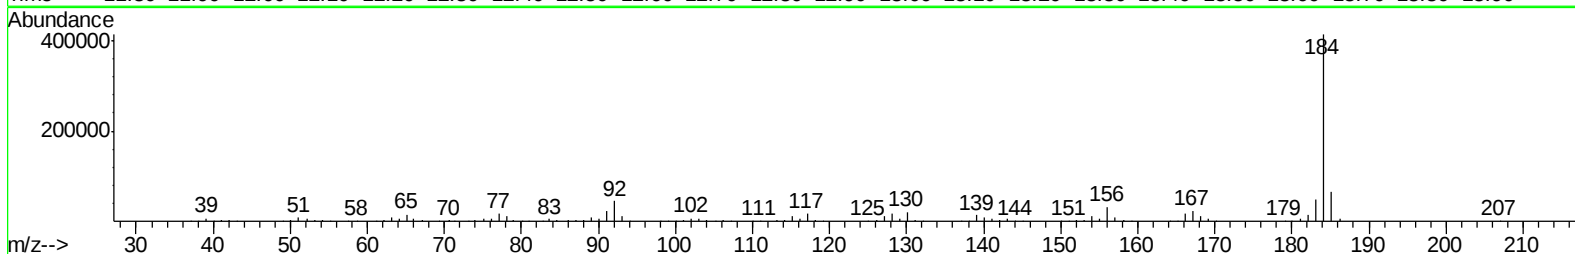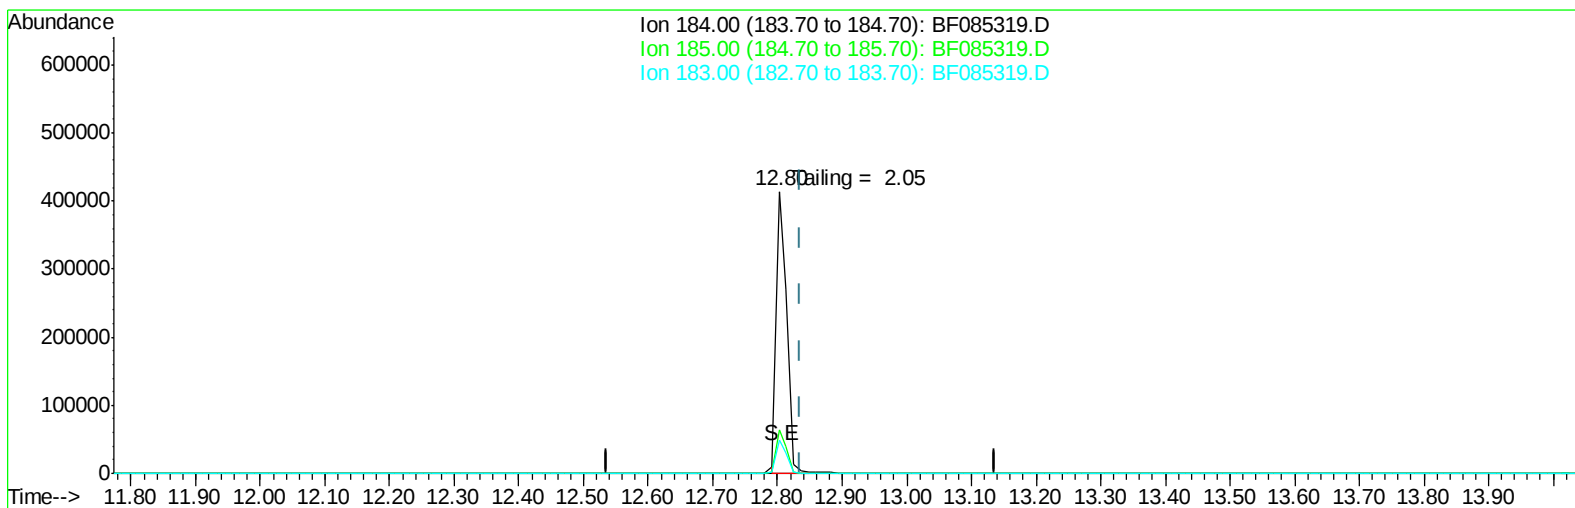

TIC: BF085319.D

(76) Benzidine

12.802min (-0.034) 0.00ng

response 496443

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	15.62
183.00	11.80	11.76
0.00	0.00	0.00