

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030916\
 Data File : BF085317.D
 Acq On : 9 Mar 2016 23:58
 Operator : UM/SJ
 Sample : H1724-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 UST-FD-3-8-16

Quant Time: Mar 10 01:23:16 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 04 00:54:58 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.94	152	152001	20.00	ng	-0.05
21) Naphthalene-d8	8.23	136	694325	20.00	ng	-0.03
38) Acenaphthene-d10	9.99	164	323314	20.00	ng	-0.03
63) Phenanthrene-d10	11.48	188	581127	20.00	ng	-0.03
75) Chrysene-d12	14.11	240	379192	20.00	ng	-0.05
86) Perylene-d12	15.57	264	245854	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	1148841	126.78	ng	-0.02
7) Phenol-d6	6.57	99	1480586	124.71	ng	-0.03
23) Nitrobenzene-d5	7.51	82	1110371	85.58	ng	-0.03
41) 2,4,6-Tribromophenol	10.78	330	379036	137.01	ng	-0.03
44) 2-Fluorobiphenyl	9.30	172	1570647	73.88	ng	-0.05
78) Terphenyl-d14	13.07	244	1503796	92.06	ng	-0.02
Target Compounds						
49) Dimethylphthalate	9.70	163	395974	15.96	ng	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030916\
Data File : BF085317.D
Acq On : 9 Mar 2016 23:58
Operator : UM/SJ
Sample : H1724-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
UST-FD-3-8-16

Quant Time: Mar 10 01:23:16 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 04 00:54:58 2016
Response via : Initial Calibration

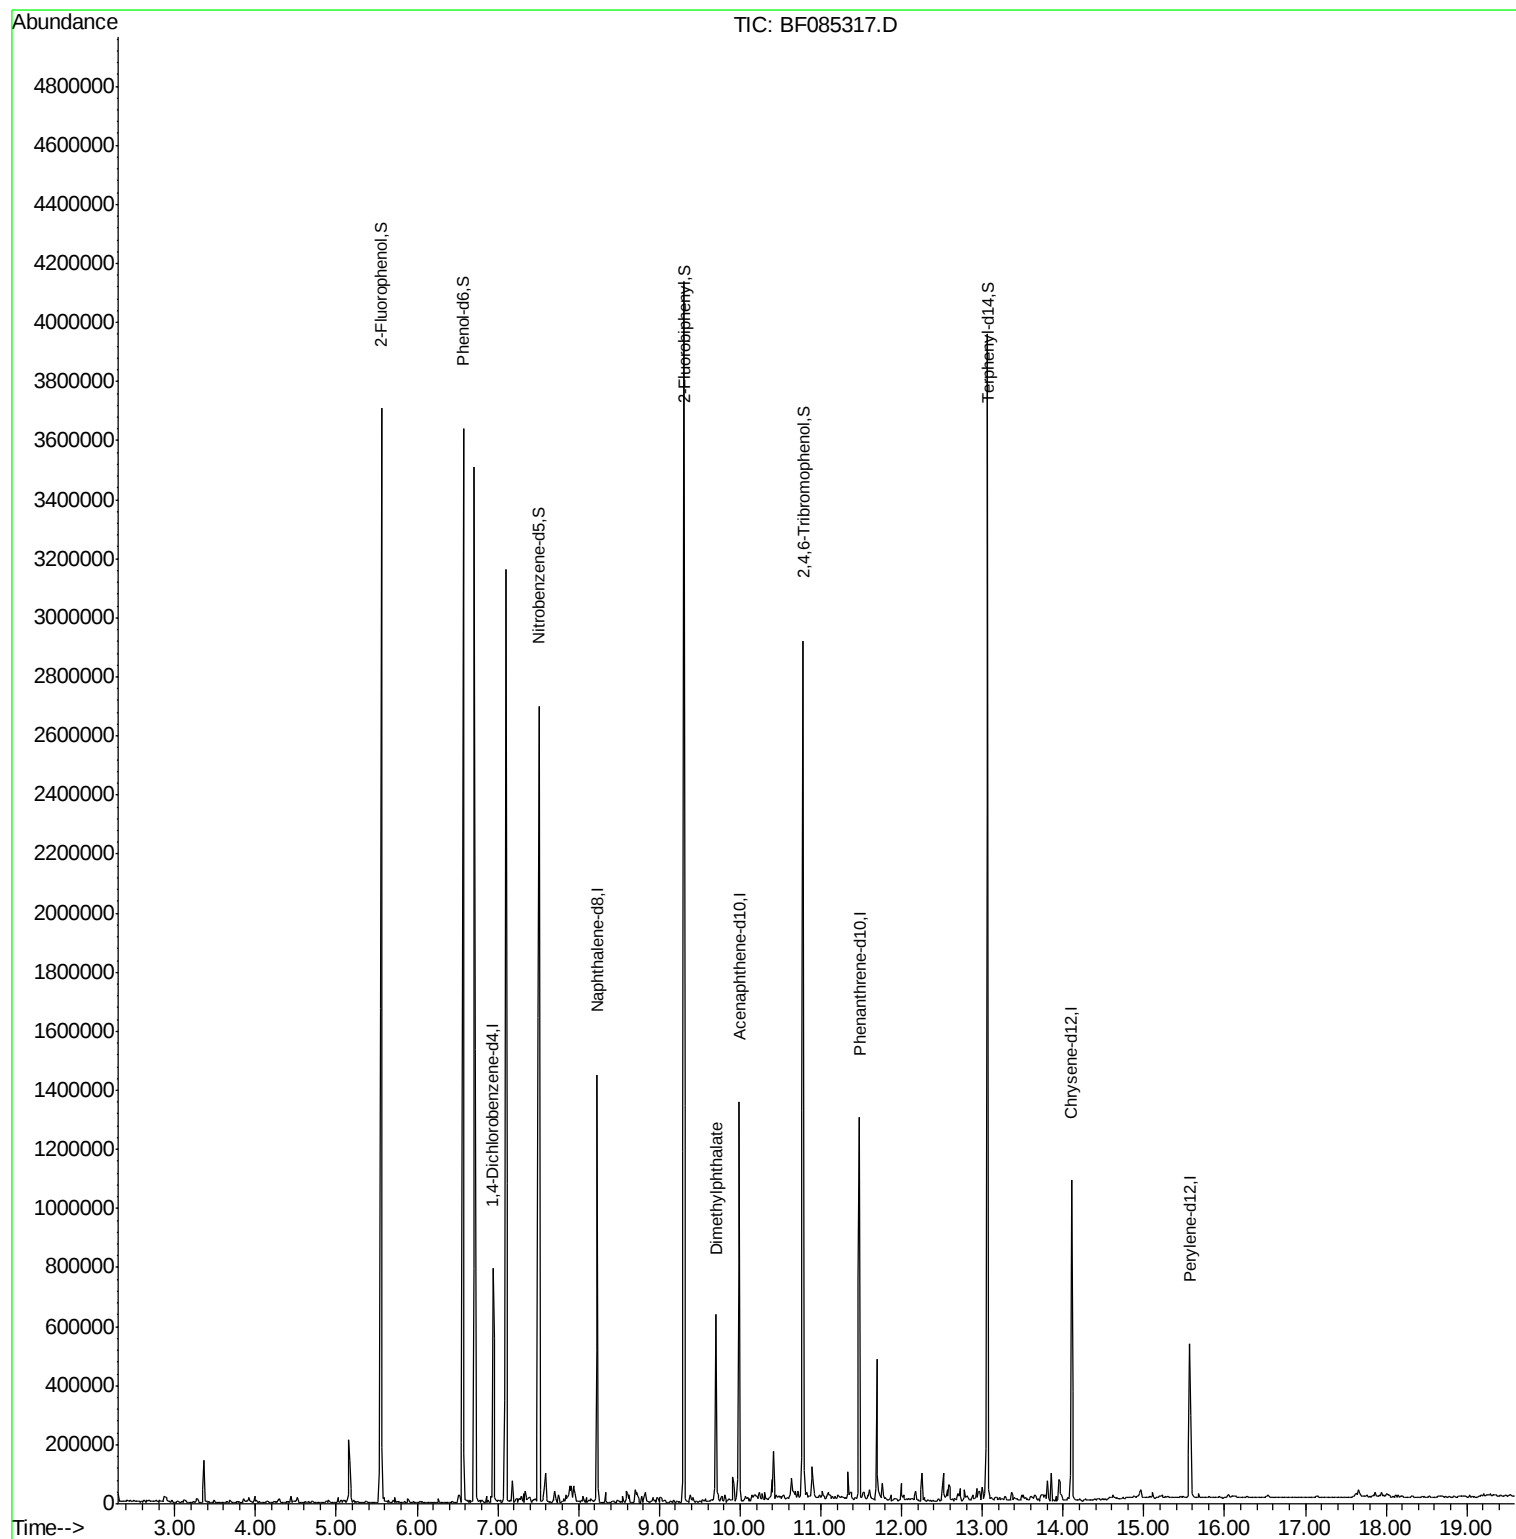

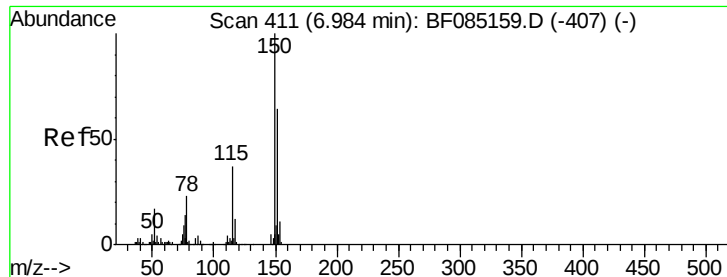

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.94 min Scan# 407

Delta R.T. -0.05 min

Lab File: BF085317.D

Acq: 9 Mar 2016 23:58

Instrument :

BNA_F

ClientSampleId :

UST-FD-3-8-16


Tgt Ion:152 Resp: 152001

Ion Ratio Lower Upper

152 100

150 163.6 124.6 186.8




115 75.5 46.6 70.0#

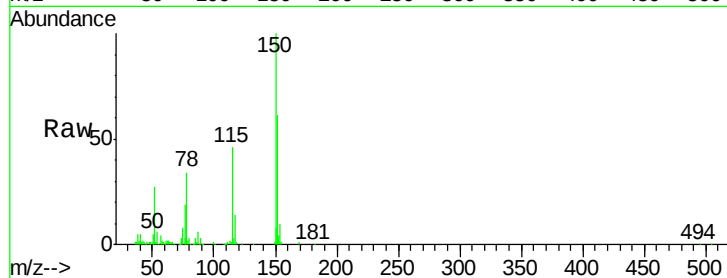

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

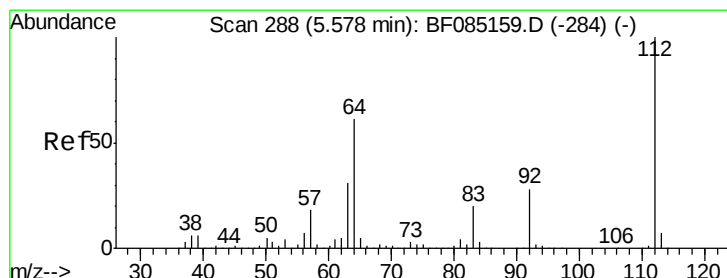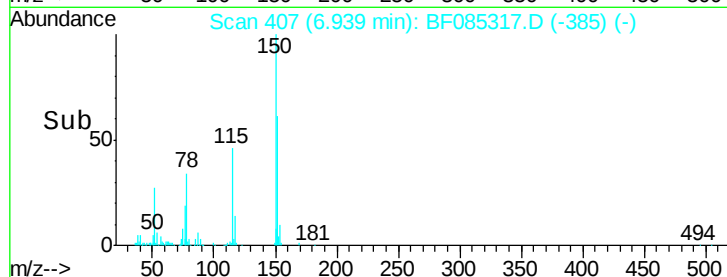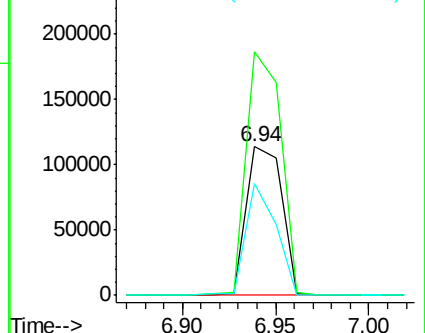

#5

2-Fluorophenol

Concen: 126.78 ng

RT: 5.56 min Scan# 286

Delta R.T. -0.02 min

Lab File: BF085317.D

Acq: 9 Mar 2016 23:58


Tgt Ion:112 Resp: 1148841

Ion Ratio Lower Upper

112 100

64 58.0 49.0 73.4



63 28.9 24.8 37.2

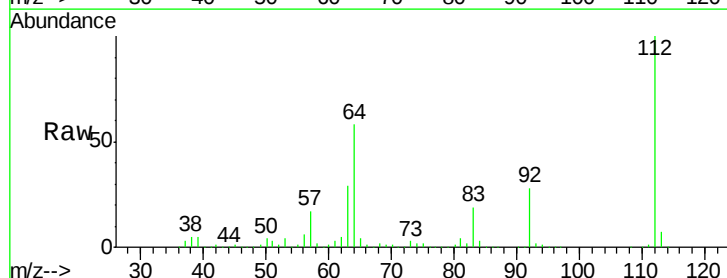


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

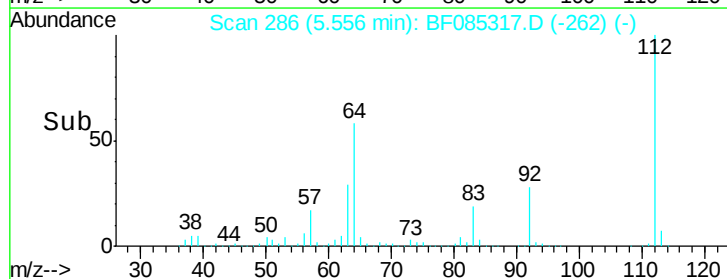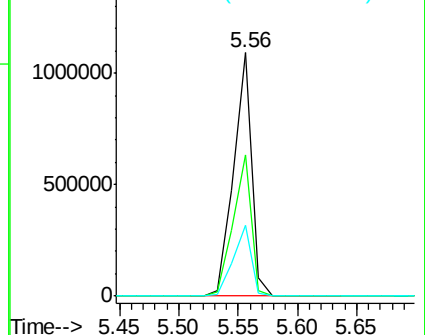

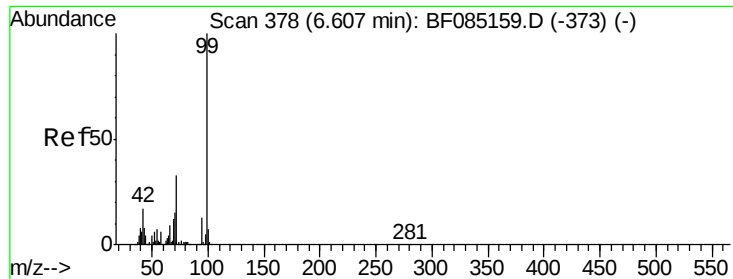

#7

Phenol-d6

Concen: 124.71 ng

RT: 6.57 min Scan# 375

Delta R.T. -0.03 min

Lab File: BF085317.D

Acq: 9 Mar 2016 23:58

Instrument :

BNA_F

ClientSampleId :

UST-FD-3-8-16


Tgt Ion: 99 Resp: 1480586

Ion Ratio Lower Upper

99 100

42 15.6 13.6 20.4




71 33.7 26.7 40.1

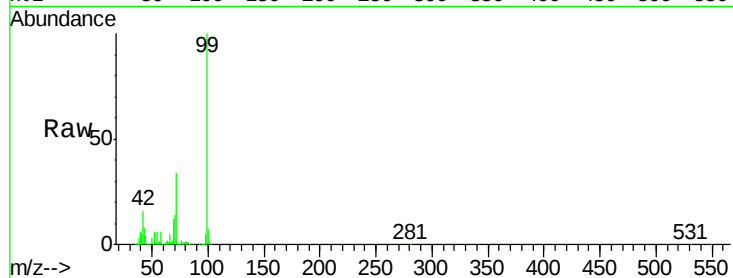

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

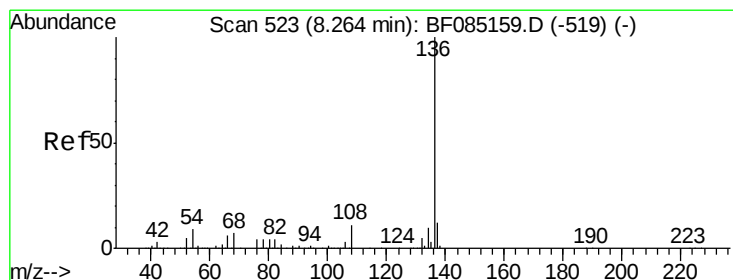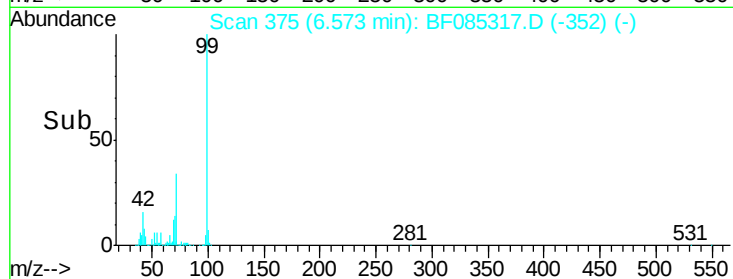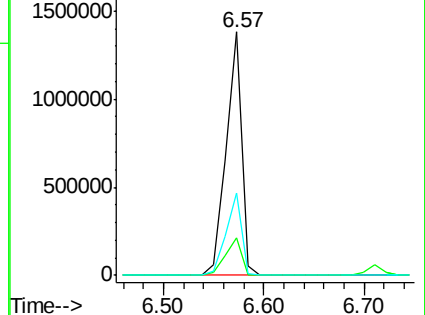

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.23 min Scan# 520

Delta R.T. -0.03 min

Lab File: BF085317.D

Acq: 9 Mar 2016 23:58

Tgt Ion: 136 Resp: 694325


Ion Ratio Lower Upper

136 100

137 10.9 9.3 13.9

54 6.4 7.4 11.2#

68 5.5 6.0 9.0#


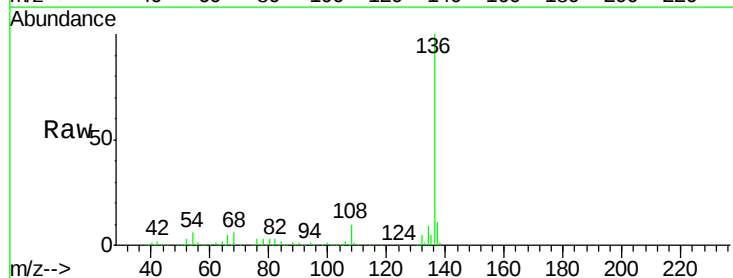



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



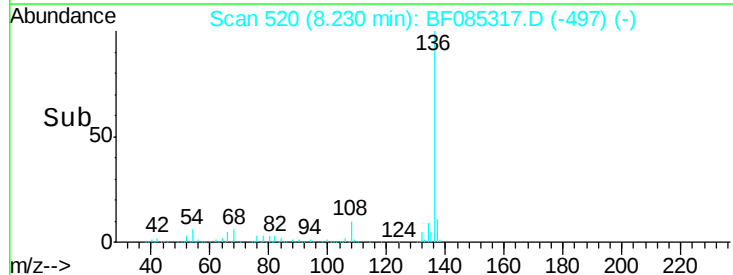
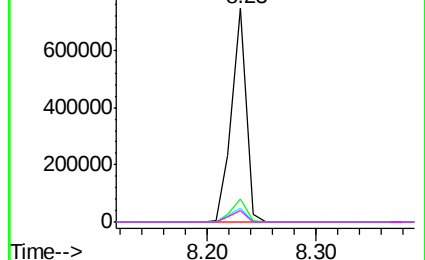


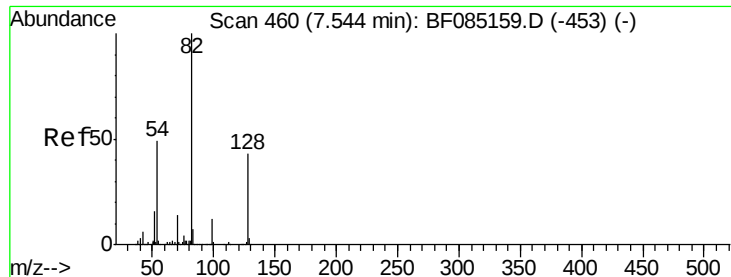

#23
 Nitrobenzene-d5
 Concen: 85.58 ng
 RT: 7.51 min Scan# 457
 Delta R.T. -0.03 min
 Lab File: BF085317.D
 Acq: 9 Mar 2016 23:58




Instrument :
 BNA_F
 ClientSampleId :
 UST-FD-3-8-16


Tgt Ion: 82 Resp: 1110371
 Ion Ratio Lower Upper
 82 100
 128 48.9 34.5 51.7
 54 43.8 39.3 58.9

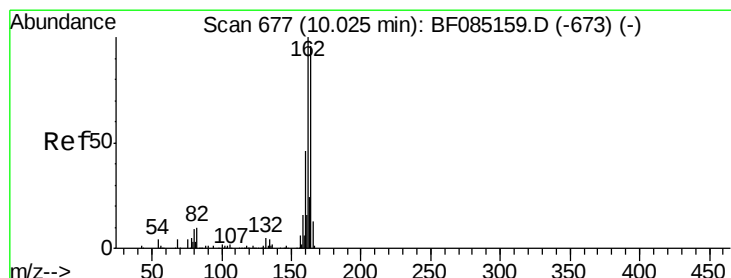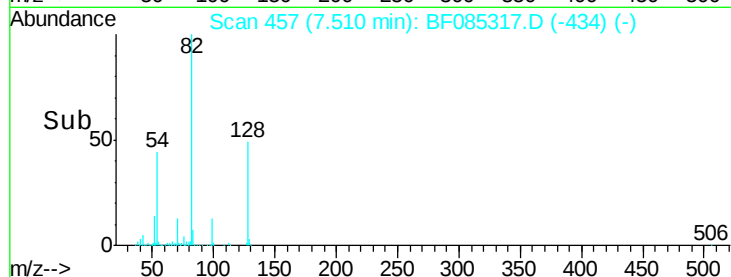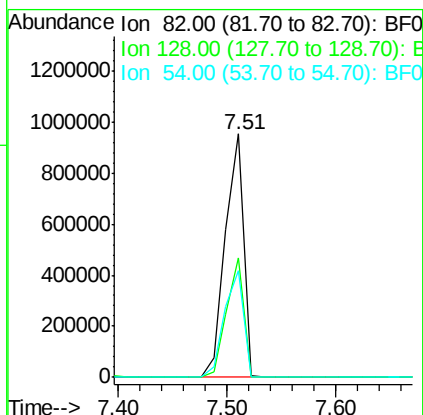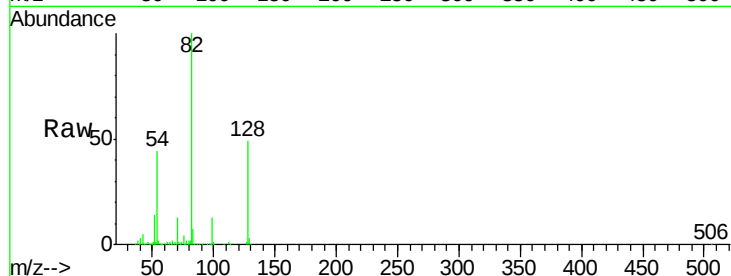

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.99 min Scan# 674
 Delta R.T. -0.03 min
 Lab File: BF085317.D
 Acq: 9 Mar 2016 23:58

Tgt Ion: 164 Resp: 323314
 Ion Ratio Lower Upper
 164 100
 162 103.2 83.3 124.9
 160 47.3 37.9 56.9

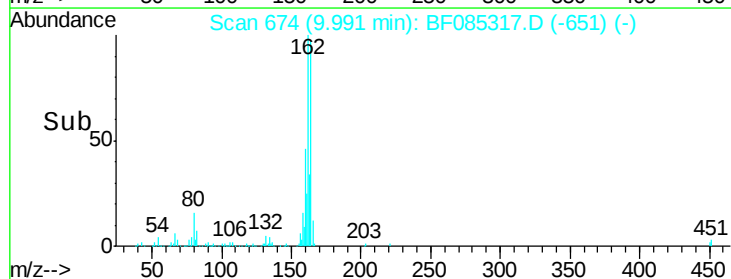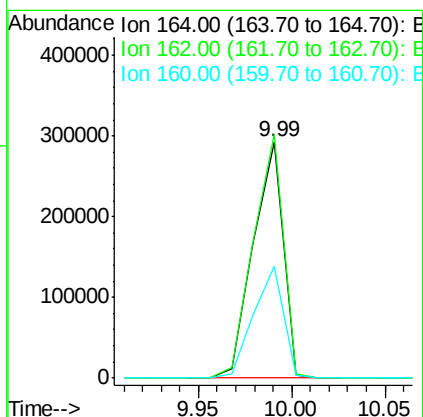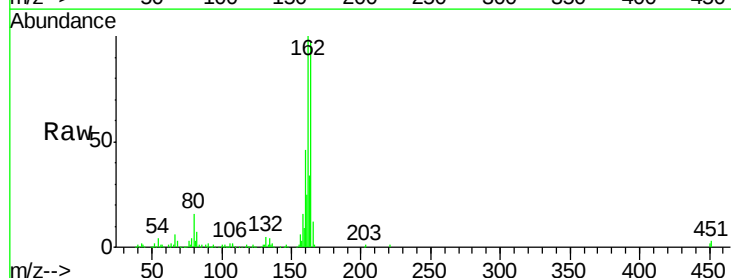


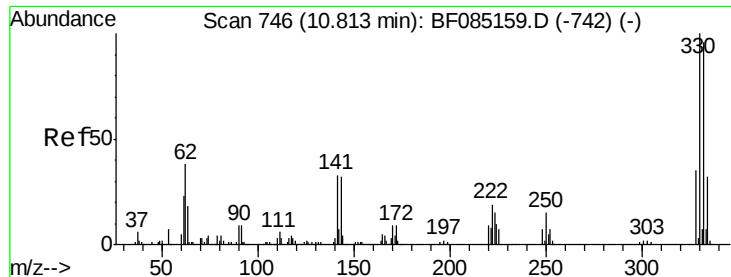




#41
 2,4,6-Tribromophenol
 Concen: 137.01 ng
 RT: 10.78 min Scan# 743
 Delta R.T. -0.03 min
 Lab File: BF085317.D
 Acq: 9 Mar 2016 23:58

Instrument :
 BNA_F
 ClientSampleId :
 UST-FD-3-8-16

Tgt Ion:330 Resp: 379036
 Ion Ratio Lower Upper
 330 100
 332 96.5 77.1 115.7
 141 37.1 35.0 52.6

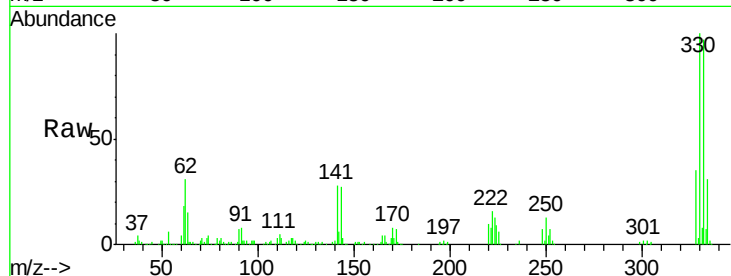


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

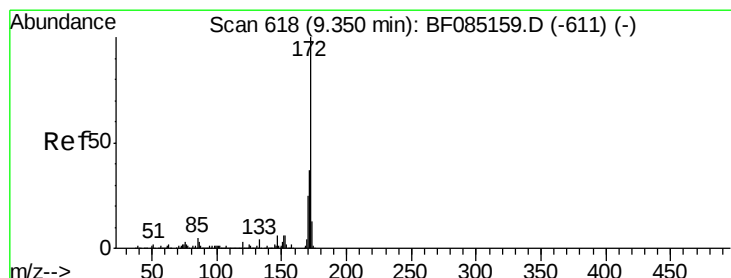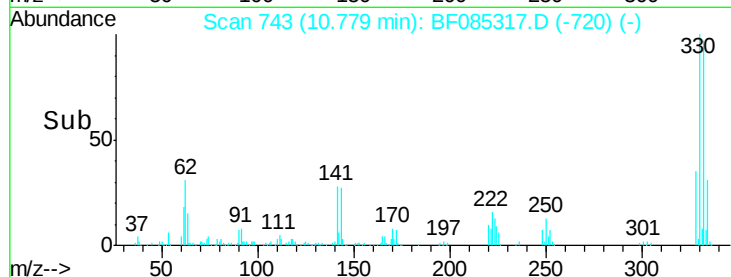
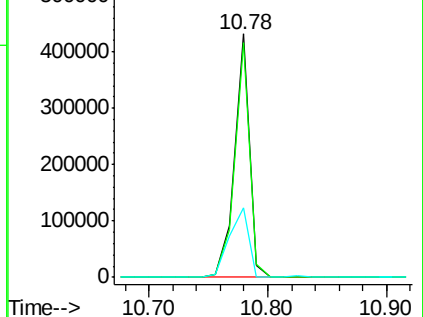



#44
 2-Fluorobiphenyl
 Concen: 73.88 ng
 RT: 9.30 min Scan# 614
 Delta R.T. -0.05 min
 Lab File: BF085317.D
 Acq: 9 Mar 2016 23:58

Tgt Ion:172 Resp: 1570647
 Ion Ratio Lower Upper
 172 100
 171 36.8 29.3 43.9
 170 24.8 20.0 30.0

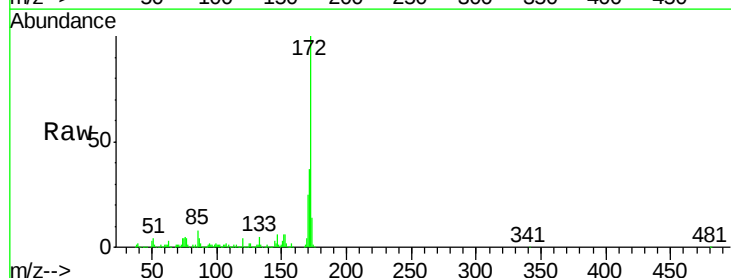

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

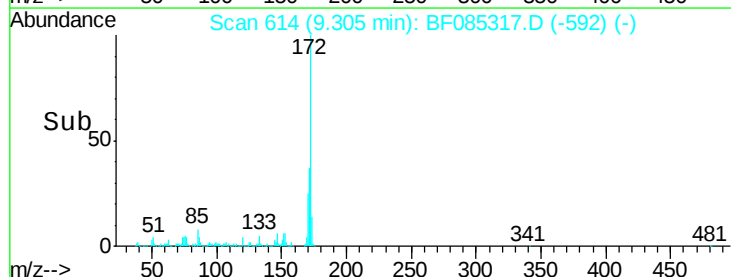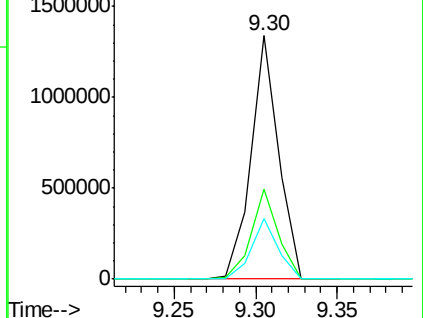

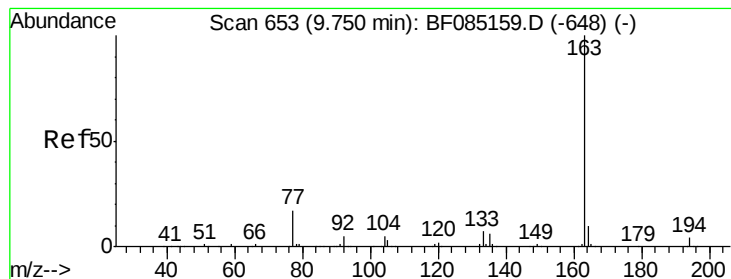

#49

Dimethylphthalate

Concen: 15.96 ng

RT: 9.70 min Scan# 649

Delta R.T. -0.05 min

Lab File: BF085317.D

Acq: 9 Mar 2016 23:58

Instrument :

BNA_F

ClientSampleId :

UST-FD-3-8-16


Tgt Ion:163 Resp: 395974

Ion Ratio Lower Upper

163 100

194 4.1 3.1 4.7




164 9.1 8.2 12.4

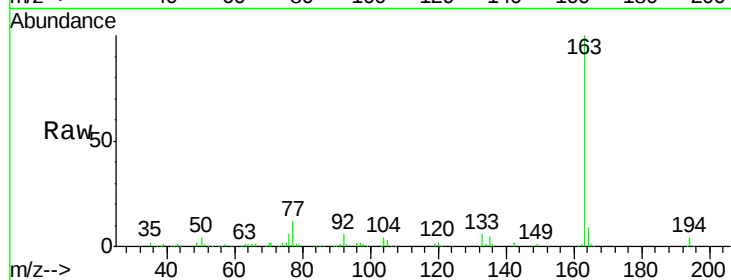

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

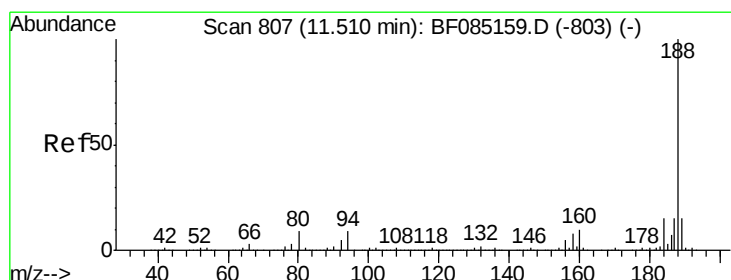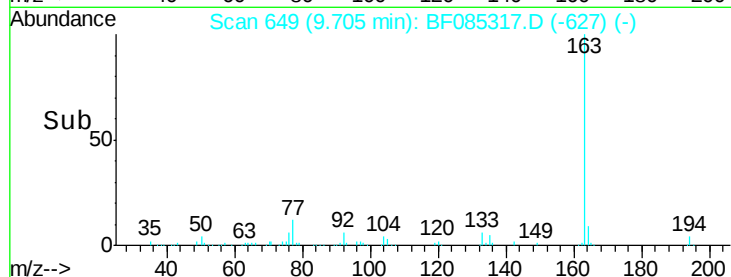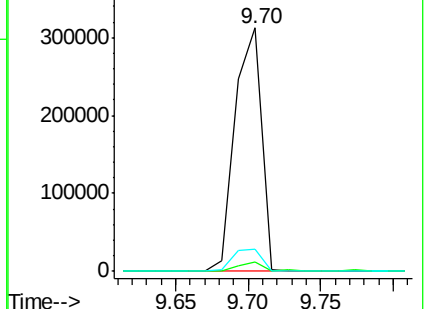

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.48 min Scan# 804

Delta R.T. -0.03 min

Lab File: BF085317.D

Acq: 9 Mar 2016 23:58


Tgt Ion:188 Resp: 581127

Ion Ratio Lower Upper

188 100

94 7.1 7.0 10.6



80 7.2 7.4 11.0#

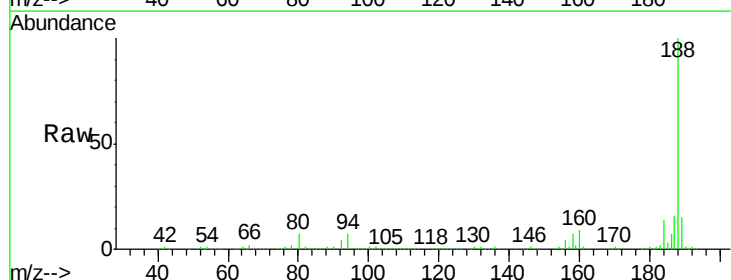


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

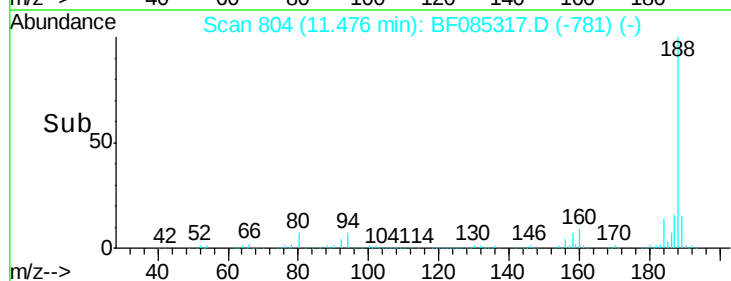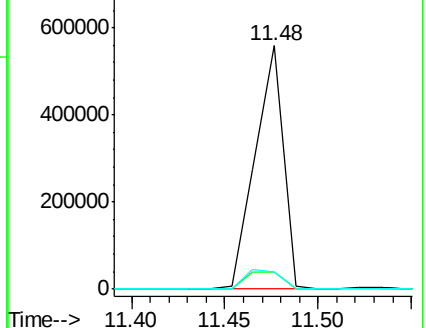

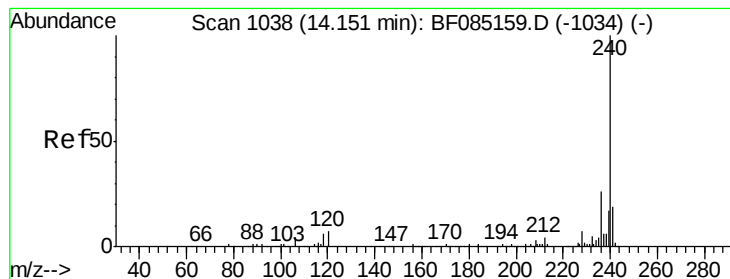

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.11 min Scan# 1034

Delta R.T. -0.05 min

Lab File: BF085317.D

Acq: 9 Mar 2016 23:58

Instrument :

BNA_F

ClientSampleId :

UST-FD-3-8-16


Tgt Ion:240 Resp: 379192

Ion Ratio Lower Upper

240 100

120 16.1 5.3 7.9#




236 25.9 20.7 31.1

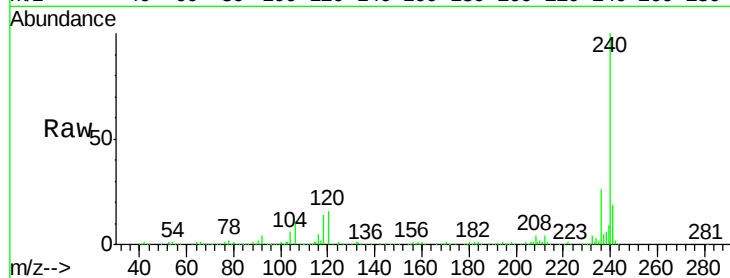

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

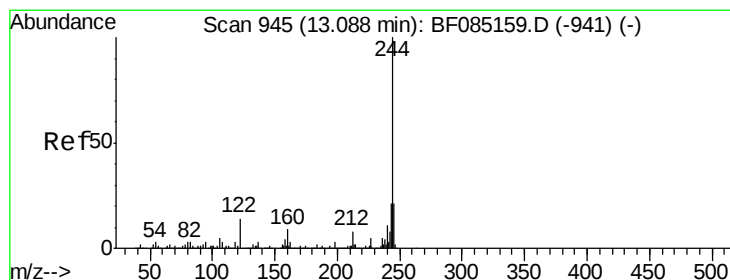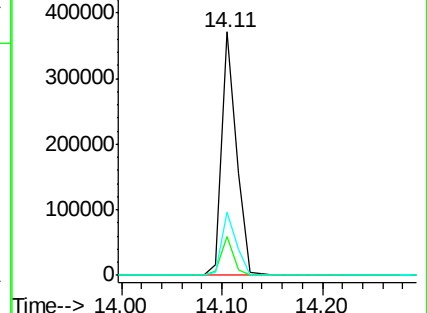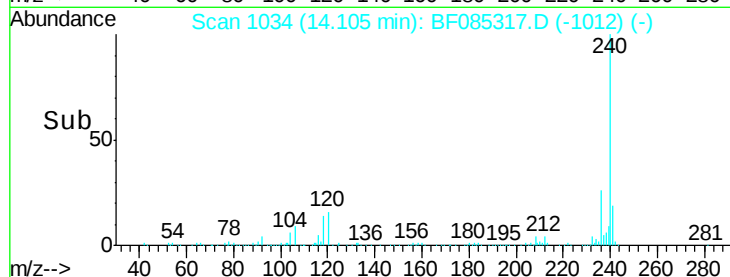

#78

Terphenyl-d14

Concen: 92.06 ng

RT: 13.07 min Scan# 943

Delta R.T. -0.02 min

Lab File: BF085317.D

Acq: 9 Mar 2016 23:58


Tgt Ion:244 Resp: 1503796

Ion Ratio Lower Upper

244 100

212 7.1 6.4 9.6



122 9.1 11.4 17.2#

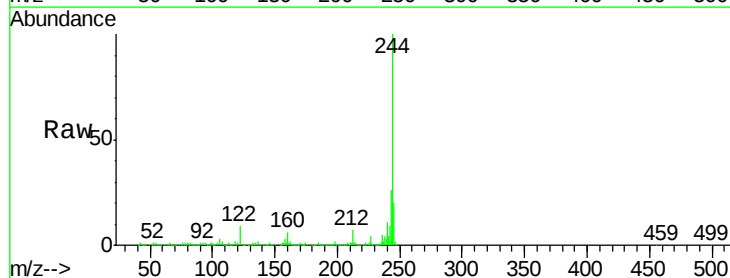


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

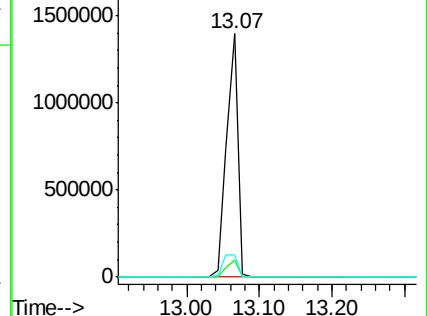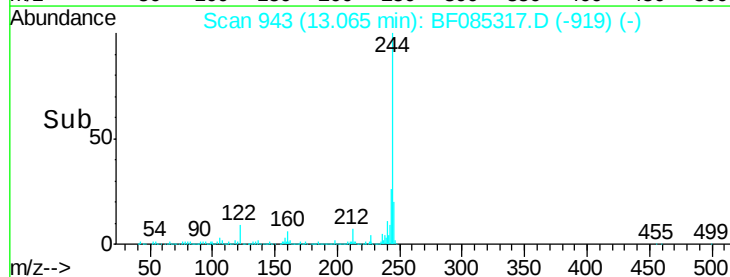


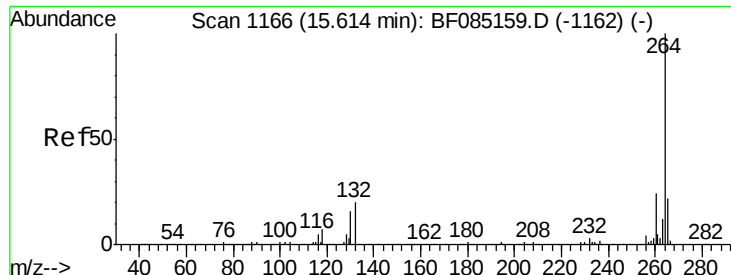

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.57 min Scan# 1162
Delta R.T. -0.05 min
Lab File: BF085317.D
Acq: 9 Mar 2016 23:58

Instrument :
BNA_F
ClientSampleId :
UST-FD-3-8-16

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.9	19.2	28.8
265	21.2	17.3	25.9

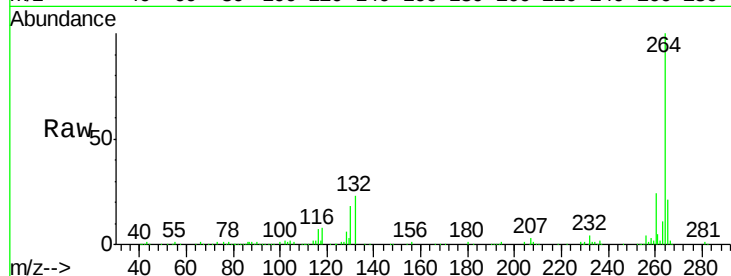

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

