


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030916\
 Data File : BF085299.D
 Acq On : 9 Mar 2016 14:06
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 04 00:54:58 2016

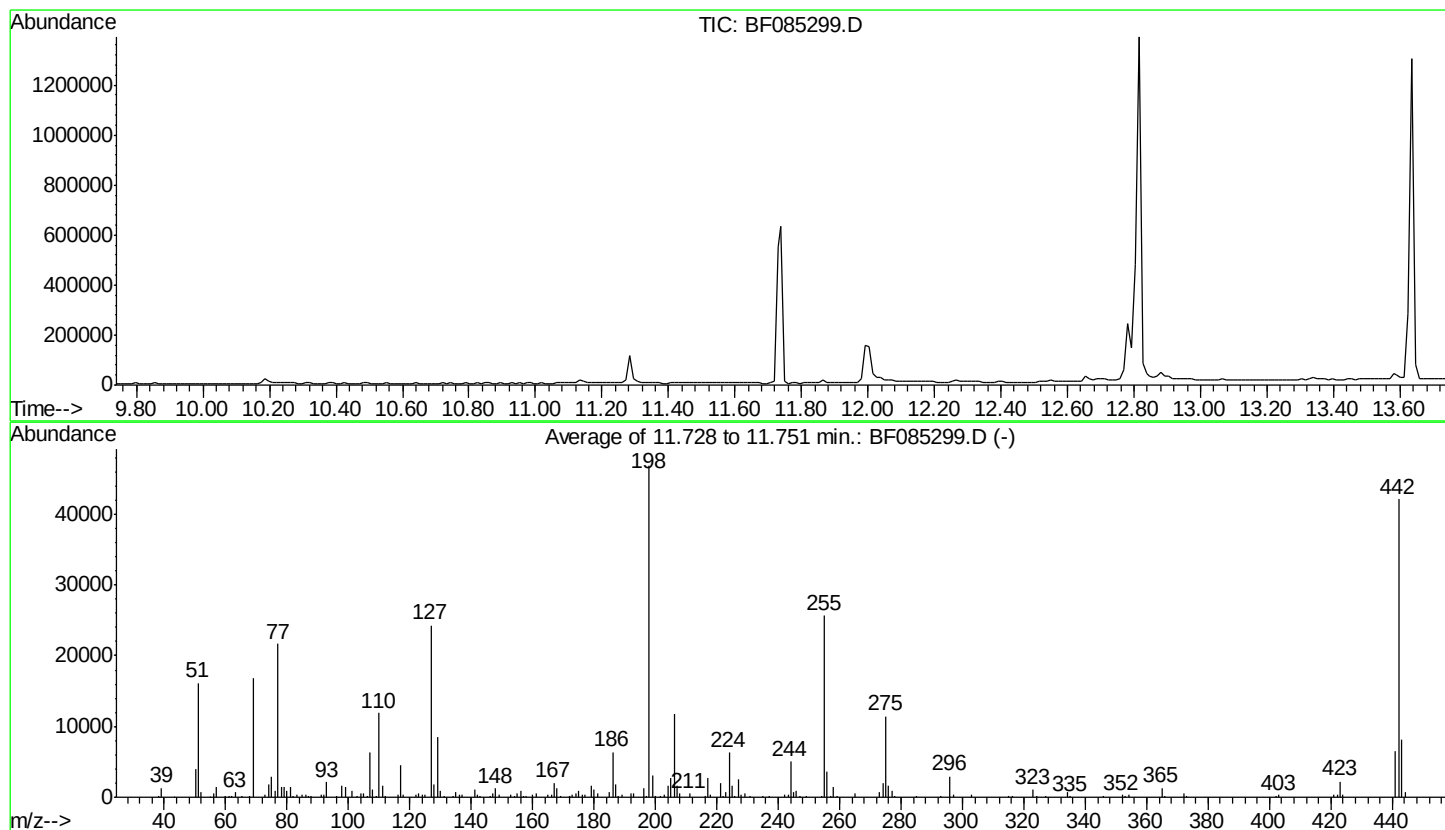

AutoFind: Scans 826, 827, 828; Background Corrected with Scan 822

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	16171	PASS
68	69	0.00	2	1.4	242	PASS
69	198	0.00	100	36.0	16890	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.9	24325	PASS
197	198	0.00	2	0.4	174	PASS
198	198	100	100	100.0	46870	PASS
199	198	5	9	6.4	2992	PASS
275	198	10	60	24.5	11490	PASS
365	198	1	100	2.8	1294	PASS
441	442	0.01	24	15.5	6510	PASS
442	198	50	100	89.9	42127	PASS
443	442	15	24	19.4	8165	PASS