
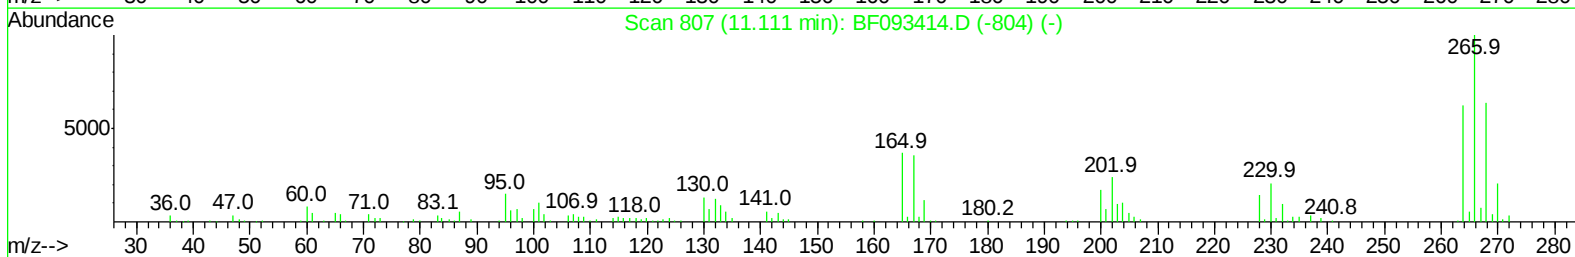
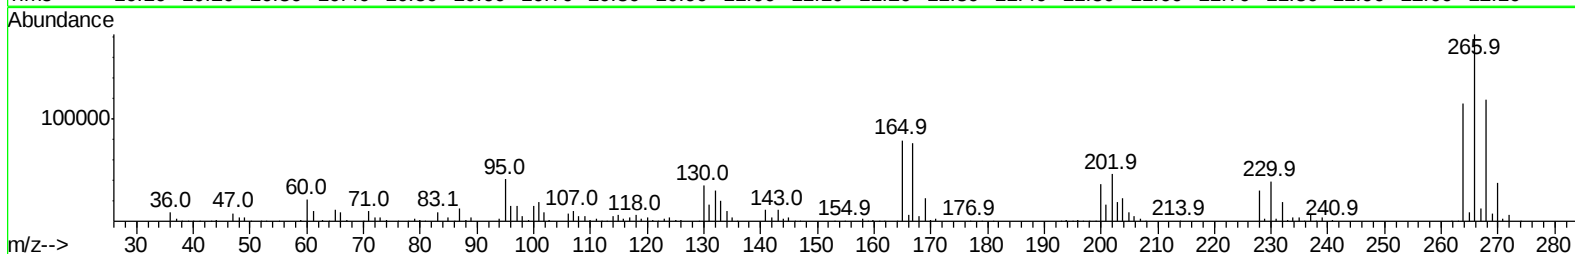


Data Path : Z:\HPCHEM1\BNA F\DATA\BF030917\
Data File : BF093481.D
Acq On : 9 Mar 2017 17:27
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 06:14:17 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 15:55:22 2017
Response via : Initial Calibration

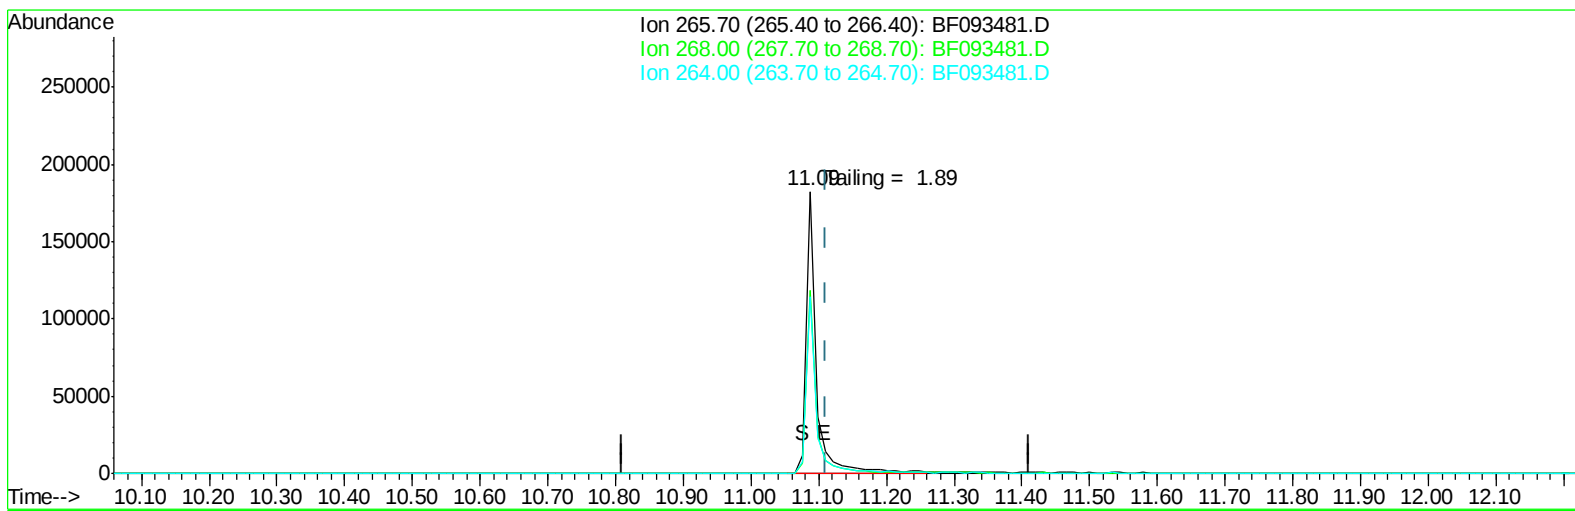

TIC: BF093481.D

(69) Pentachlorophenol (C)




11.088min (-0.023) 64077.53ng

response 189435

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	65.04
264.00	62.90	62.94
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030917\
Data File : BF093481.D
Acq On : 9 Mar 2017 17:27
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 06:14:17 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 15:55:22 2017
Response via : Initial Calibration

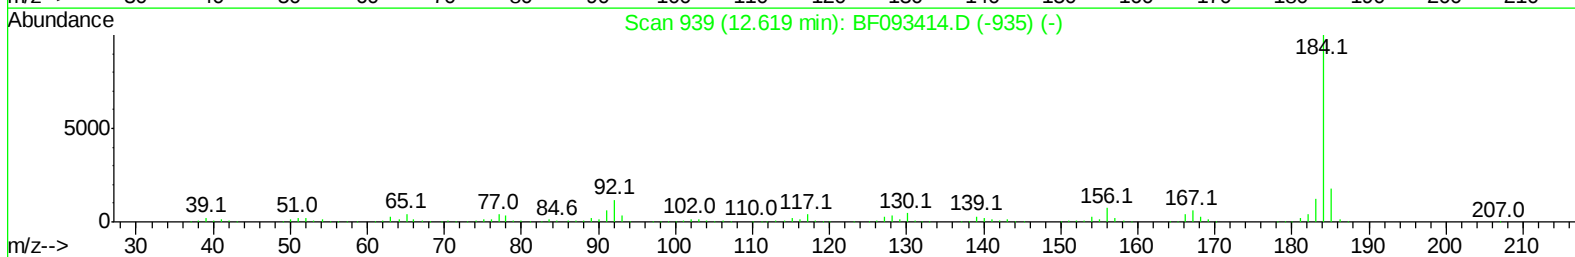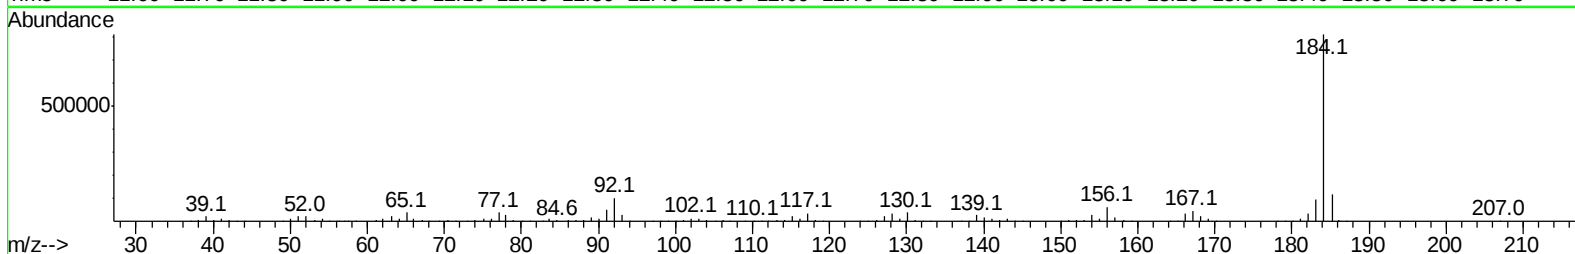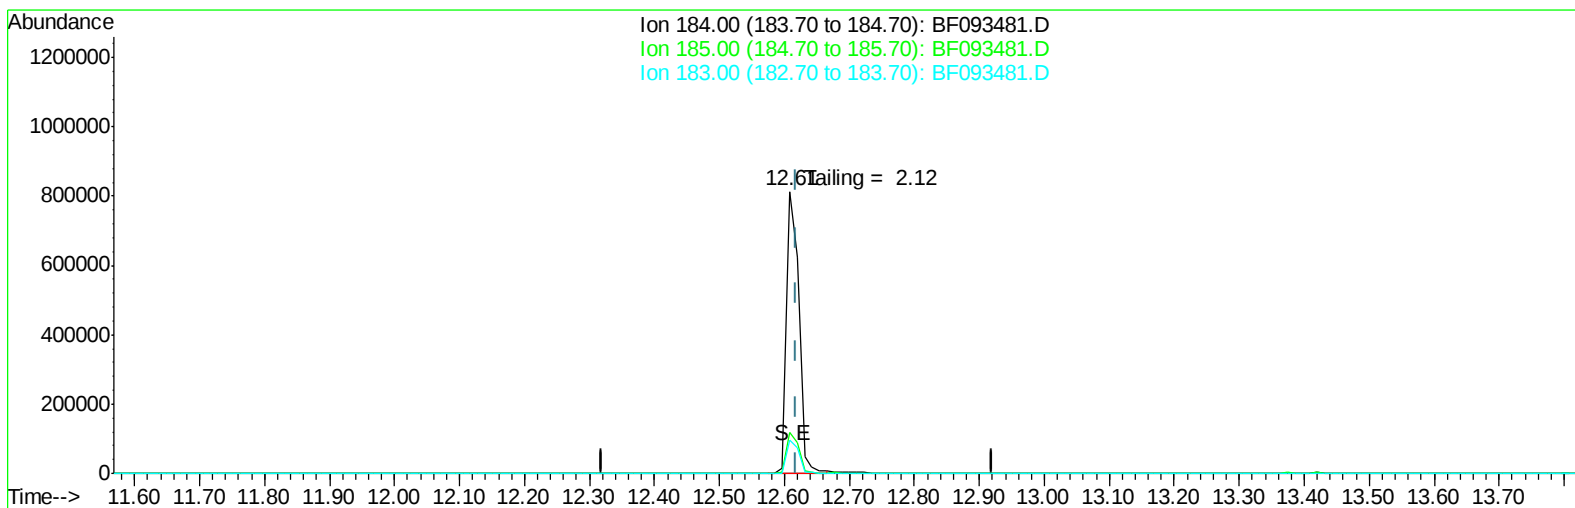

TIC: BF093481.D

(76) Benzidine

12.608min (-0.011) 0.00ng

response 1068793

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.52
183.00	11.50	11.64
0.00	0.00	0.00