
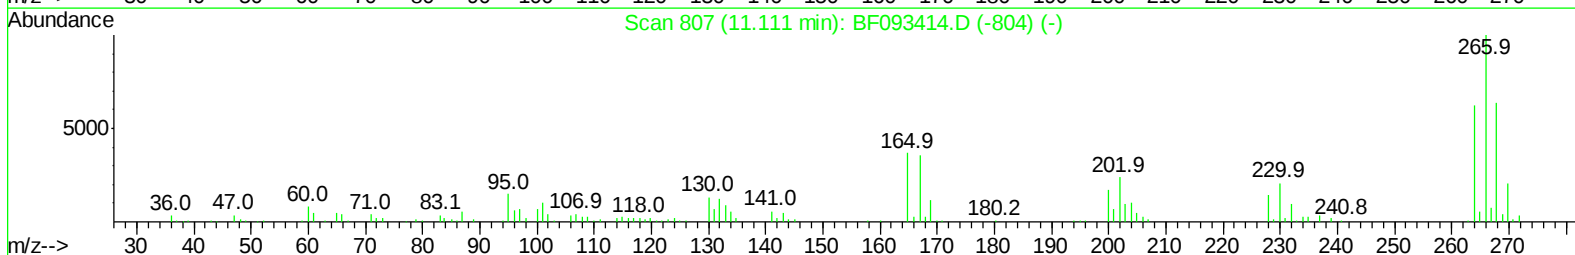
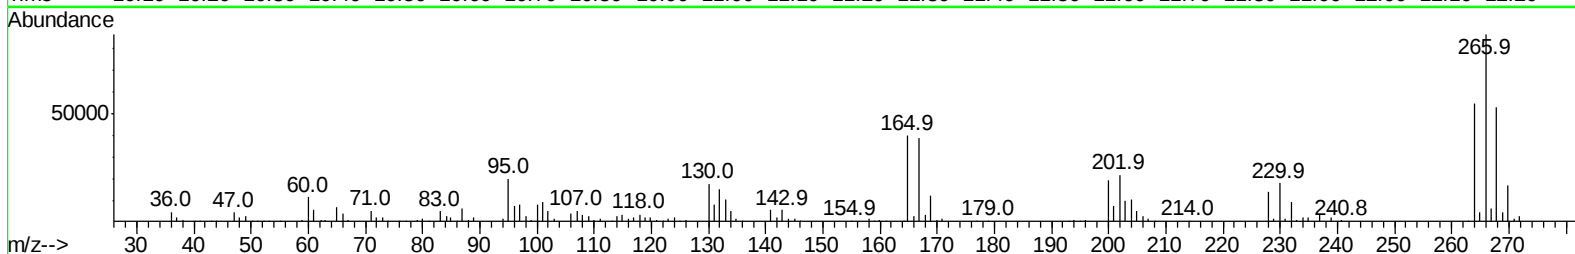


Data Path : Z:\HPCHEM1\BNA F\DATA\BF030917\
Data File : BF093507.D
Acq On : 10 Mar 2017 6:48
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 07:13:15 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 15:55:22 2017
Response via : Initial Calibration

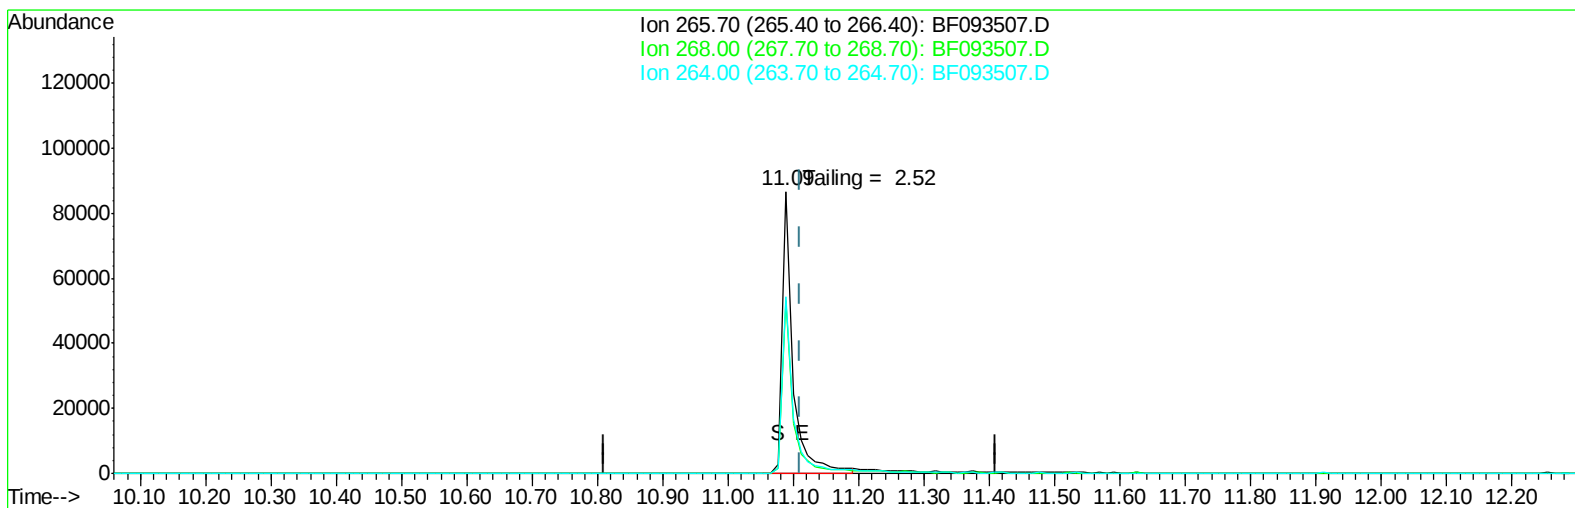

TIC: BF093507.D

(69) Pentachlorophenol (C)




11.088min (-0.023) 60693.47ng

response 103892

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	61.24
264.00	62.90	62.93
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030917\
Data File : BF093507.D
Acq On : 10 Mar 2017 6:48
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 07:13:15 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 15:55:22 2017
Response via : Initial Calibration

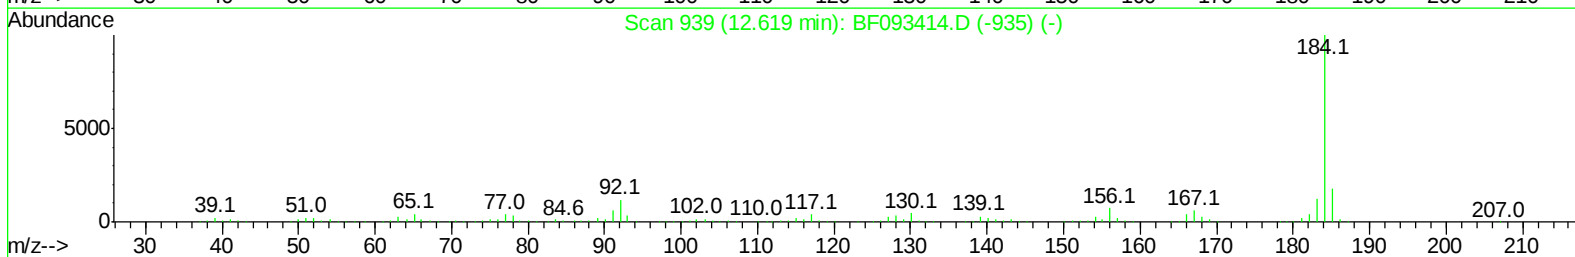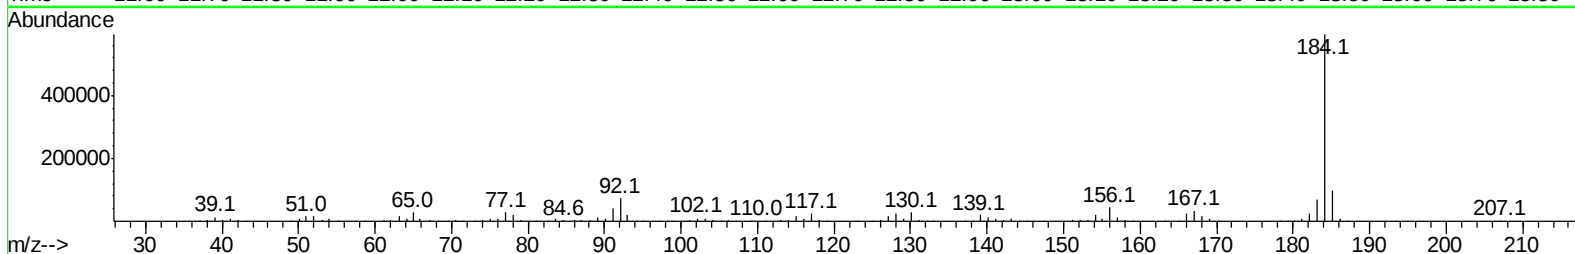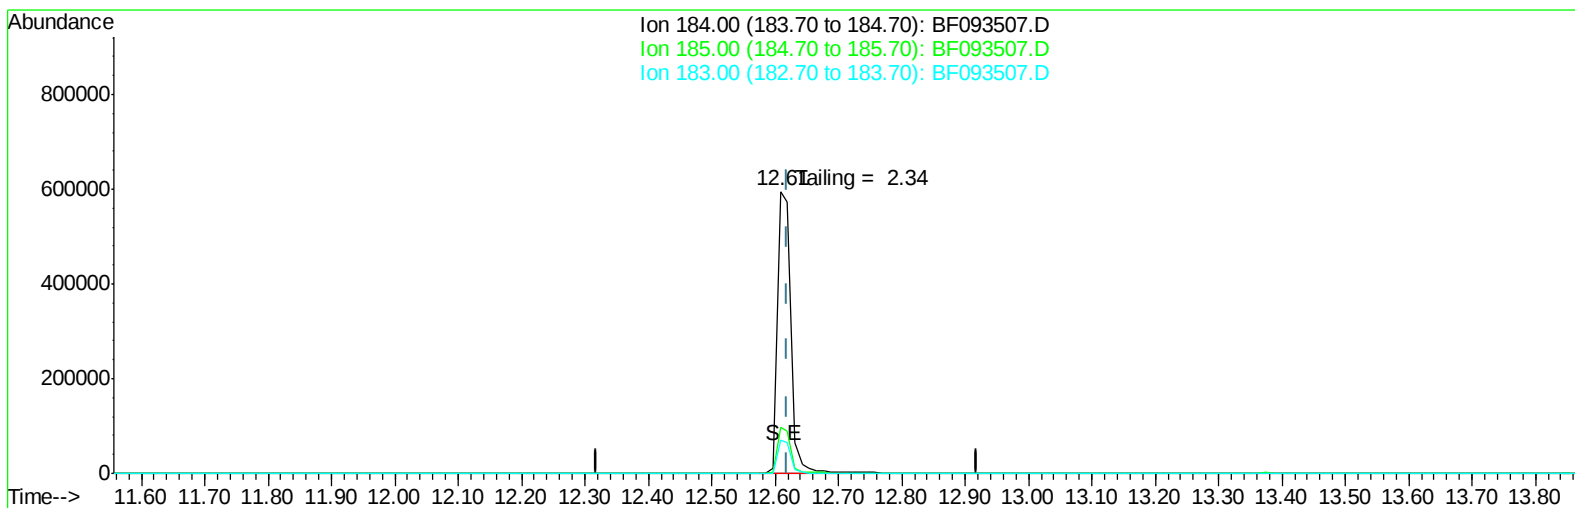

TIC: BF093507.D

(76) Benzidine

12.608min (-0.011) 0.00ng

response 899893

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	16.57
183.00	11.50	11.72
0.00	0.00	0.00