


Data Path : Z:\HPCHEM1\BNA F\DATA\BF030917\
 Data File : BF093481.D
 Acq On : 9 Mar 2017 17:27
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 07 15:55:22 2017

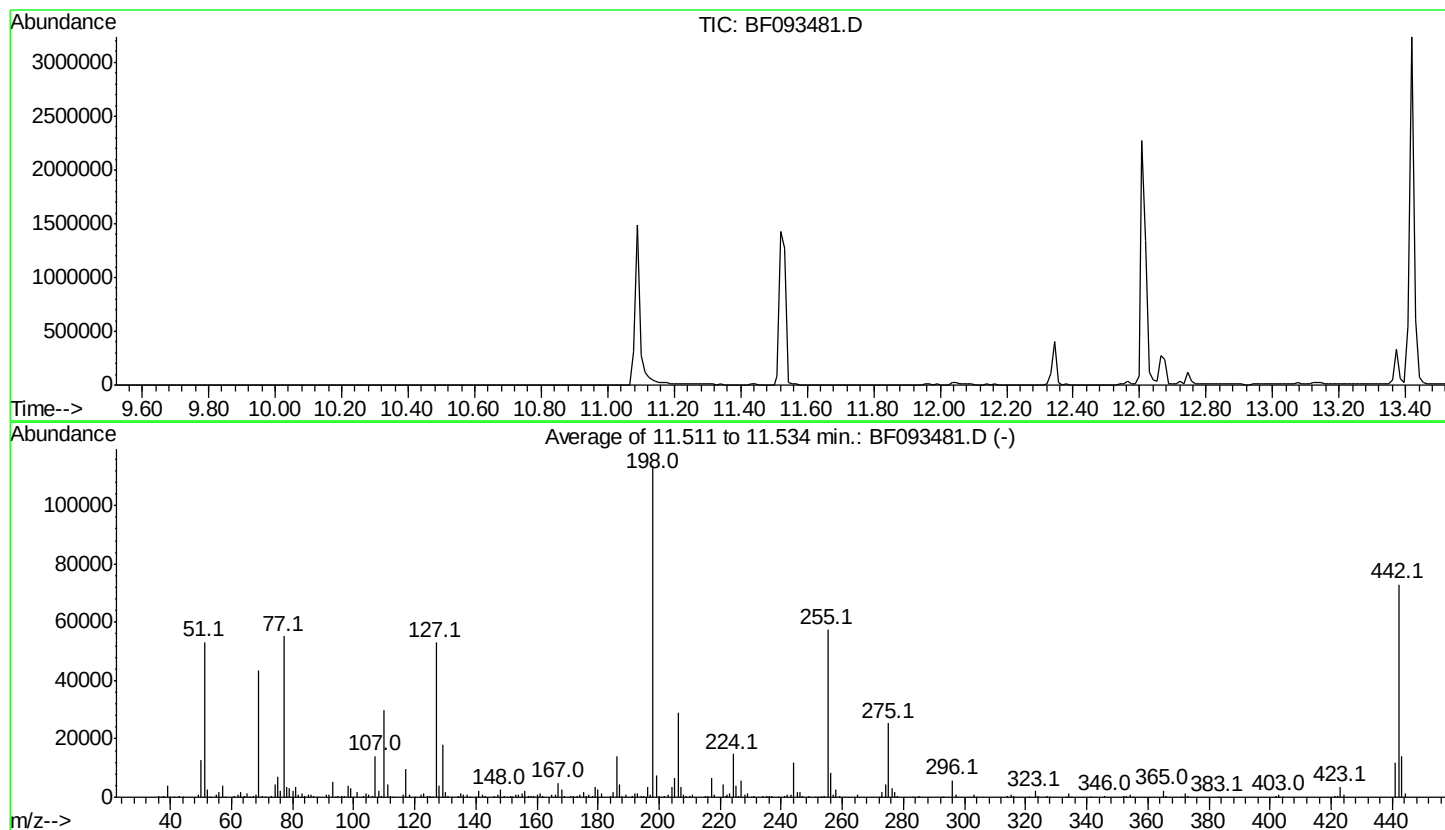

AutoFind: Scans 842, 843, 844; Background Corrected with Scan 839

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.7	53133	PASS
68	69	0.00	2	1.9	820	PASS
69	198	0.00	100	38.3	43527	PASS
70	69	0.00	2	0.9	388	PASS
127	198	10	80	46.5	52909	PASS
197	198	0.00	2	0.9	1038	PASS
198	198	100	100	100.0	113691	PASS
199	198	5	9	6.5	7364	PASS
275	198	10	60	22.3	25342	PASS
365	198	1	100	2.0	2283	PASS
441	442	0.01	24	16.1	11796	PASS
442	198	50	100	64.3	73072	PASS
443	442	15	24	19.3	14070	PASS