


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030917\
 Data File : BF093507.D
 Acq On : 10 Mar 2017 6:48
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 07 15:55:22 2017

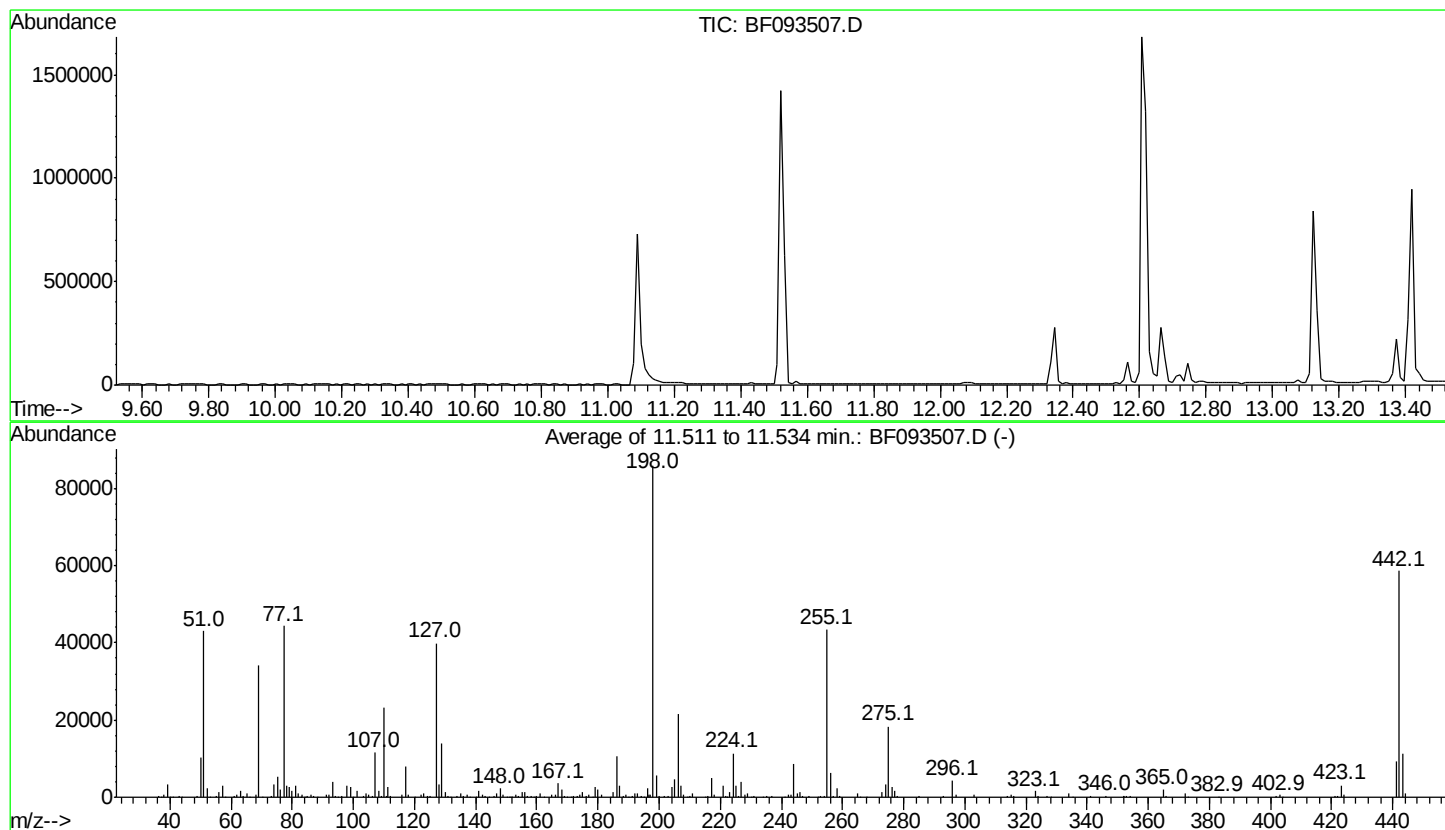

AutoFind: Scans 842, 843, 844; Background Corrected with Scan 839

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.1	43062	PASS
68	69	0.00	2	1.5	520	PASS
69	198	0.00	100	39.9	34258	PASS
70	69	0.00	2	0.5	155	PASS
127	198	10	80	46.5	39936	PASS
197	198	0.00	2	0.8	705	PASS
198	198	100	100	100.0	85882	PASS
199	198	5	9	6.6	5684	PASS
275	198	10	60	21.3	18316	PASS
365	198	1	100	2.2	1855	PASS
441	442	0.01	24	15.8	9263	PASS
442	198	50	100	68.2	58612	PASS
443	442	15	24	19.0	11133	PASS