
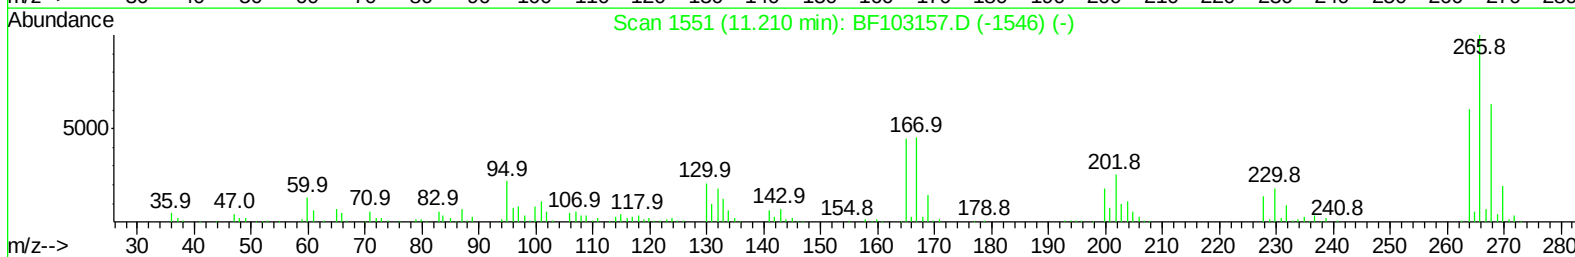
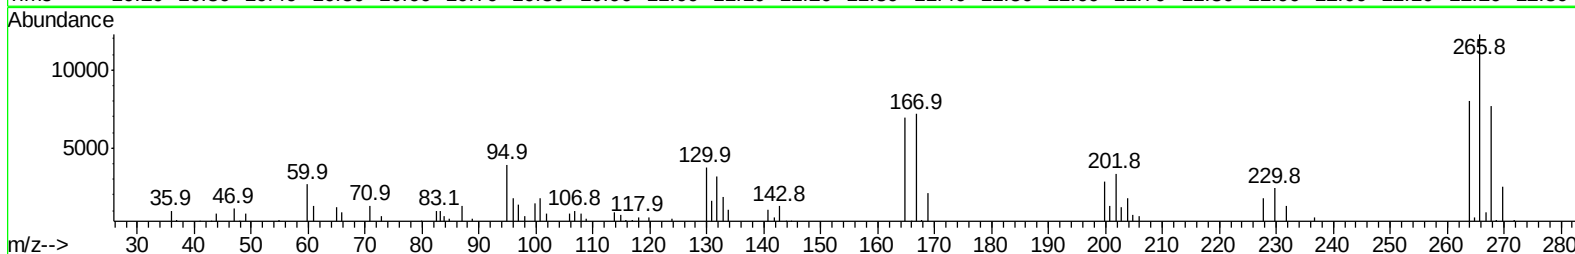


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF030918\
Data File : BF103550.D
Acq On : 9 Mar 2018 9:53
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 09 22:47:53 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 09 11:47:13 2018
Response via : Initial Calibration

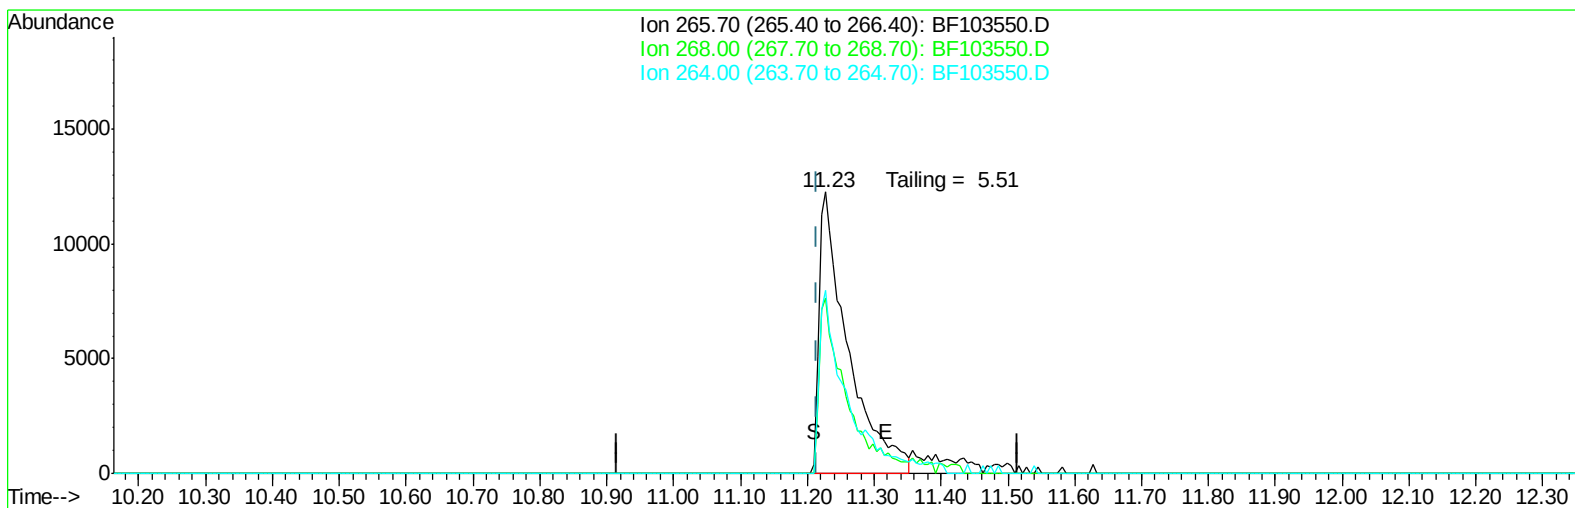

TIC: BF103550.D

(69) Pentachlorophenol (C)




11.228min (+0.012) 23380.05ng

response 36428

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.36
264.00	61.90	65.09
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF030918\
Data File : BF103550.D
Acq On : 9 Mar 2018 9:53
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 09 22:47:53 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 09 11:47:13 2018
Response via : Initial Calibration

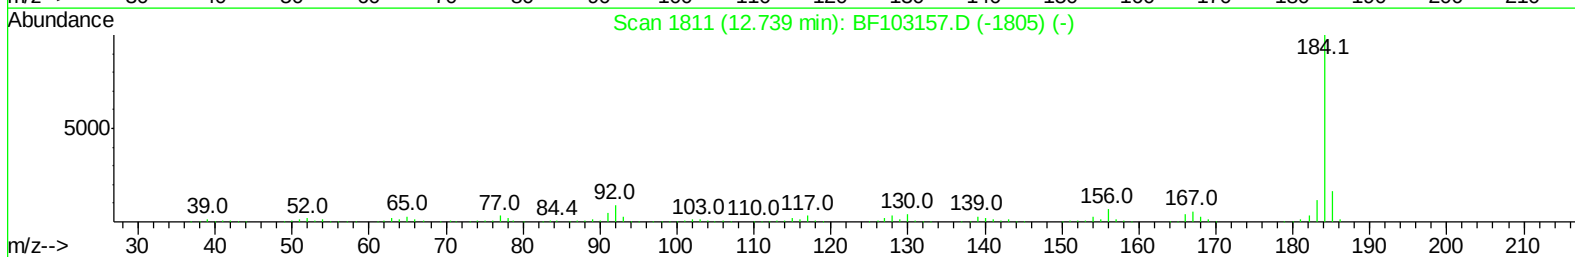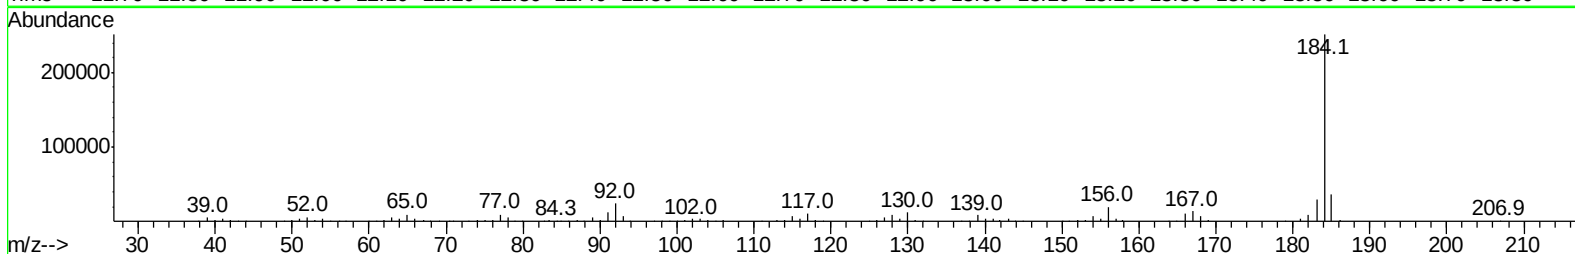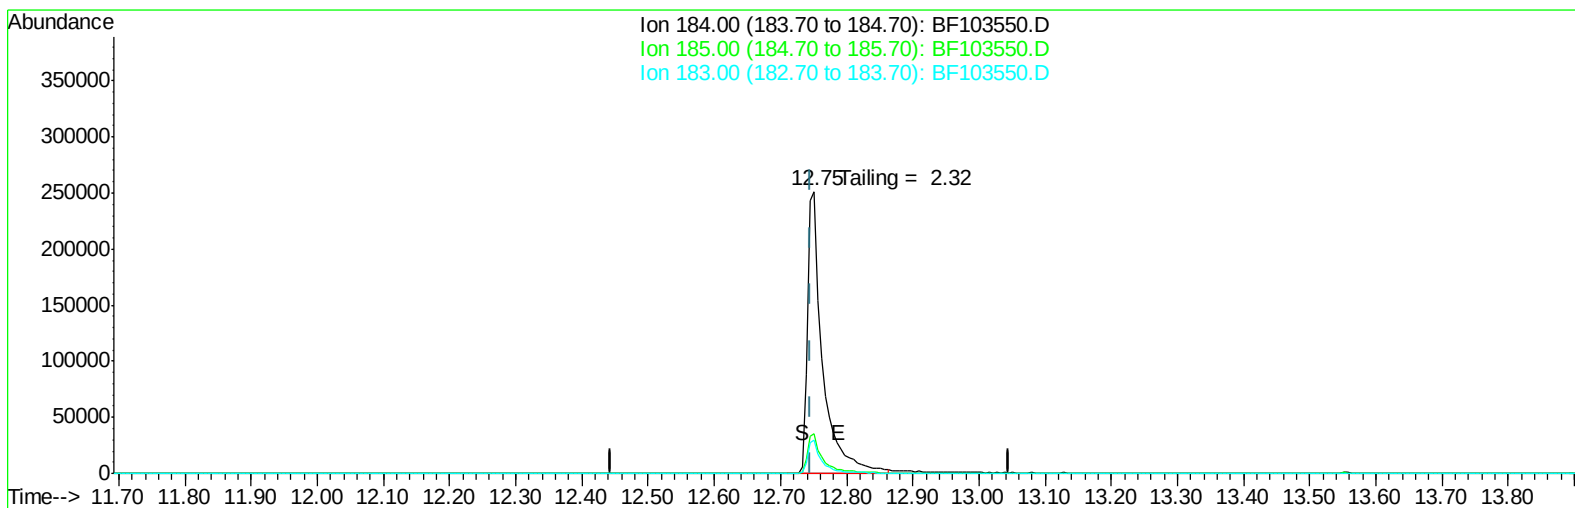

TIC: BF103550.D

(76) Benzidine

12.751min (+0.006) 0.00ng

response 409378

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.32
183.00	11.60	11.63
0.00	0.00	0.00