


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF030918\
 Data File : BF103550.D
 Acq On : 9 Mar 2018 9:53
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 09 11:47:13 2018

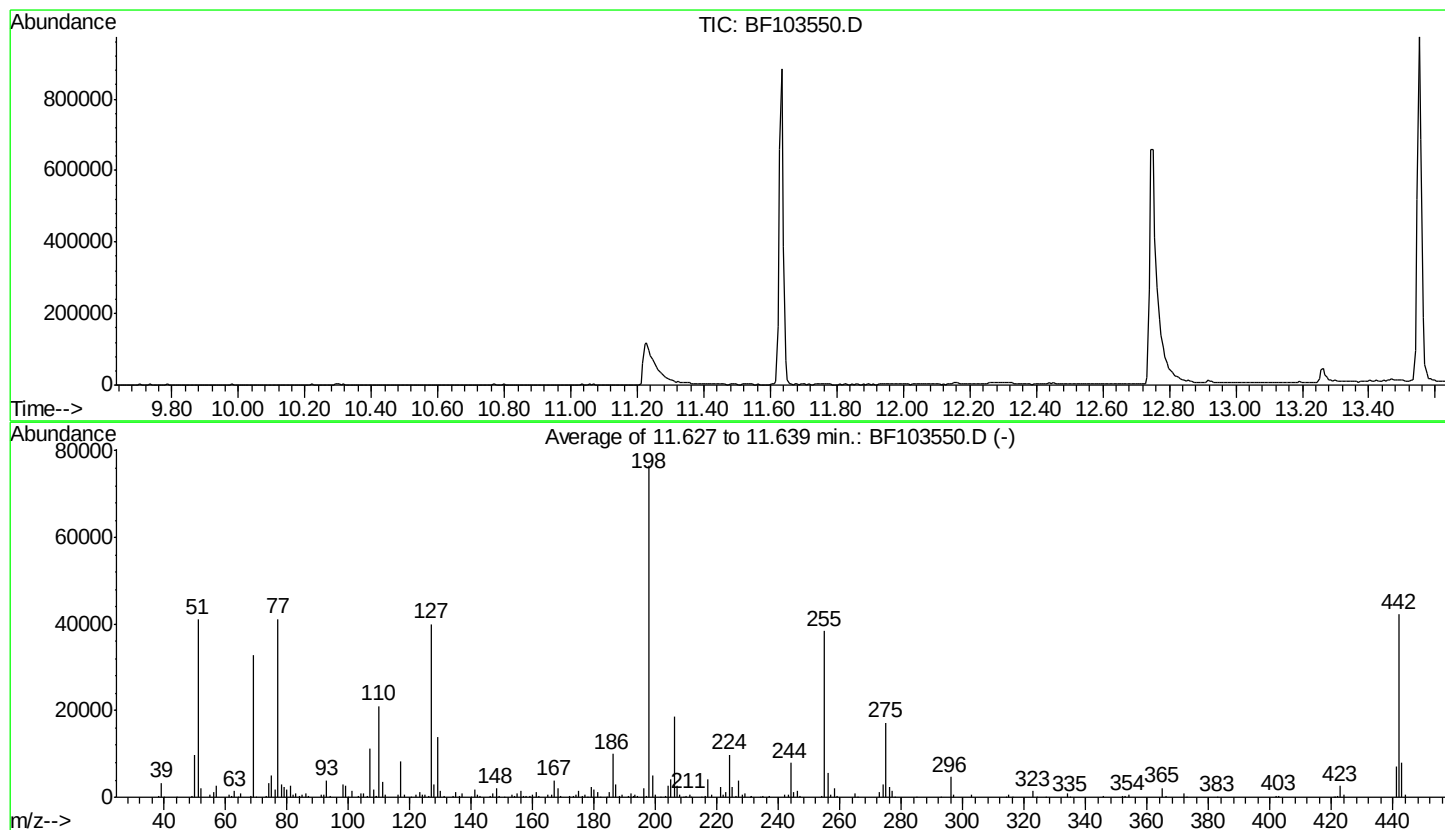

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.5	40992	PASS
68	69	0.00	2	1.4	455	PASS
69	198	0.00	100	43.0	32943	PASS
70	69	0.00	2	0.4	129	PASS
127	198	10	80	52.1	39938	PASS
197	198	0.00	2	0.5	417	PASS
198	198	100	100	100.0	76594	PASS
199	198	5	9	6.7	5153	PASS
275	198	10	60	22.5	17256	PASS
365	198	1	100	2.8	2168	PASS
441	443	0.01	100	86.5	7028	PASS
442	198	50	100	55.2	42248	PASS
443	442	15	24	19.2	8128	PASS