
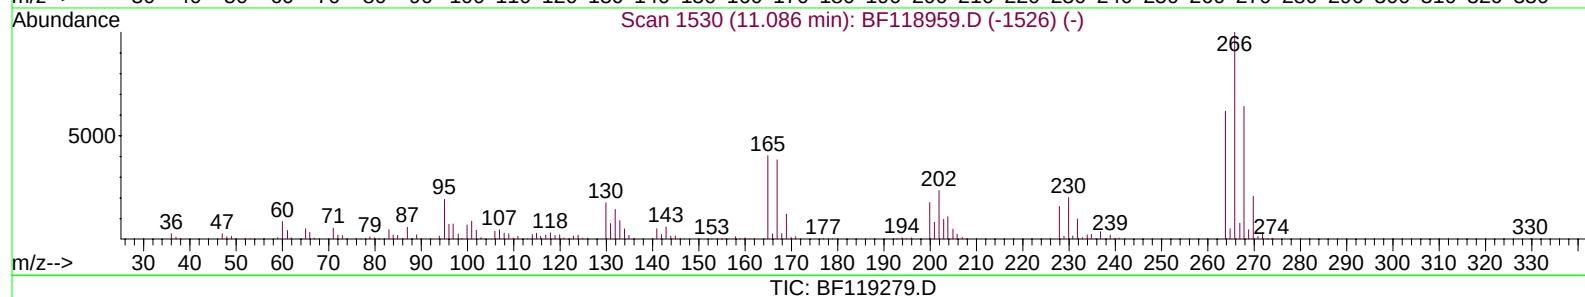
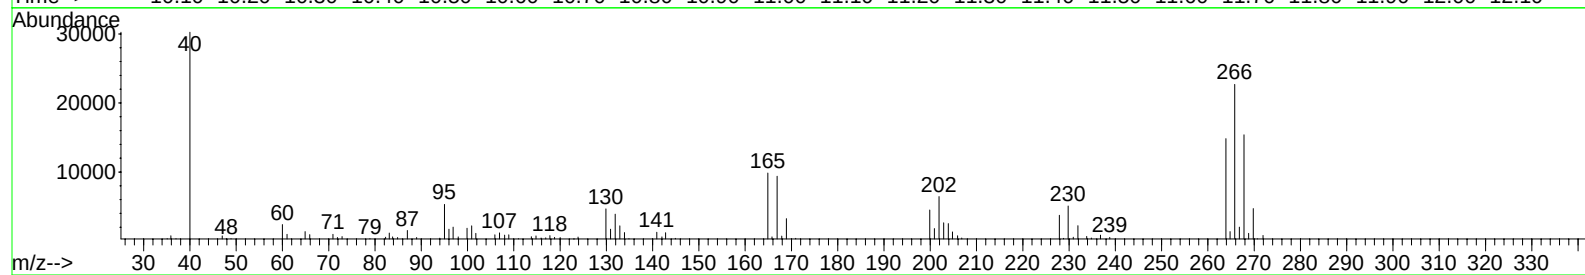


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF030920\
Data File : BF119279.D
Acq On : 9 Mar 2020 9:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 19:14:43 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 06 23:38:46 2020
Response via : Initial Calibration

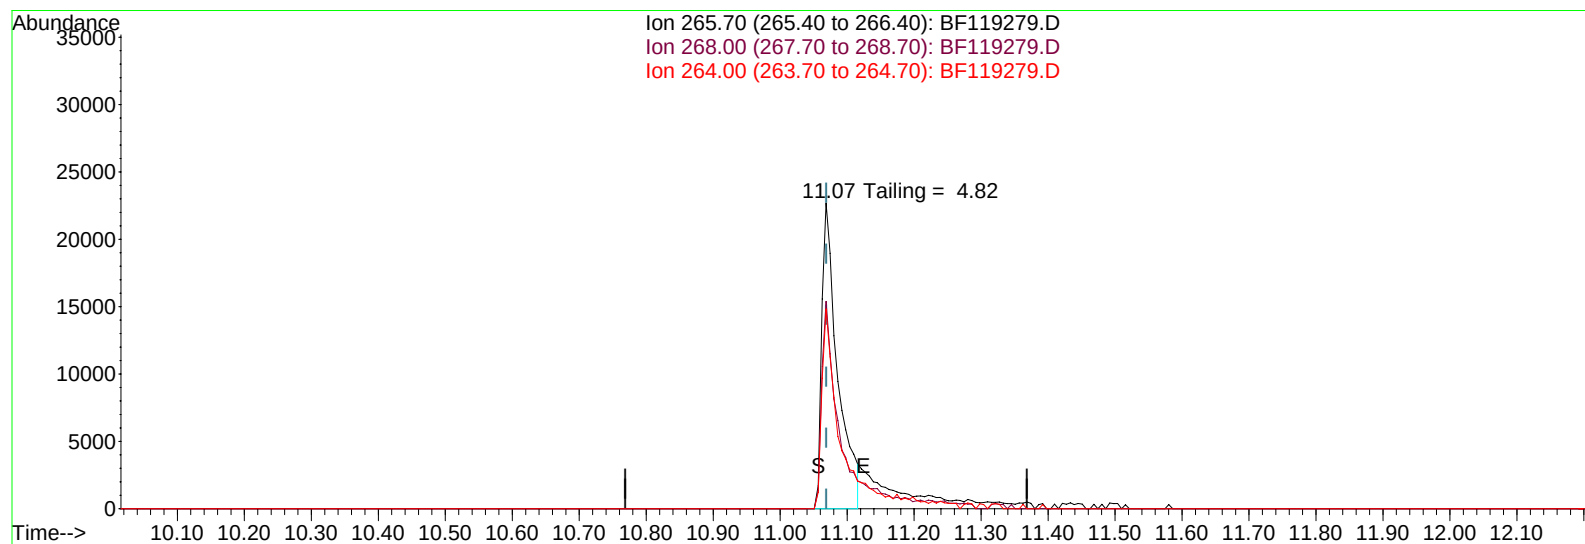

(70) Pentachlorophenol (C)




11.069min (+0.000) 28074.18ng

response 46187

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	67.81
264.00	63.70	65.35
0.00	0.00	0.00

```
Data Path   : Z:\svoasrv\HPCHEM1\BNA F\Data\BF030920\  
Data File   : BF119279.D  
Acq On      : 9 Mar 2020    9:29  
Operator    : CG/JU  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Mar 10 19:14:43 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 06 23:38:46 2020
Response via : Initial Calibration

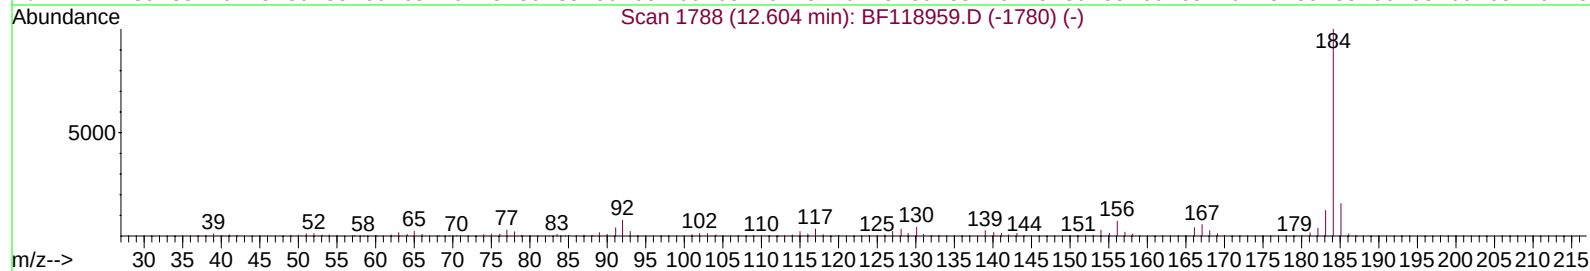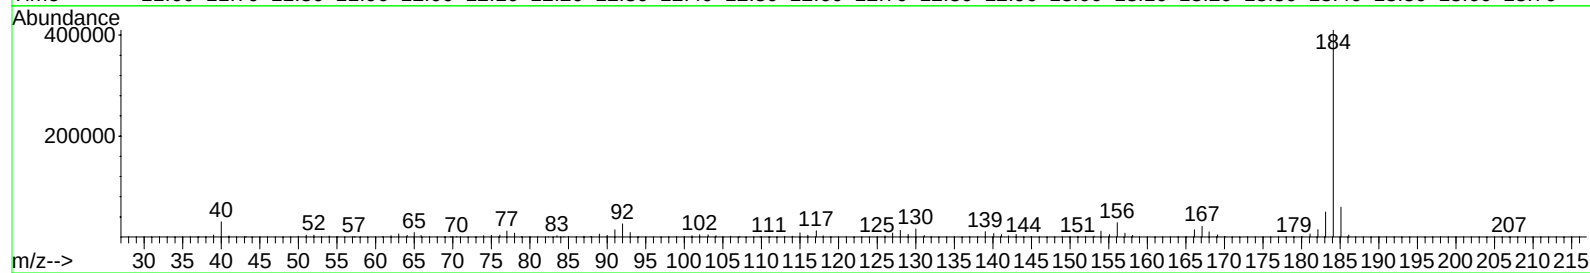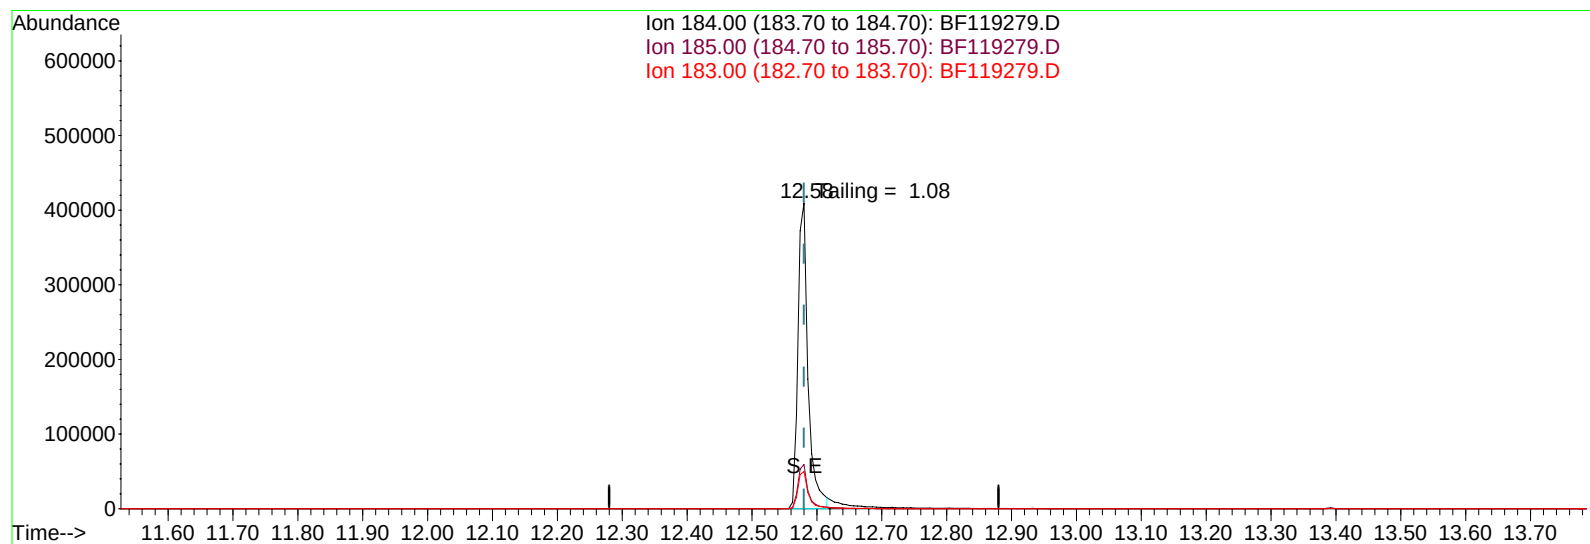

TIC: BF119279.D

(77) Benzidine

12.580min (+0.000) 0.00ng

response 475328

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.44
183.00	12.40	12.15
0.00	0.00	0.00