
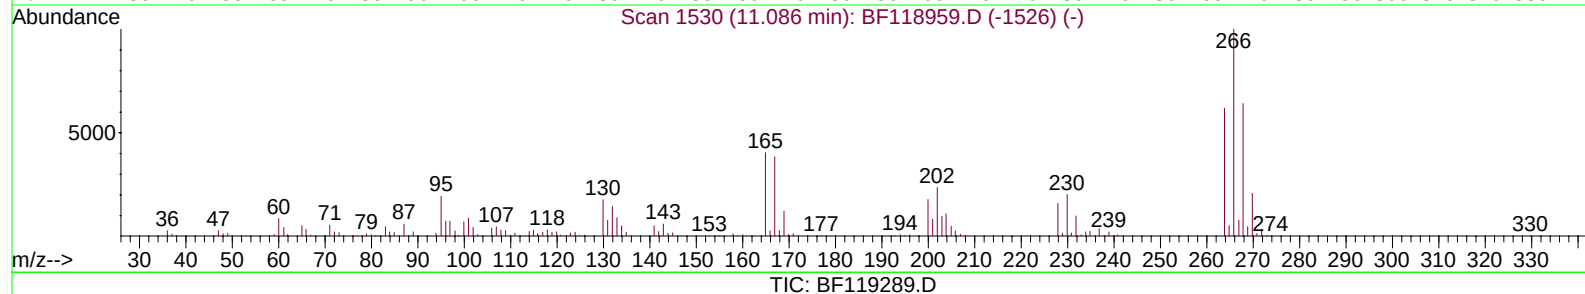
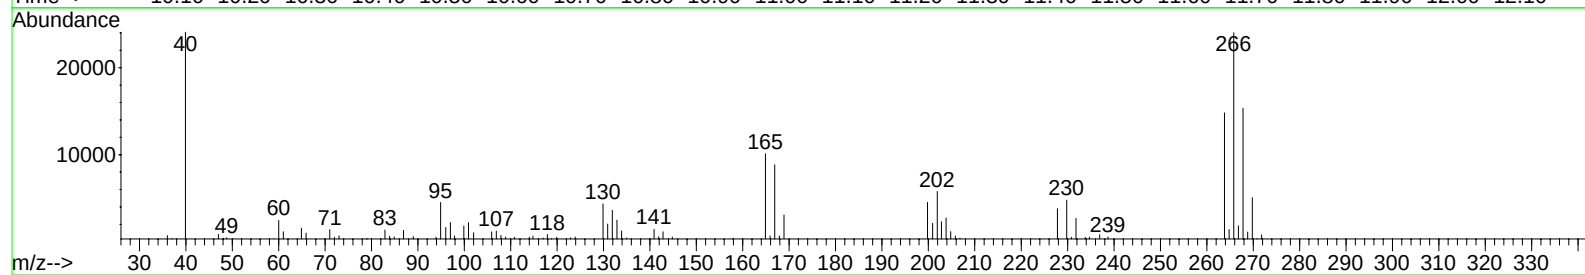


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF030920\
Data File : BF119289.D
Acq On : 9 Mar 2020 16:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 19:16:04 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 06 23:38:46 2020
Response via : Initial Calibration

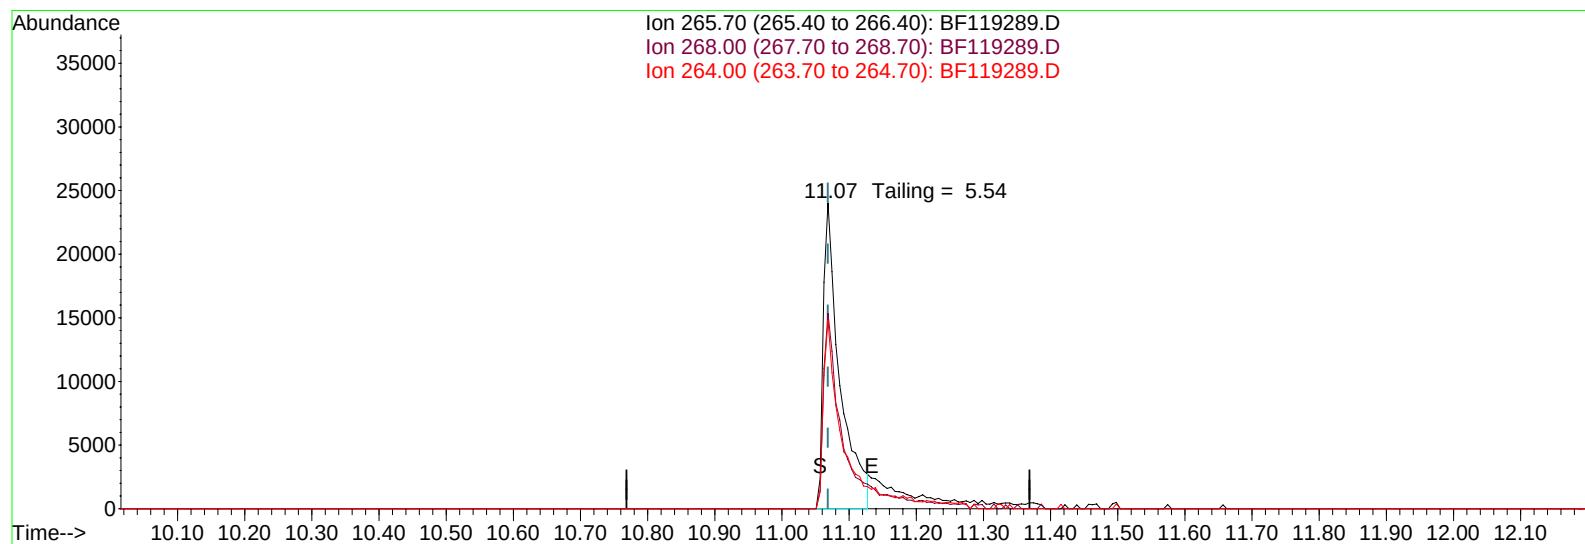

(70) Pentachlorophenol (C)




11.069min (+0.000) 17224.03ng

response 48099

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	63.89
264.00	63.70	61.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF030920\
 Data File : BF119289.D
 Acq On : 9 Mar 2020 16:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 19:16:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF022020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 06 23:38:46 2020
 Response via : Initial Calibration

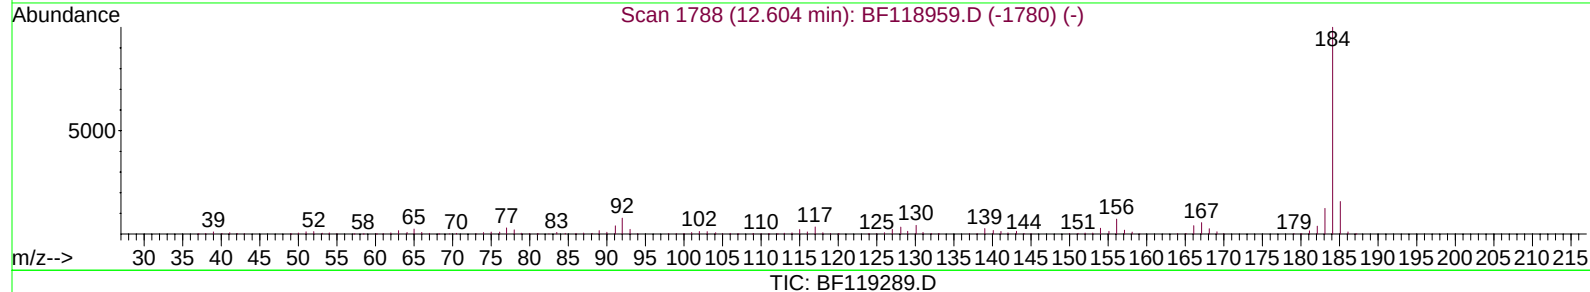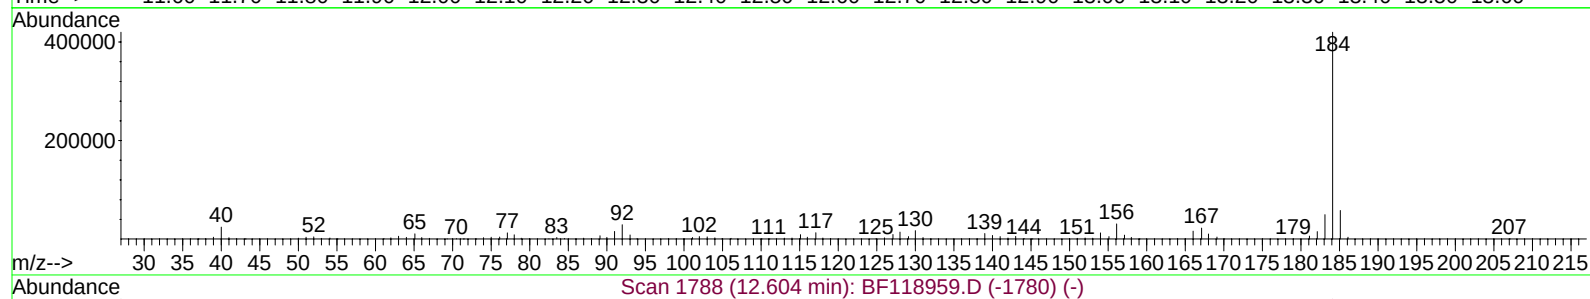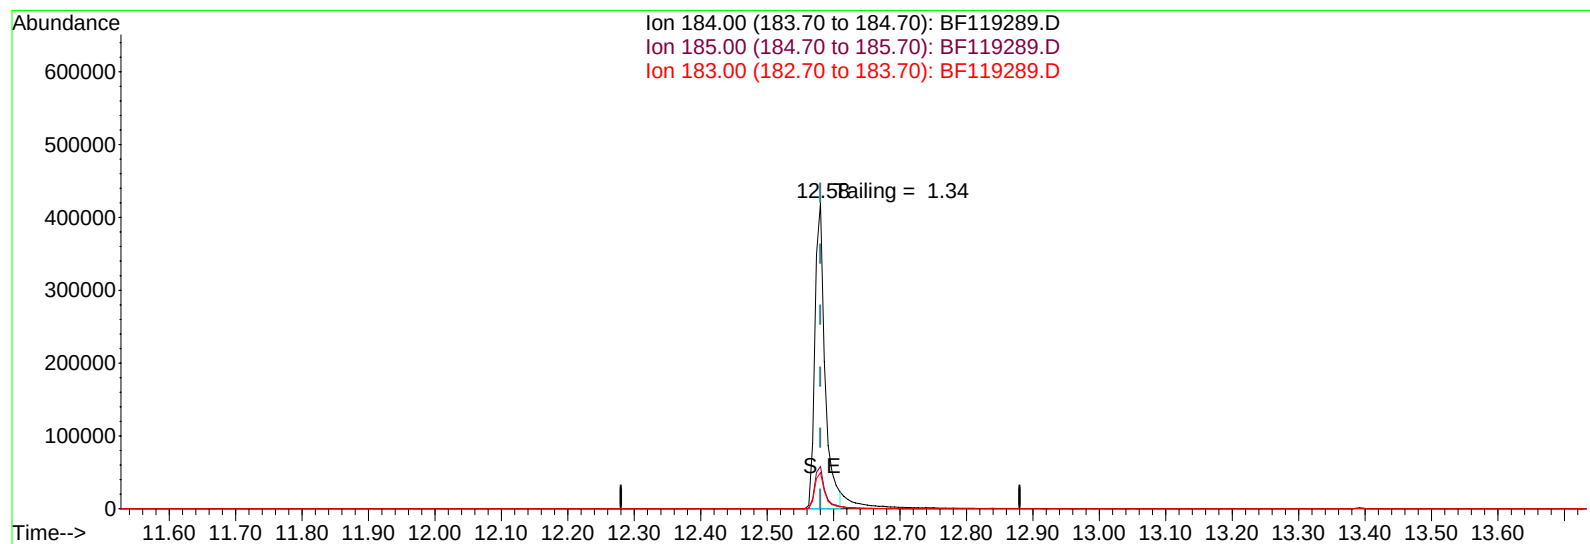

(77) Benzidine

12.580min (+0.000) 0.00ng

response 478014

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	13.88
183.00	12.40	11.85
0.00	0.00	0.00