


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF030920\
 Data File : BF119289.D
 Acq On : 9 Mar 2020 16:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 06 23:38:46 2020

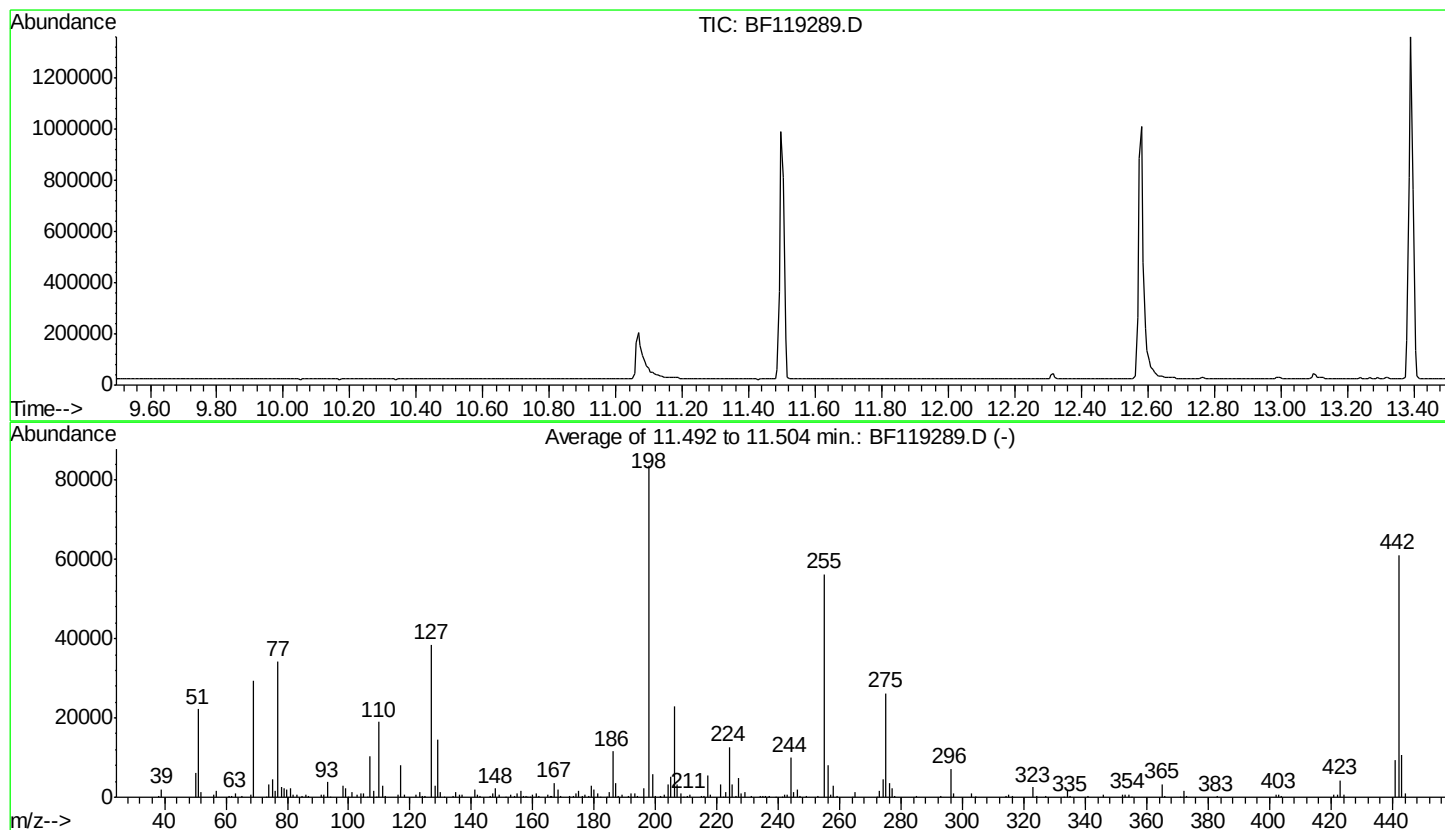

AutoFind: Scans 1599, 1600, 1601; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.5	22181	PASS
68	69	0.00	2	1.7	508	PASS
69	198	0.00	100	35.1	29314	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.1	38578	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	83624	PASS
199	198	5	9	6.8	5701	PASS
275	198	10	60	31.4	26280	PASS
365	198	1	100	4.0	3319	PASS
441	198	0.01	100	11.3	9411	PASS
442	198	50	100	73.0	61026	PASS
443	442	15	24	17.7	10776	PASS