

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030922\
 Data File : BF127282.D
 Acq On : 09 Mar 2022 18:13
 Operator : CG\JU
 Sample : PB143199BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB143199BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF030922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127282.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.504	542	547	550	rBV	2598444	2527408	76.94%	13.710%
2	6.504	712	717	720	rBV	2252451	2392972	72.85%	12.980%
3	6.869	775	779	782	rBV	540782	458069	13.95%	2.485%
4	7.433	870	875	878	rBV	1587681	1686168	51.33%	9.146%
5	8.151	992	997	1000	rBV	658087	584456	17.79%	3.170%
6	9.227	1174	1180	1183	rBV	2998393	2783696	84.74%	15.100%
7	9.910	1291	1296	1299	rBV	836613	726727	22.12%	3.942%
8	10.704	1426	1431	1434	rBV	2044497	1832556	55.79%	9.941%
9	11.398	1546	1549	1553	rBV	867211	775208	23.60%	4.205%
10	12.992	1815	1820	1823	rBV	3448417	3284811	100.00%	17.818%
11	14.045	1995	1999	2003	rBV	729682	672751	20.48%	3.649%
12	14.139	2009	2015	2021	rBV	65298	72812	2.22%	0.395%
13	15.533	2247	2252	2261	rVB	469047	580158	17.66%	3.147%
14	17.221	2529	2539	2540	rBV6	31122	57422	1.75%	0.311%




Sum of corrected areas: 18435214

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030922\
Data File : BF127282.D
Acq On : 09 Mar 2022 18:13
Operator : CG\JU
Sample : PB143199BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143199BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

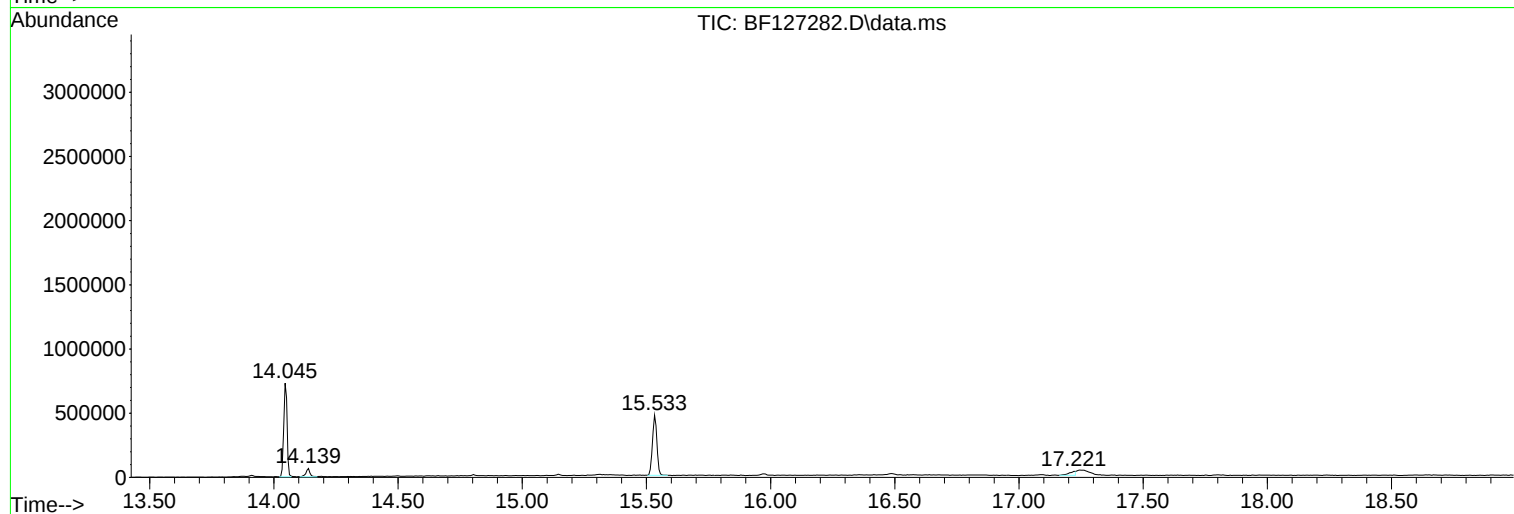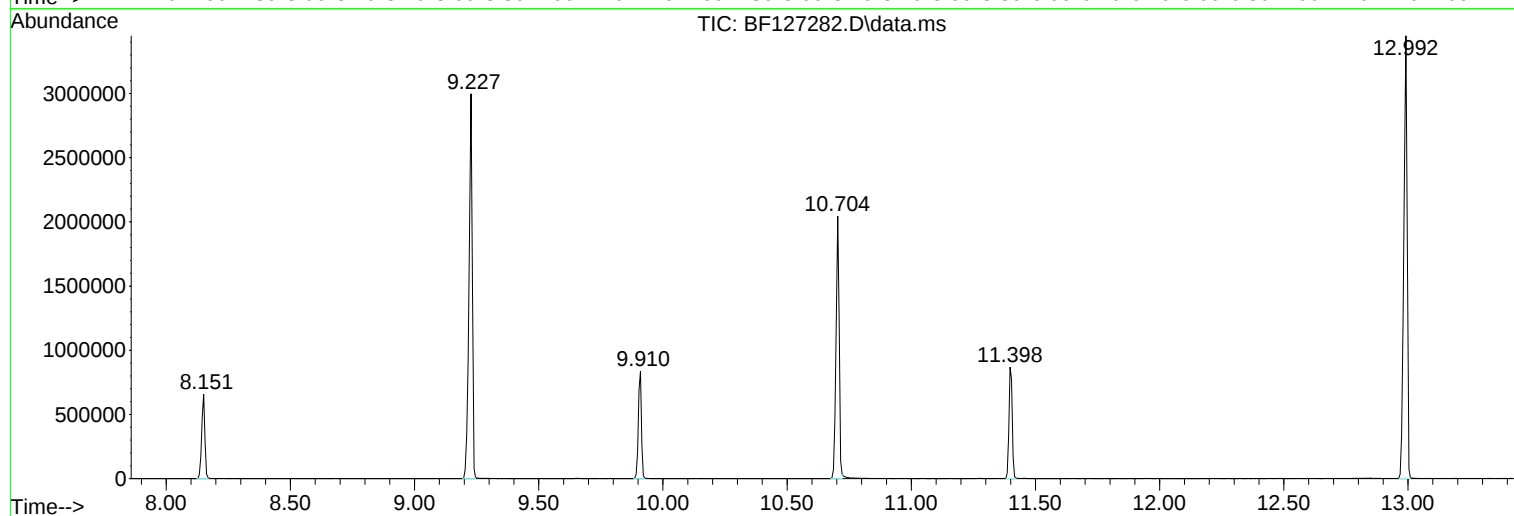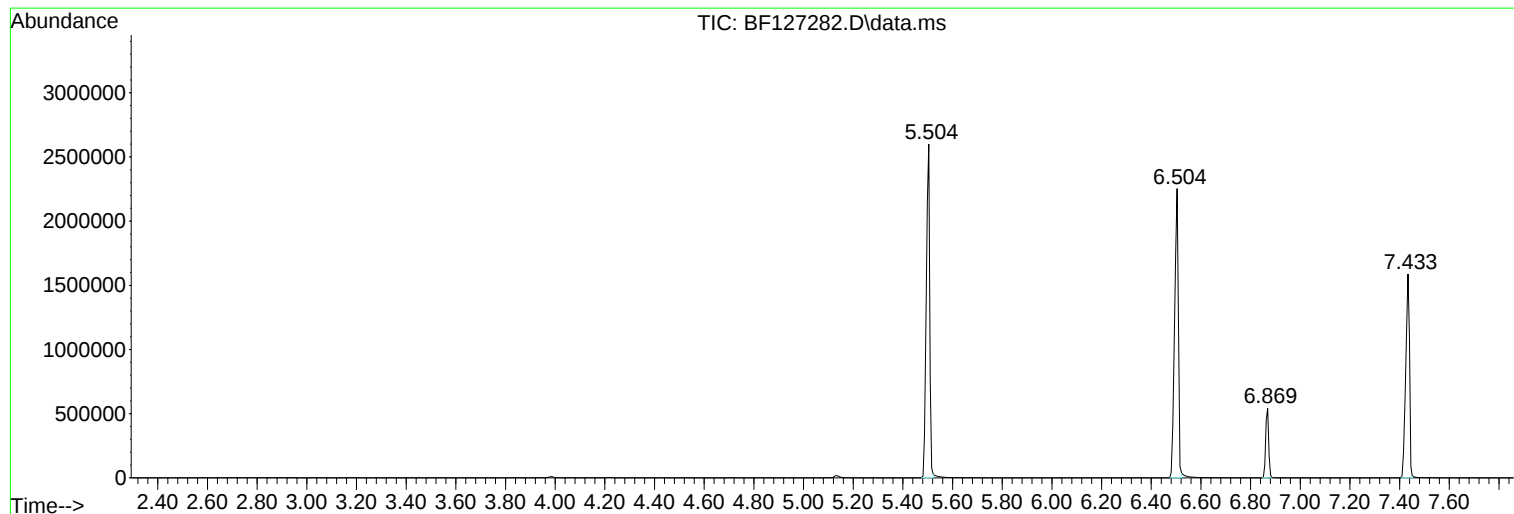

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030922\
Data File : BF127282.D
Acq On : 09 Mar 2022 18:13
Operator : CG\JU
Sample : PB143199BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143199BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.139	2.16 ng	72812	Chrysene-d12	14.045

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	93
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19N03S	1000483-83-4	62
3			5-Methyl-8-phenylfuro[3',2':5,6]...	277	C16H11N3O2	1000460-07-9	40
4			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	38
5			2-Phenyl-6-(trifluoromethyl)-1H-...	277	C15H10F3NO	1000387-59-3	28

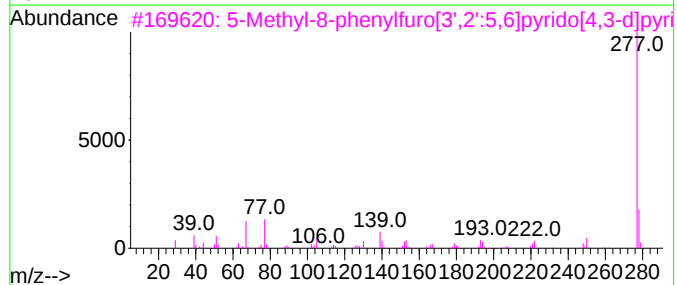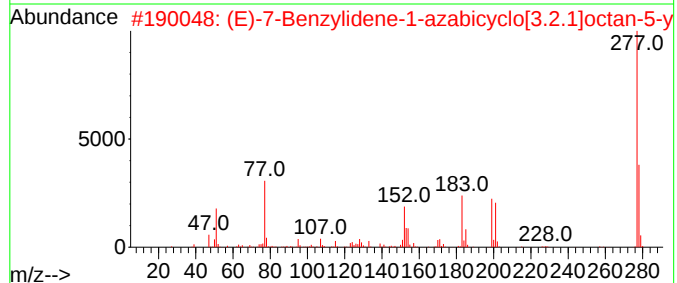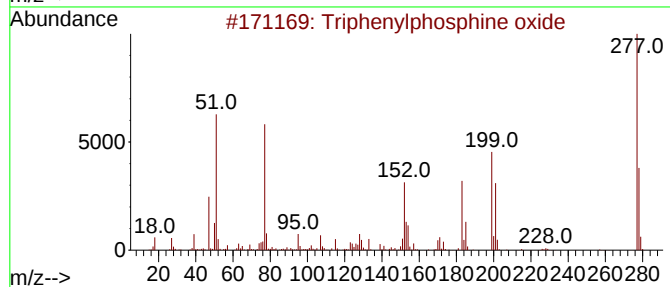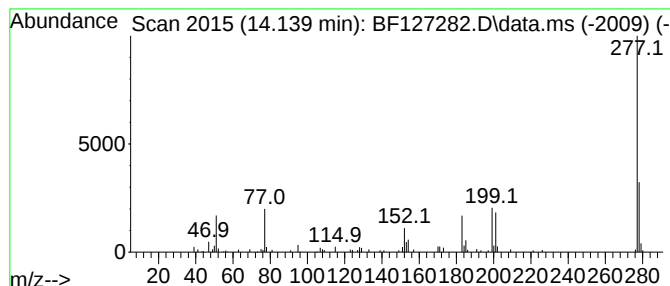

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030922\
Data File : BF127282.D
Acq On : 09 Mar 2022 18:13
Operator : CG\JU
Sample : PB143199BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143199BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.139	2.2	ng	72812	5	14.045	672751	20.0