
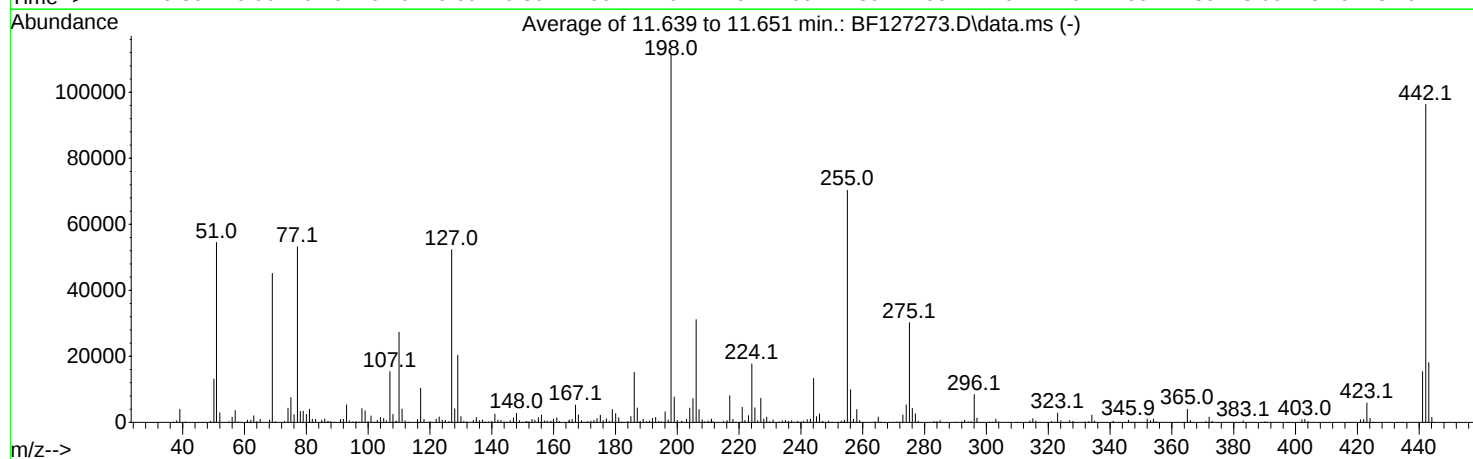


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030922\
 Data File : BF127273.D
 Acq On : 09 Mar 2022 13:14
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF030922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 09 17:59:49 2022

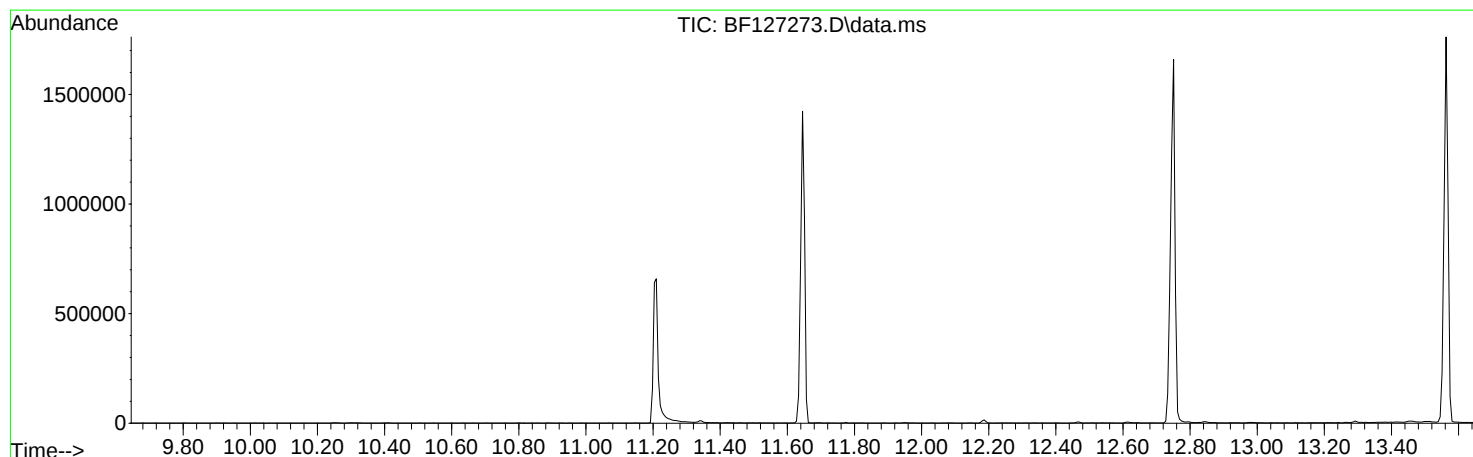

AutoFind: Scans 1590, 1591, 1592; Background Corrected with Scan 1585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.9	54471	PASS
68	69	0.00	2	1.7	753	PASS
69	198	0.00	100	40.5	45112	PASS
70	69	0.00	2	0.5	208	PASS
127	198	10	80	46.9	52280	PASS
197	198	0.00	2	0.6	723	PASS
198	198	100	100	100.0	111435	PASS
199	198	5	9	6.9	7645	PASS
275	198	10	60	27.1	30219	PASS
365	198	1	100	3.6	3956	PASS
441	198	0.01	100	13.8	15334	PASS
442	442	50	100	100.0	96307	PASS
443	442	15	24	18.8	18097	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/9/2022	BNA_F	<u>BF127273.D</u>
Compound Name	Response	Retention Time
DDT	291182	13.56
DDD	471	13.26
DDE	59	12.97
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
530	291712	0.18

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030922\
Data File : BF127273.D
Acq On : 09 Mar 2022 13:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 09 14:47:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 09 14:41:52 2022
Response via : Initial Calibration

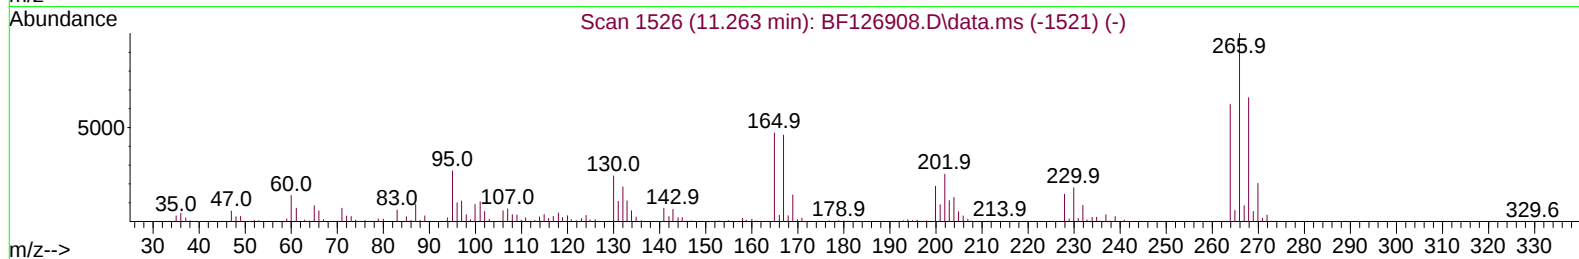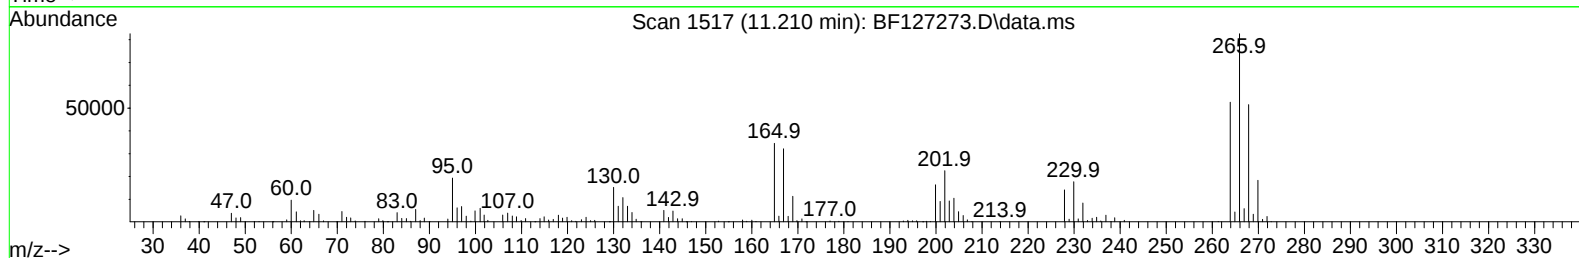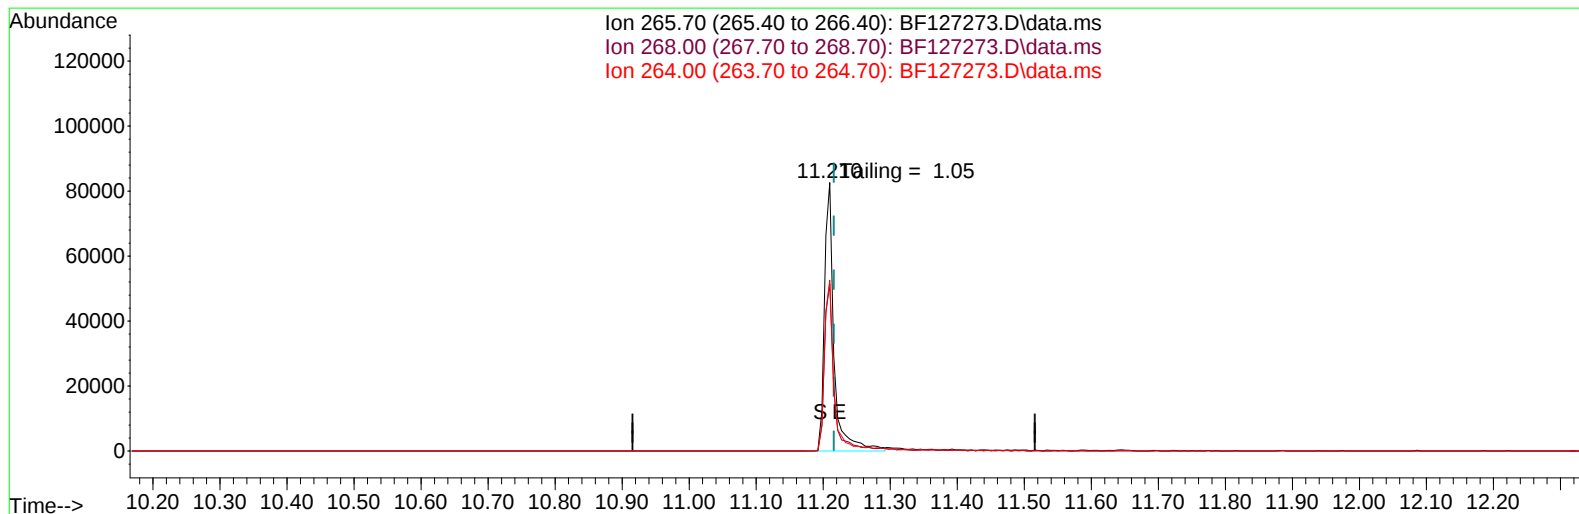

TIC: BF127273.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.006) 27675.97 ng




response 83591

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	62.33
264.00	63.00	63.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030922\
Data File : BF127273.D
Acq On : 09 Mar 2022 13:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 09 14:47:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 09 14:41:52 2022
Response via : Initial Calibration

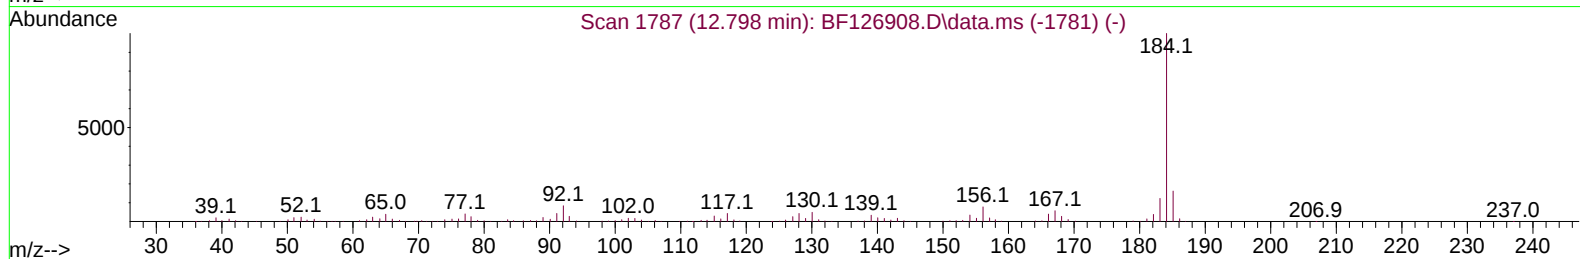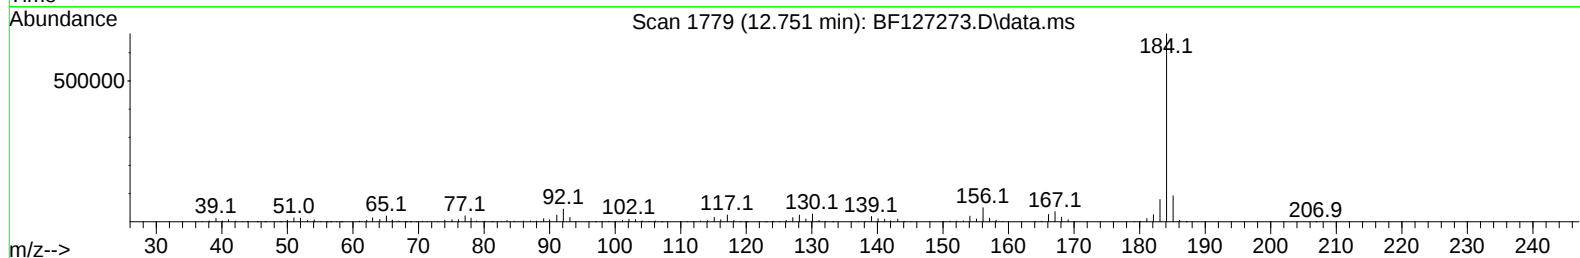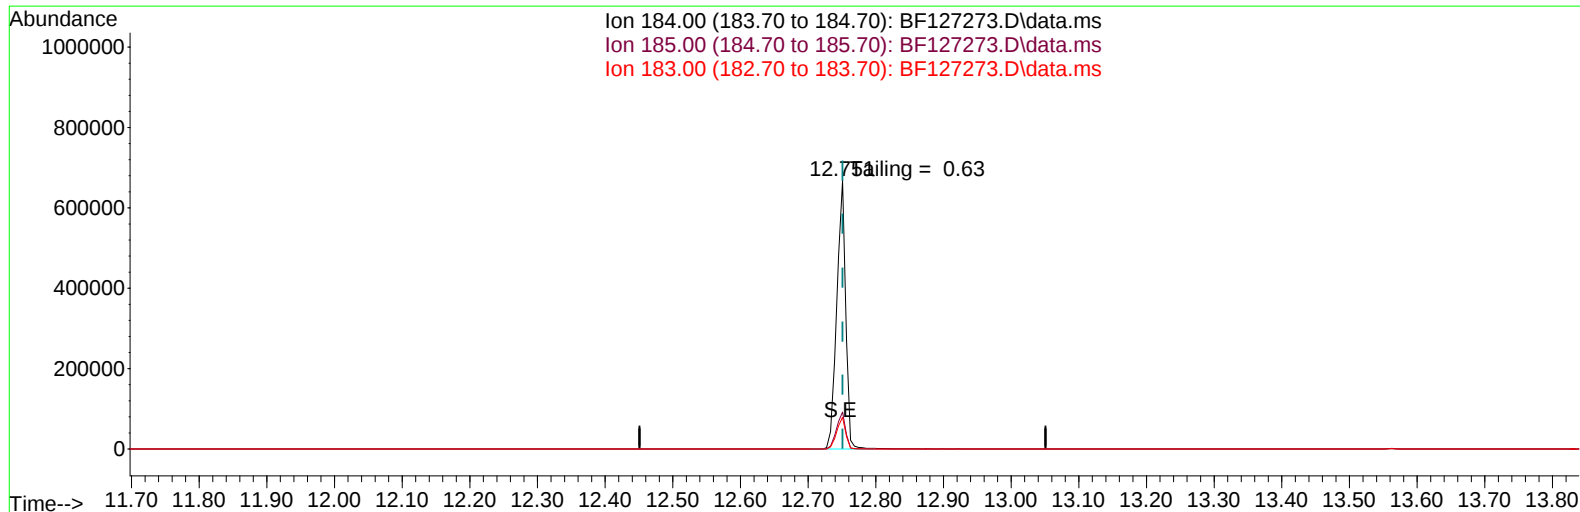

TIC: BF127273.D\data.ms

(77) Benzidine

12.751min (-0.000) 0.00 ng

response 610724

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.81
183.00	10.20	11.83
0.00	0.00	0.00