


Data Path : Z:\HPCHEM1\BNA_F\Data\BF031015\
 Data File : BF077657.D
 Acq On : 10 Mar 2015 11:53
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 10 13:44:42 2015

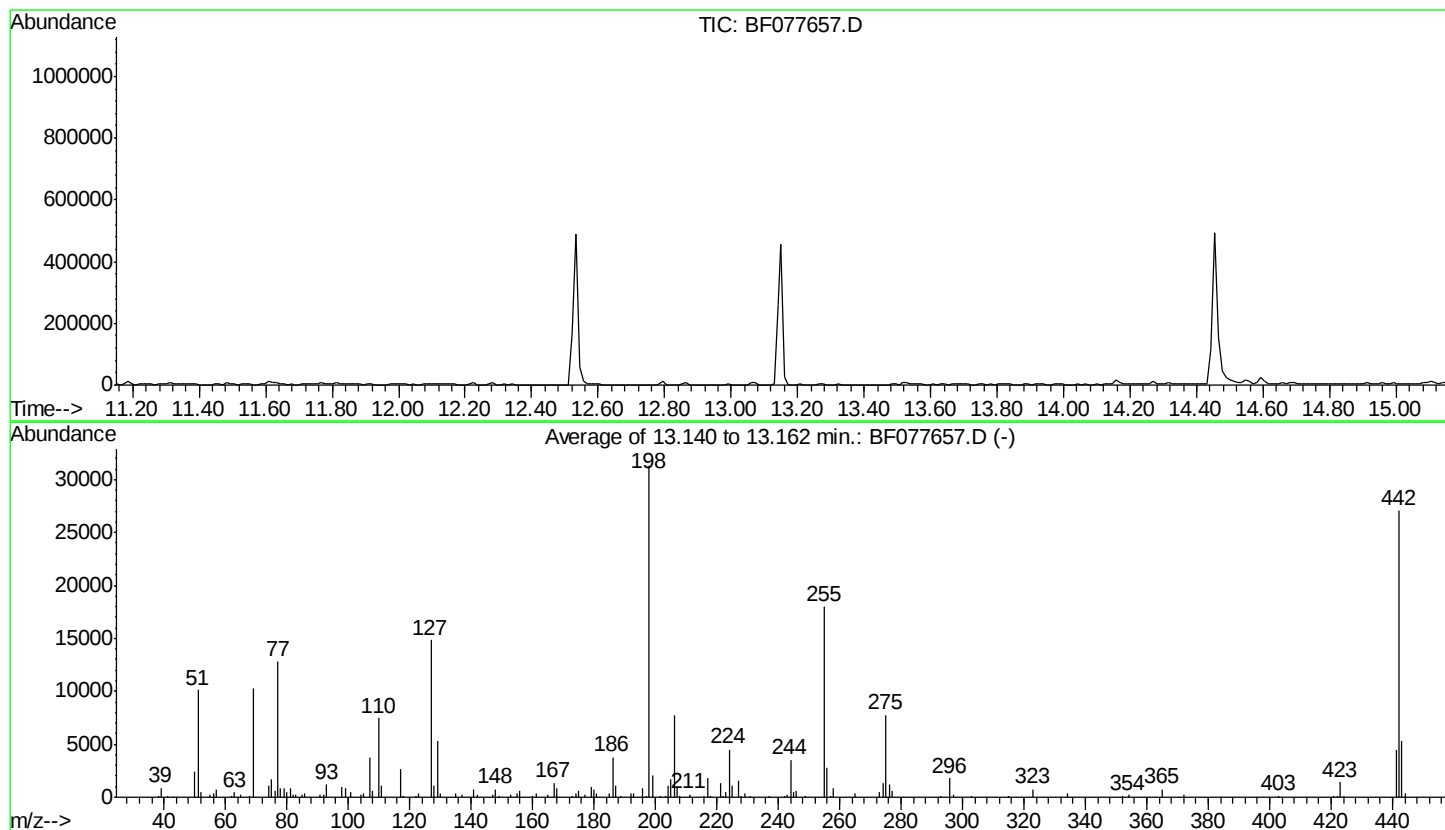

AutoFind: Scans 1072, 1073, 1074; Background Corrected with Scan 1068

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.4	10140	PASS
68	69	0.00	2	1.3	129	PASS
69	198	0.00	100	32.8	10278	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.3	14817	PASS
197	198	0.00	2	0.5	152	PASS
198	198	100	100	100.0	31309	PASS
199	198	5	9	6.6	2059	PASS
275	198	10	60	24.8	7760	PASS
365	198	1	100	2.4	752	PASS
441	442	0.01	24	16.4	4433	PASS
442	198	50	100	86.4	27057	PASS
443	442	15	24	19.6	5290	PASS