
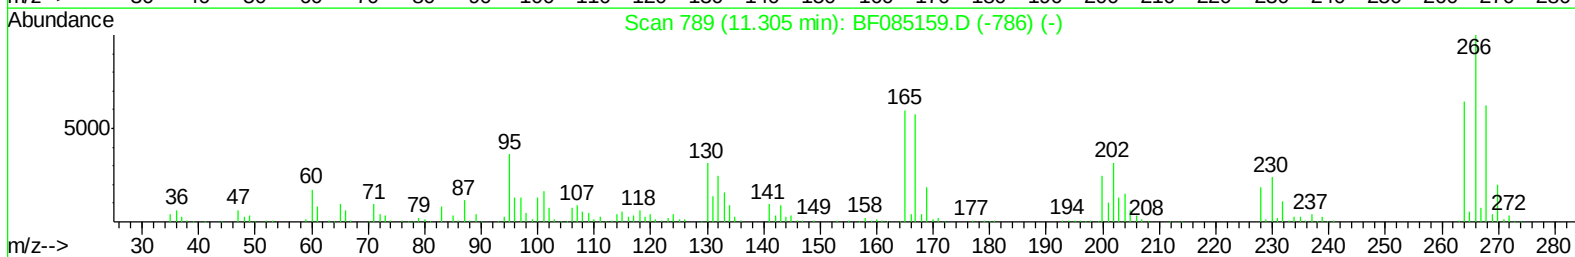
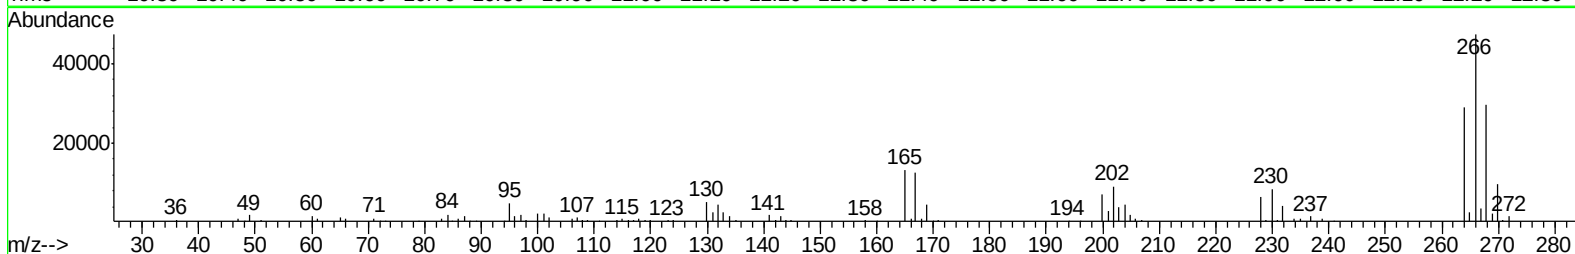


Data Path : S:\HPCHEM1\BNA_F\DATA\BF031016\
Data File : BF085328.D
Acq On : 10 Mar 2016 12:11
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 11 17:07:55 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 04 00:54:58 2016
Response via : Initial Calibration

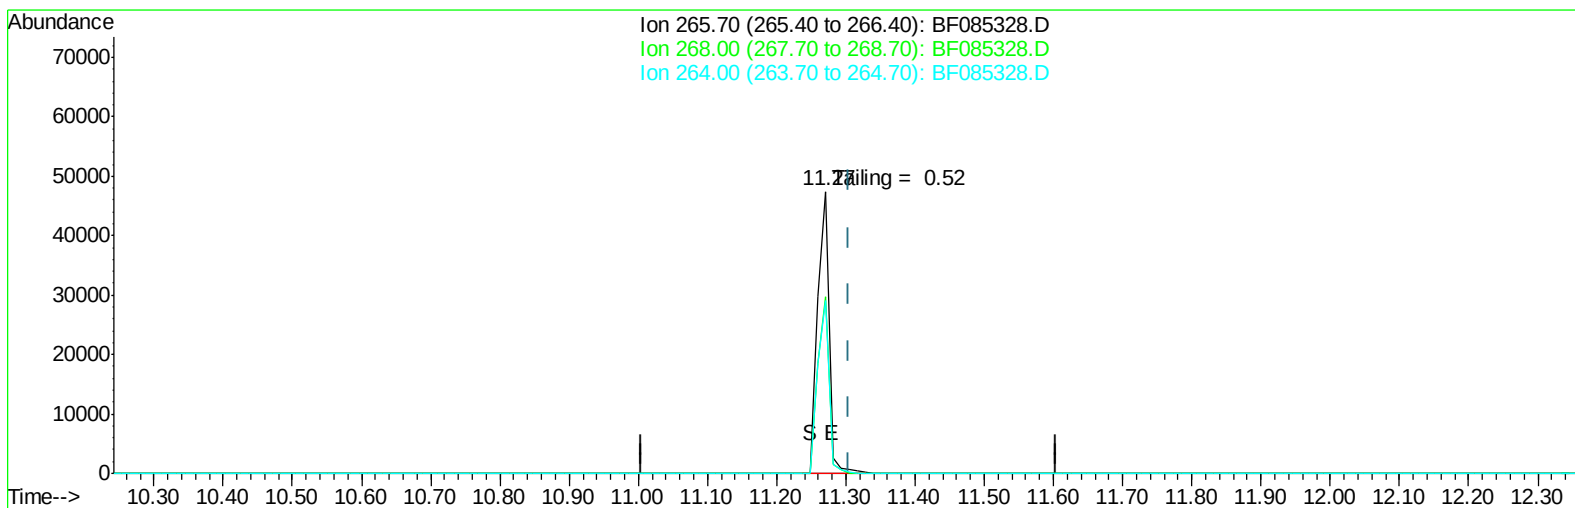

TIC: BF085328.D

(69) Pentachlorophenol (C)




11.271min (-0.034) 32640.54ng

response 56116

Ion	Exp%	Act%
265.70	100	100
268.00	62.50	62.81
264.00	64.30	61.25
0.00	0.00	0.00

```
Data Path : S:\HPCHEM1\BNA_F\DATA\BF031016\  
Data File : BF085328.D  
Acq On    : 10 Mar 2016 12:11  
Operator  : UM/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Quant Time: Mar 11 17:07:55 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 04 00:54:58 2016
Response via : Initial Calibration

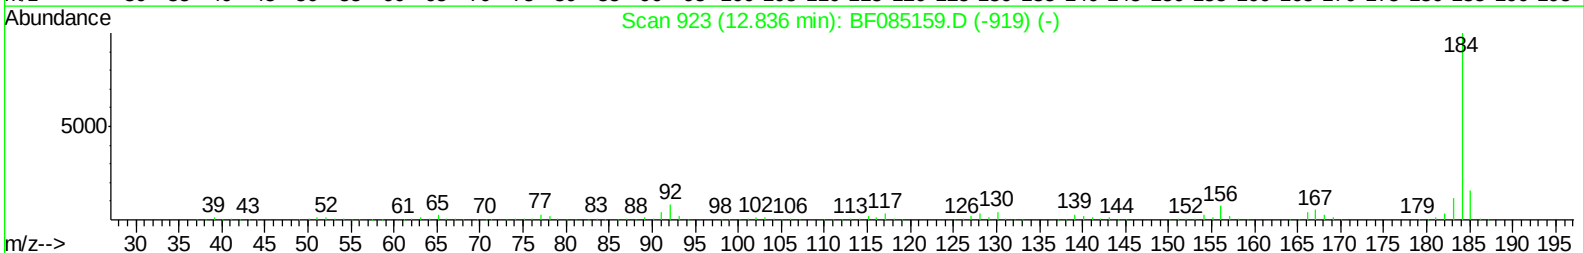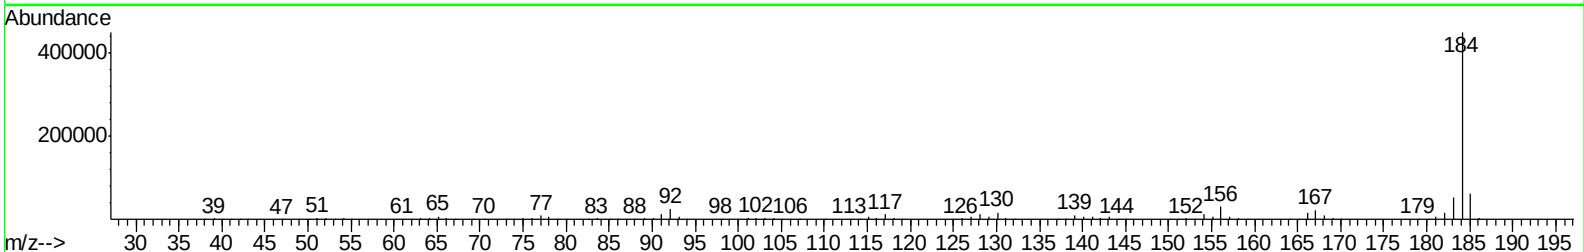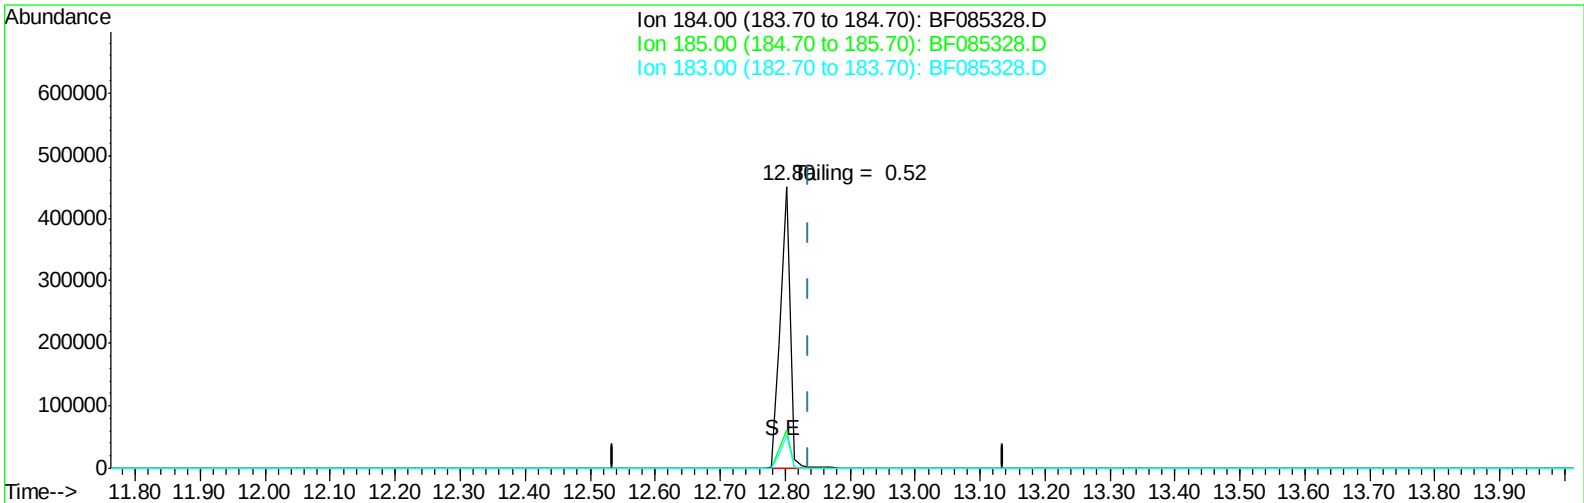

TIC: BF085328.D

(76) Benzidine

12.802min (-0.034) 0.00ng

response 467909

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	13.83
183.00	11.80	11.86
0.00	0.00	0.00