
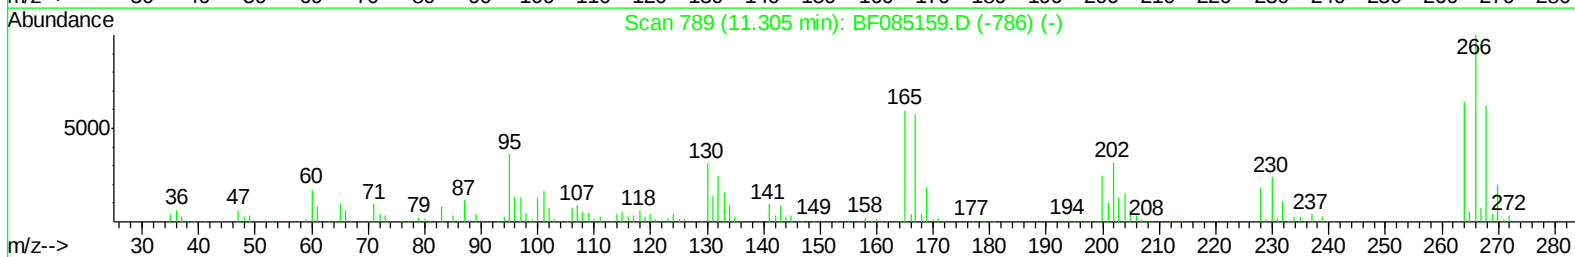
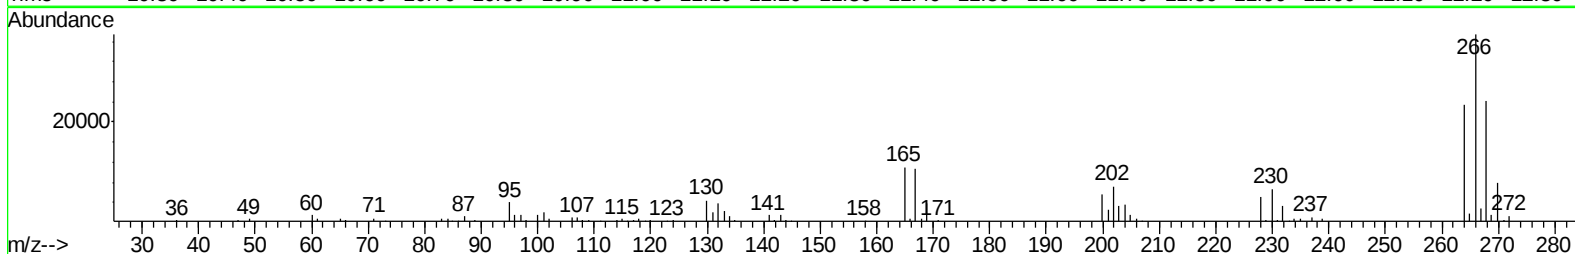


Data Path : Z:\HPCHEM1\BNA_F\Data\BF031016\
Data File : BF085353.D
Acq On : 11 Mar 2016 00:47
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 11 07:57:45 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 04 00:54:58 2016
Response via : Initial Calibration

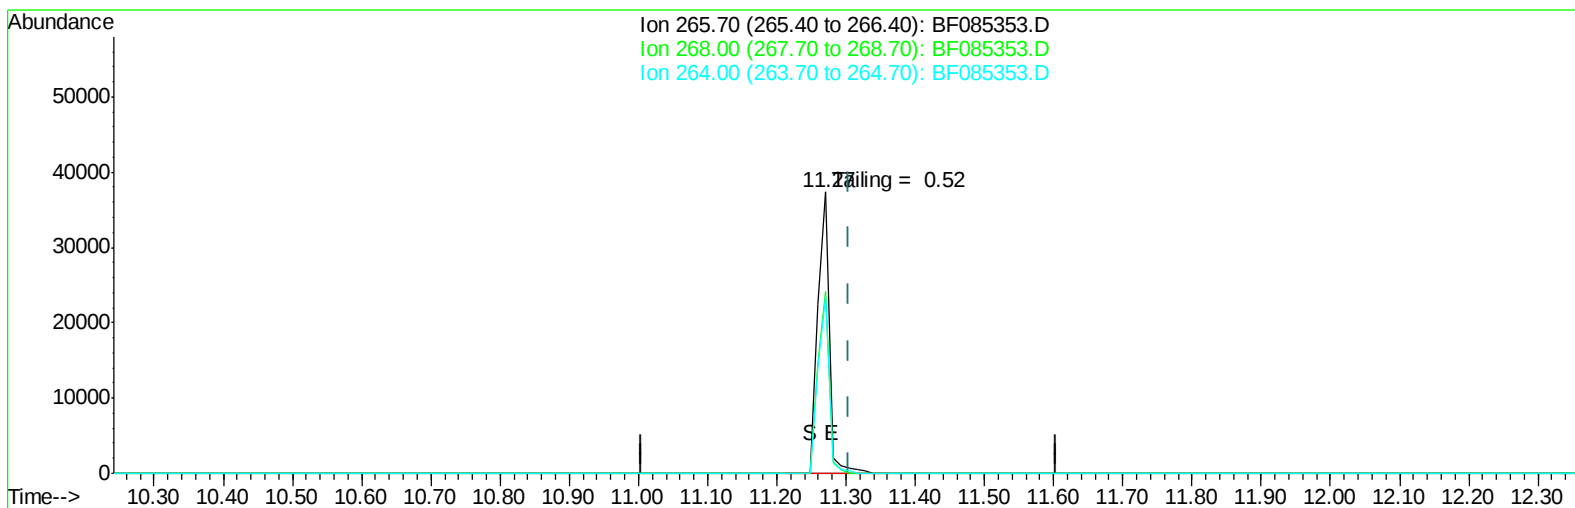

TIC: BF085353.D

(69) Pentachlorophenol (C)




11.270min (-0.034) 24084.49ng

response 44176

Ion	Exp%	Act%
265.70	100	100
268.00	62.50	64.63
264.00	64.30	62.82
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF031016\
Data File : BF085353.D
Acq On : 11 Mar 2016 00:47
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 11 07:57:45 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 04 00:54:58 2016
Response via : Initial Calibration

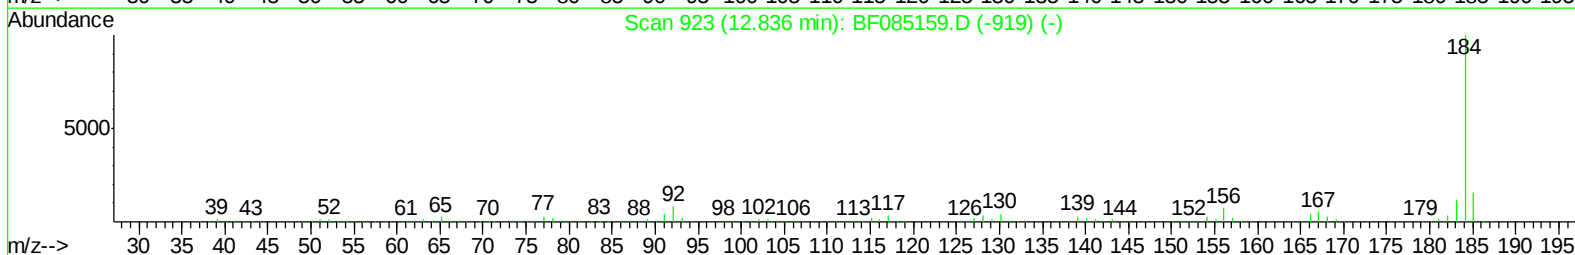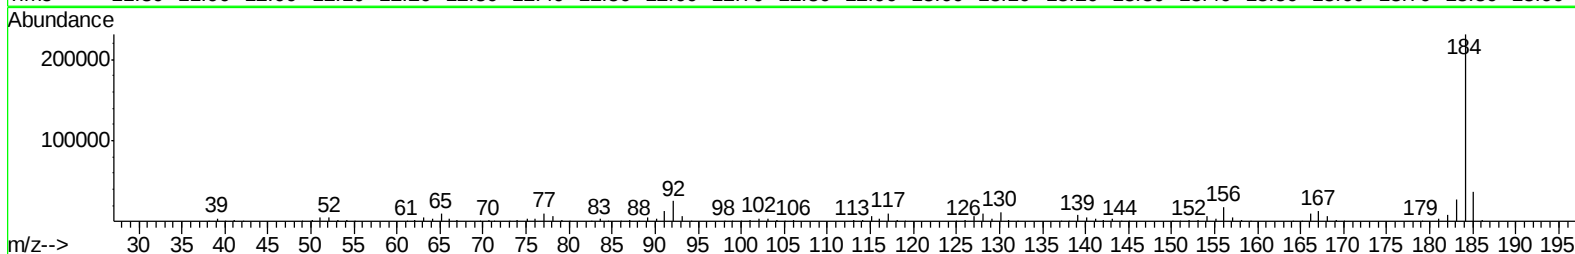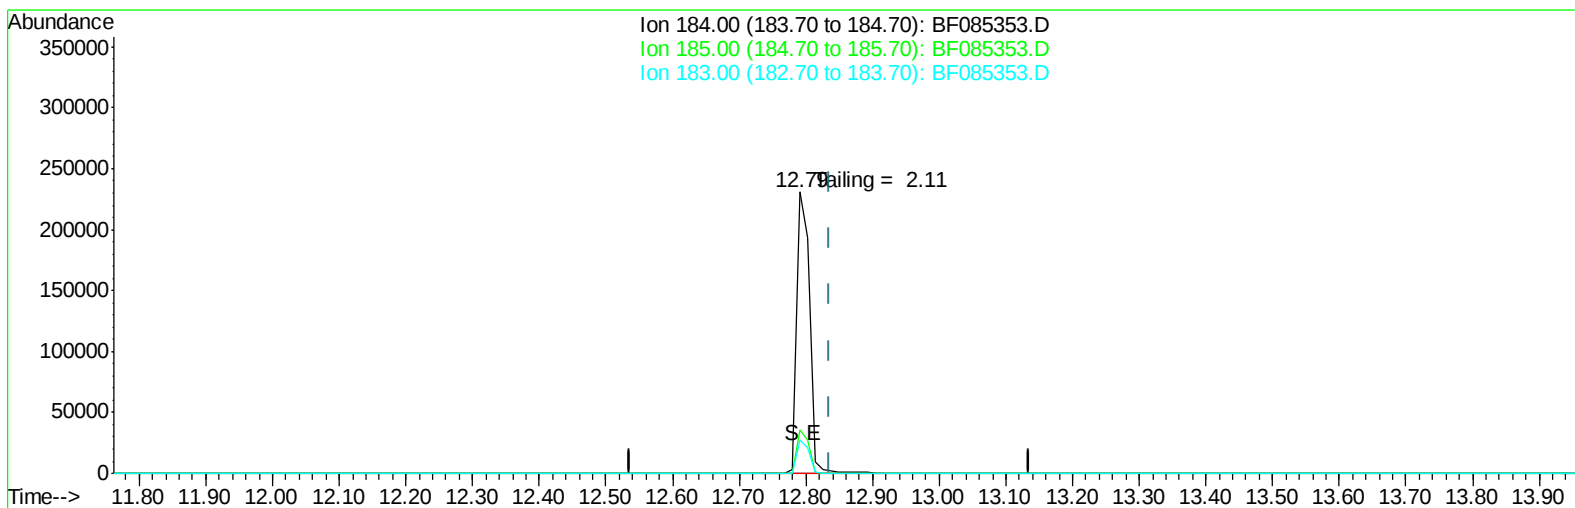

TIC: BF085353.D

(76) Benzidine

12.791min (-0.046) 0.00ng

response 307993

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	15.65
183.00	11.80	11.63
0.00	0.00	0.00