

Data Path : S:\HPCHEM1\BNA_F\DATA\BF031016\
 Data File : BF085362.D
 Acq On : 11 Mar 2016 5:05
 Operator : UM/SJ
 Sample : H1731-06
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-20-COMP

Quant Time: Mar 11 05:38:33 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 11 02:49:26 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.94	152	158119	20.00	ng	0.00
21) Naphthalene-d8	8.22	136	551623	20.00	ng	-0.01
38) Acenaphthene-d10	9.98	164	256305	20.00	ng	0.00
63) Phenanthrene-d10	11.46	188	437419	20.00	ng	0.00
75) Chrysene-d12	14.09	240	268720	20.00	ng	-0.01
86) Perylene-d12	15.56	264	268741	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.54	112	1218484	129.26	ng	0.00
7) Phenol-d6	6.57	99	1794452	145.30	ng	0.00
23) Nitrobenzene-d5	7.50	82	968385	93.94	ng	-0.01
41) 2,4,6-Tribromophenol	10.77	330	286200	130.50	ng	0.00
44) 2-Fluorobiphenyl	9.30	172	1498609	88.92	ng	0.00
78) Terphenyl-d14	13.05	244	1048602	90.59	ng	0.00
Target Compounds						Qvalue
49) Dimethylphthalate	9.69	163	349236	17.75	ng	99
83) Bis(2-ethylhexyl)phthalate	14.08	149	26302	2.18	ng	# 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : S:\HPCHEM1\BNA_F\DATA\BF031016\
Data File : BF085362.D
Acq On : 11 Mar 2016 5:05
Operator : UM/SJ
Sample : H1731-06
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-20-COMP

Quant Time: Mar 11 05:38:33 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 11 02:49:26 2016
Response via : Initial Calibration




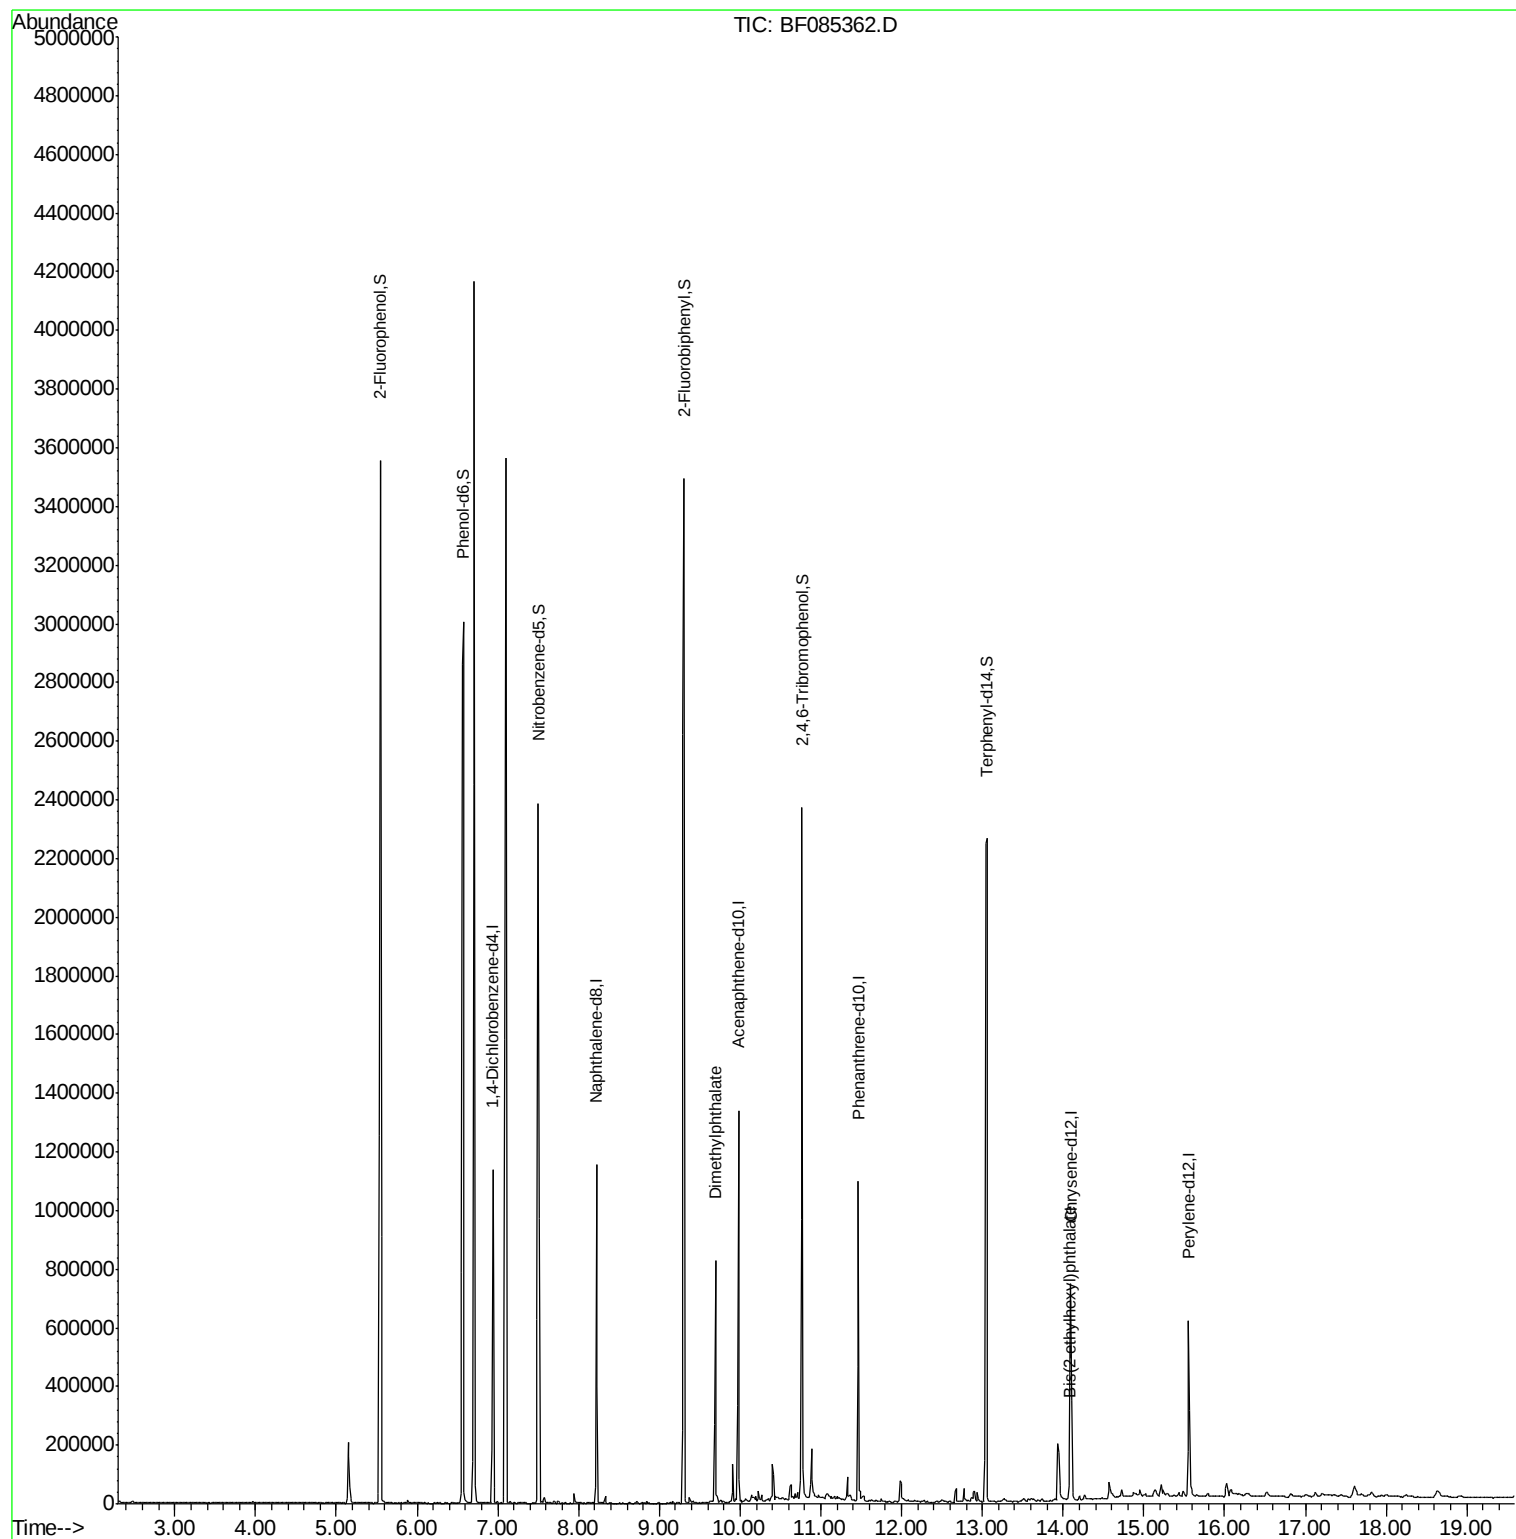




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.94 min Scan# 407
 Delta R.T. 0.00 min
 Lab File: BF085362.D
 Acq: 11 Mar 2016 5:05




Instrument :
 BNA_F
 ClientSampleId :
 SB-20-COMP

Tgt Ion:152 Resp: 158119
 Ion Ratio Lower Upper
 152 100
 150 155.5 124.6 186.8
 115 60.5 46.6 70.0

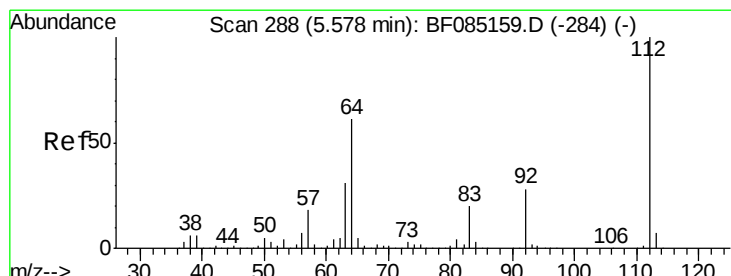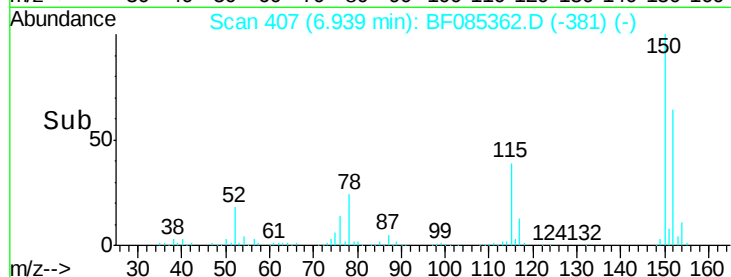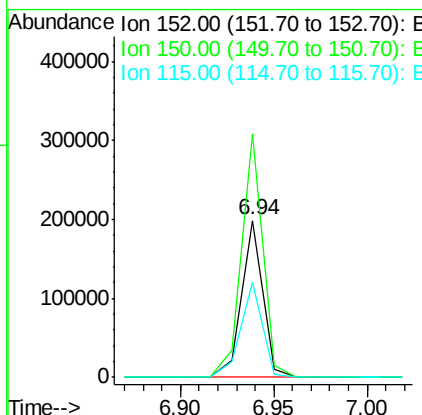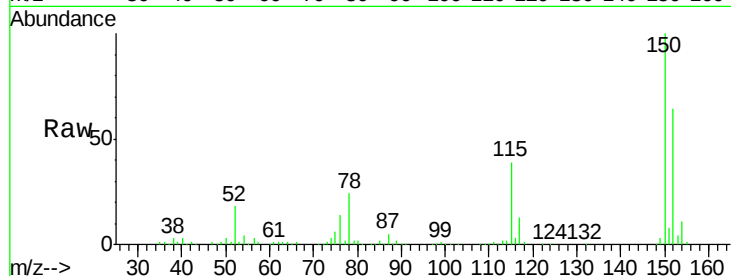

#5
 2-Fluorophenol
 Concen: 129.26 ng
 RT: 5.54 min Scan# 285
 Delta R.T. 0.00 min
 Lab File: BF085362.D
 Acq: 11 Mar 2016 5:05

Tgt Ion:112 Resp: 1218484
 Ion Ratio Lower Upper
 112 100
 64 57.1 49.0 73.4
 63 29.2 24.8 37.2

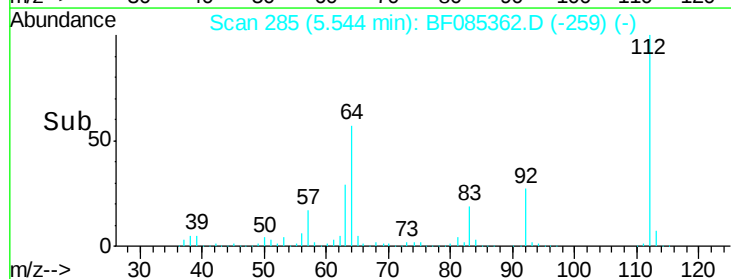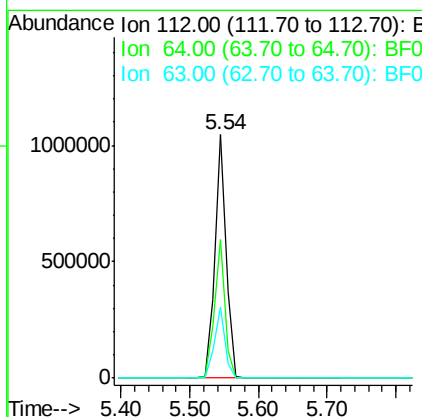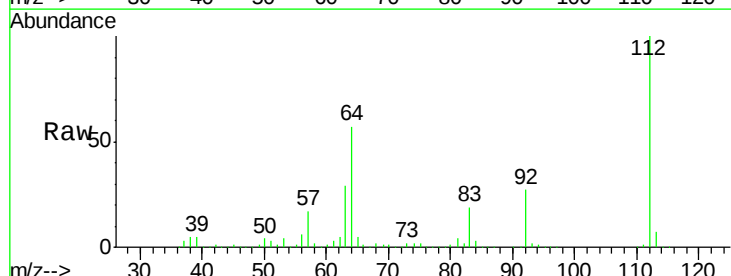



#7

Phenol-d6

Concen: 145.30 ng

RT: 6.57 min Scan# 375

Delta R.T. 0.00 min

Lab File: BF085362.D

Acq: 11 Mar 2016 5:05

Instrument :

BNA_F

ClientSampleId :

SB-20-COMP


Tgt Ion: 99 Resp: 1794452

Ion Ratio Lower Upper

99 100

42 12.1 13.6 20.4#



71 28.9 26.7 40.1

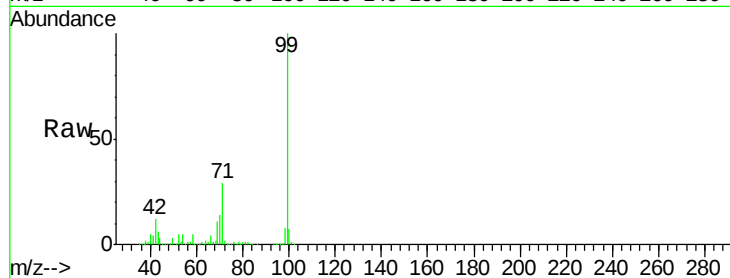

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

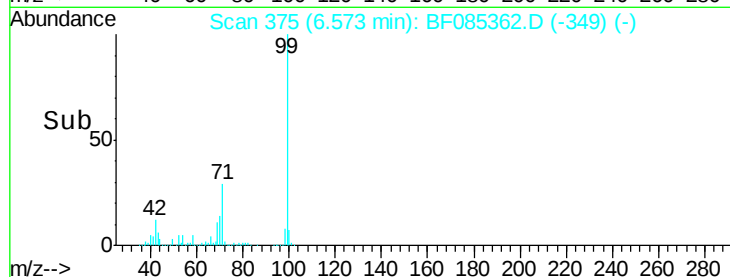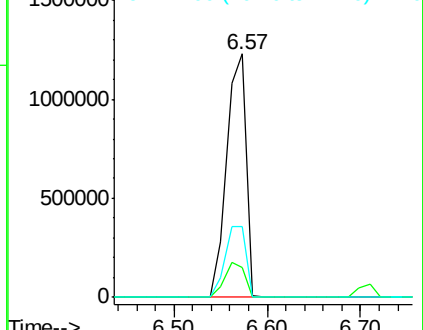

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.22 min Scan# 519

Delta R.T. -0.01 min

Lab File: BF085362.D

Acq: 11 Mar 2016 5:05

Tgt Ion: 136 Resp: 551623


Ion Ratio Lower Upper

136 100

137 11.4 9.3 13.9

54 8.9 7.4 11.2

68 6.8 6.0 9.0


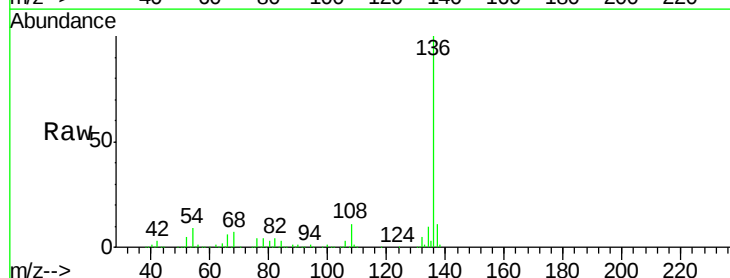


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

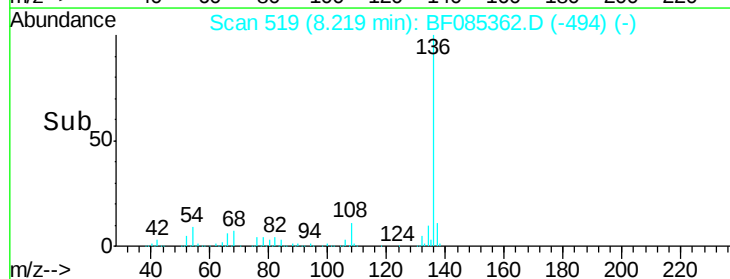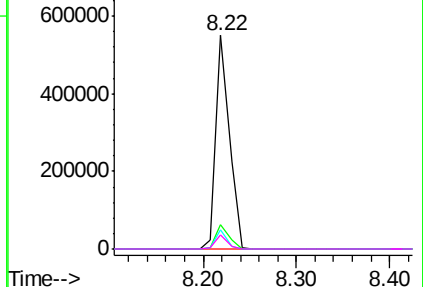






#23
 Nitrobenzene-d5
 Concen: 93.94 ng
 RT: 7.50 min Scan# 456
 Delta R.T. -0.01 min
 Lab File: BF085362.D
 Acq: 11 Mar 2016 5:05

Instrument :
 BNA_F
 ClientSampled :
 SB-20-COMP

Tgt Ion: 82 Resp: 968385
 Ion Ratio Lower Upper
 82 100
 128 43.8 34.5 51.7
 54 47.5 39.3 58.9

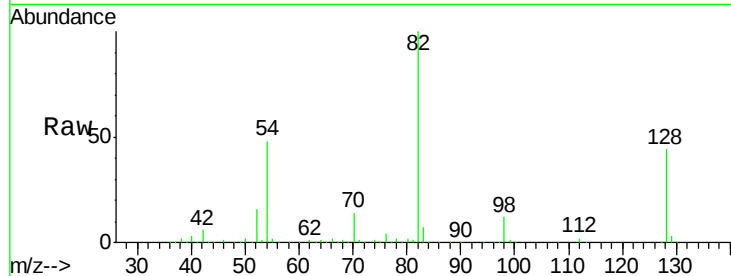


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

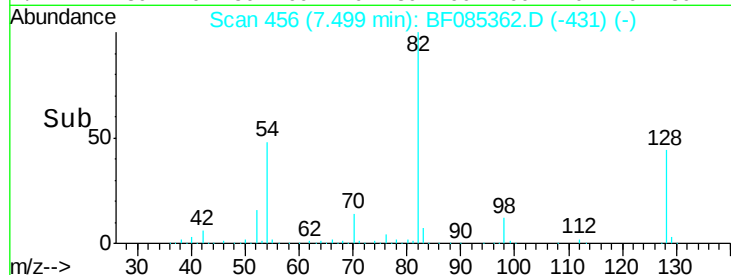
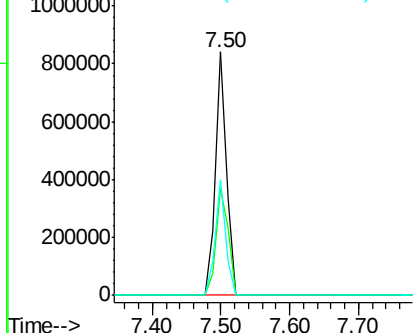


#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.98 min Scan# 673
 Delta R.T. 0.00 min
 Lab File: BF085362.D
 Acq: 11 Mar 2016 5:05

Tgt Ion: 164 Resp: 256305
 Ion Ratio Lower Upper
 164 100
 162 100.8 83.3 124.9
 160 46.4 37.9 56.9

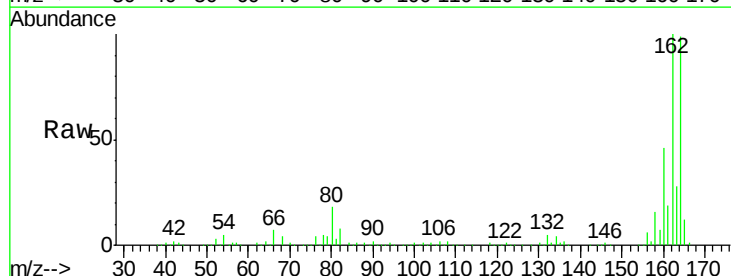

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

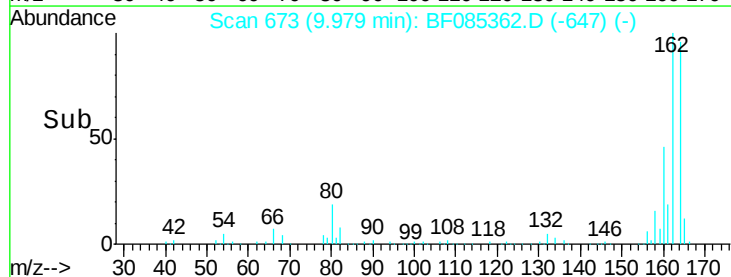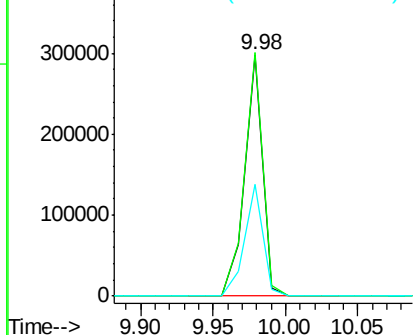







#41
 2,4,6-Tribromophenol
 Concen: 130.50 ng
 RT: 10.77 min Scan# 742
 Delta R.T. 0.00 min
 Lab File: BF085362.D
 Acq: 11 Mar 2016 5:05

Instrument :
 BNA_F
 ClientSampleId :
 SB-20-COMP

Tgt Ion:330 Resp: 286200
 Ion Ratio Lower Upper
 330 100
 332 95.8 77.1 115.7
 141 41.1 35.0 52.6

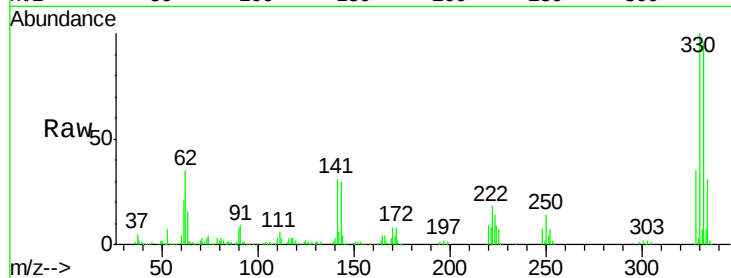


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

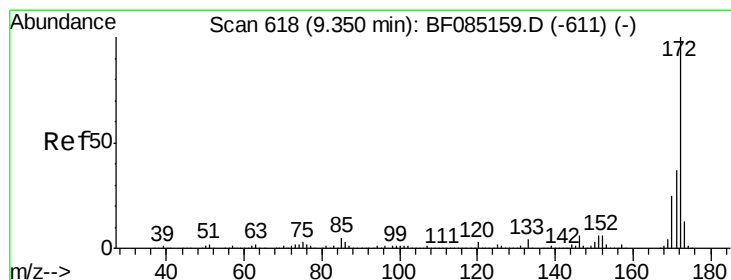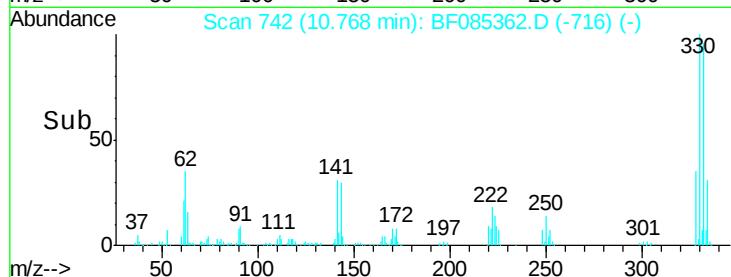
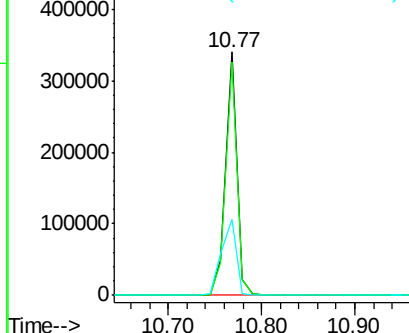



#44
 2-Fluorobiphenyl
 Concen: 88.92 ng
 RT: 9.30 min Scan# 614
 Delta R.T. 0.00 min
 Lab File: BF085362.D
 Acq: 11 Mar 2016 5:05

Tgt Ion:172 Resp: 1498609
 Ion Ratio Lower Upper
 172 100
 171 36.4 29.3 43.9
 170 24.7 20.0 30.0

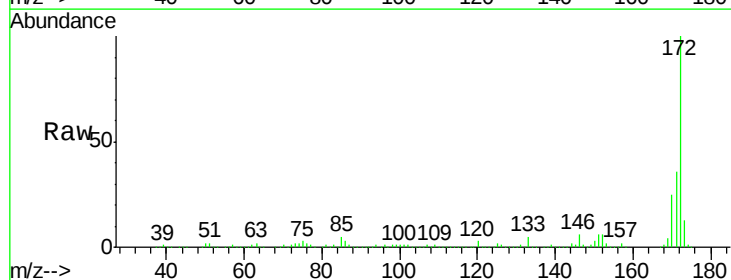

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

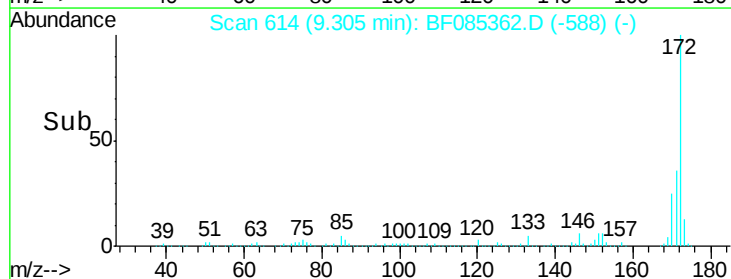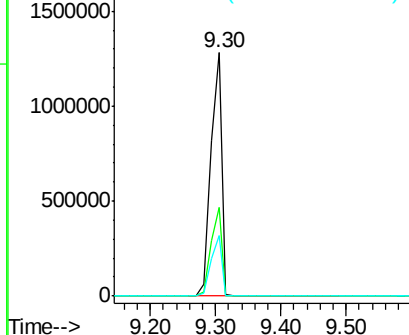

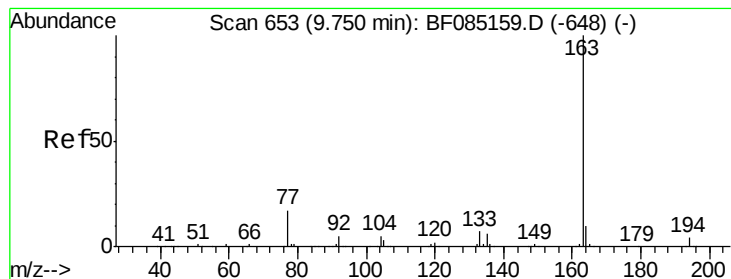

#49

Dimethylphthalate

Concen: 17.75 ng

RT: 9.69 min Scan# 648

Delta R.T. -0.01 min

Lab File: BF085362.D

Acq: 11 Mar 2016 5:05

Instrument :

BNA_F

ClientSampleId :

SB-20-COMP


Tgt Ion:163 Resp: 349236

Ion Ratio Lower Upper

163 100

194 3.9 3.1 4.7




164 9.9 8.2 12.4

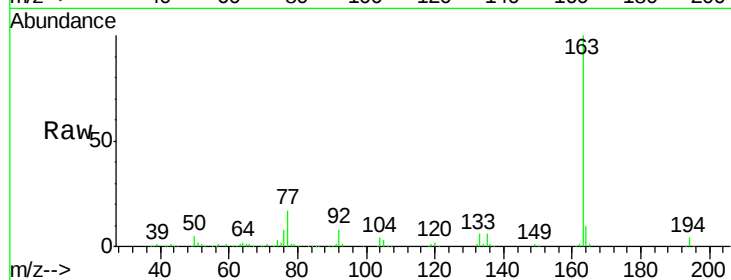

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

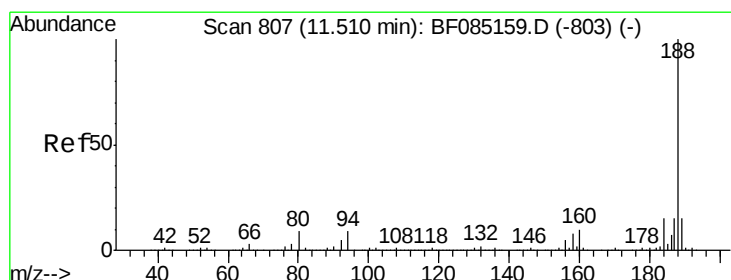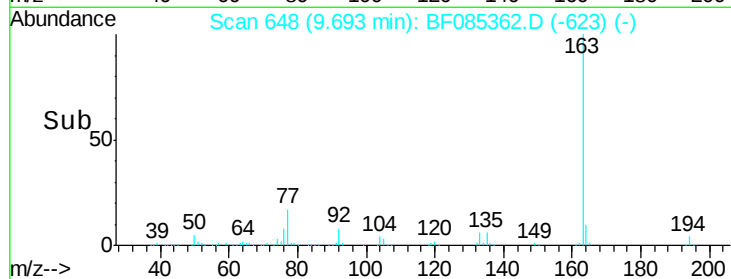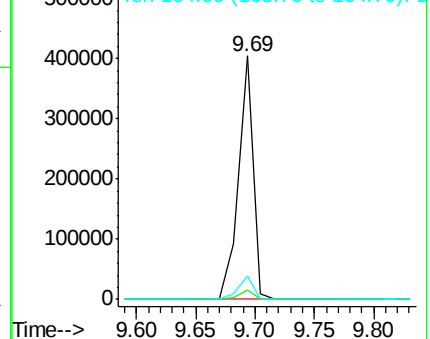

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.46 min Scan# 803

Delta R.T. 0.00 min

Lab File: BF085362.D

Acq: 11 Mar 2016 5:05


Tgt Ion:188 Resp: 437419

Ion Ratio Lower Upper

188 100

94 7.1 7.0 10.6



80 7.0 7.4 11.0#

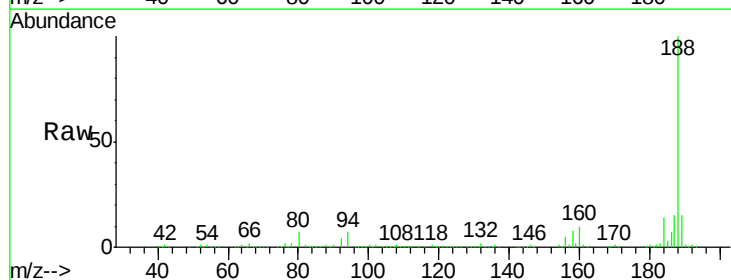


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

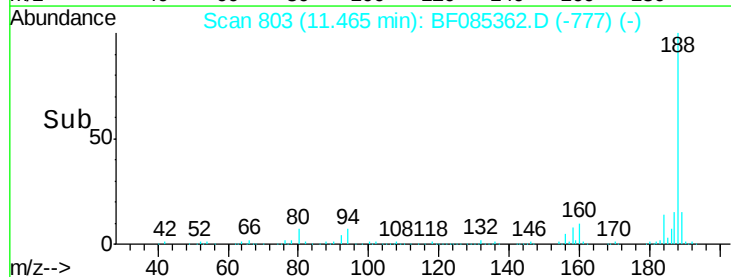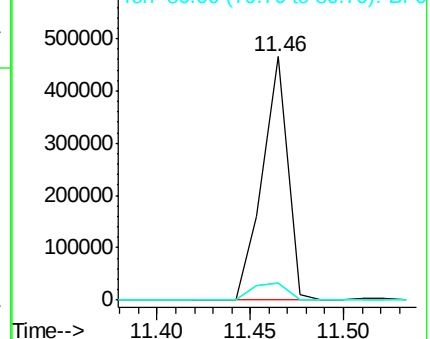

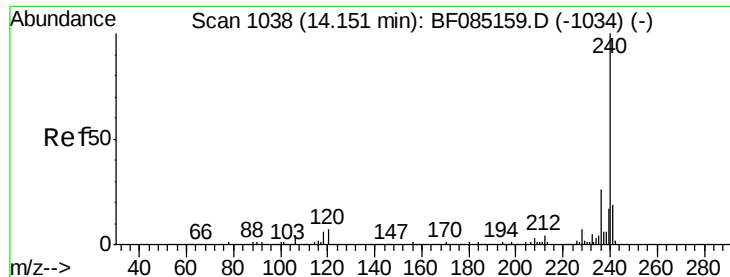

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.09 min Scan# 1033

Delta R.T. -0.01 min

Lab File: BF085362.D

Acq: 11 Mar 2016 5:05

Instrument :

BNA_F

ClientSampleId :

SB-20-COMP


Tgt Ion:240 Resp: 268720

Ion Ratio Lower Upper

240 100

120 17.2 5.3 7.9#




236 26.6 20.7 31.1

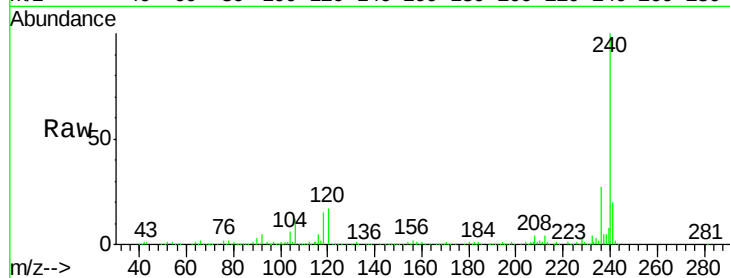

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

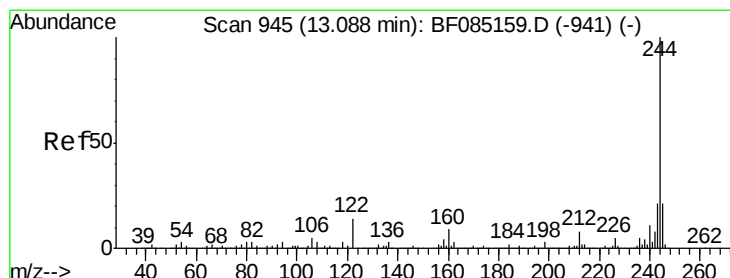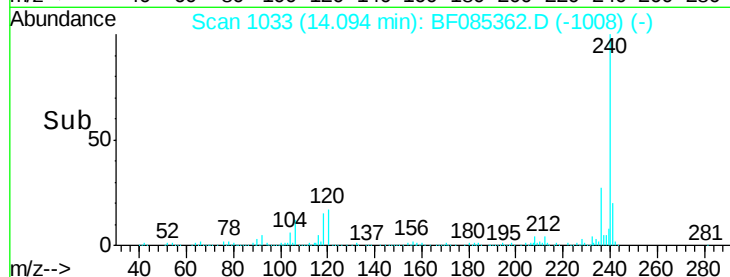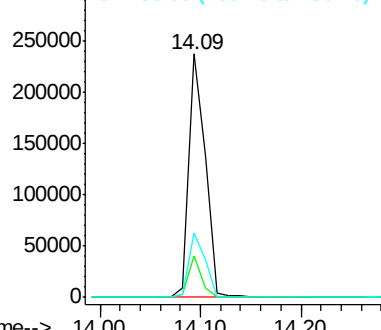

#78

Terphenyl-d14

Concen: 90.59 ng

RT: 13.05 min Scan# 942

Delta R.T. 0.00 min

Lab File: BF085362.D

Acq: 11 Mar 2016 5:05


Tgt Ion:244 Resp: 1048602

Ion Ratio Lower Upper

244 100

212 6.7 6.4 9.6



122 7.1 11.4 17.2#

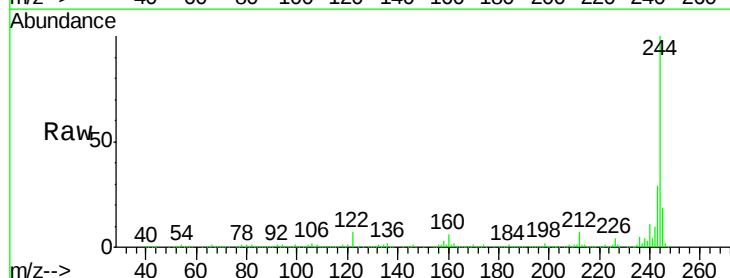


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

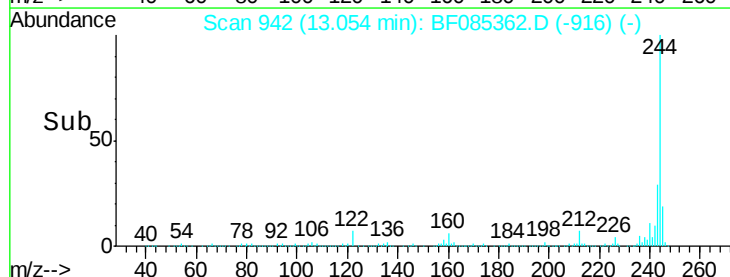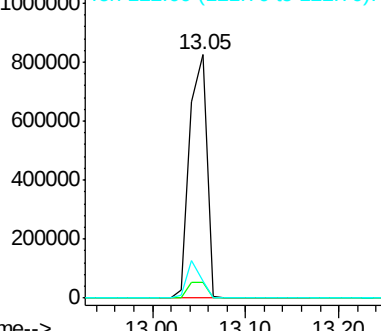


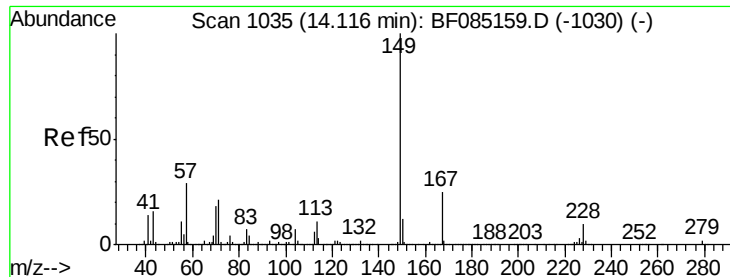




#83
 Bis(2-ethylhexyl)phthalate
 Concen: 2.18 ng
 RT: 14.08 min Scan# 1032
 Delta R.T. 0.00 min
 Lab File: BF085362.D
 Acq: 11 Mar 2016 5:05

Instrument :
 BNA_F
 ClientSampleId :
 SB-20-COMP

Tgt Ion:149 Resp: 26302
 Ion Ratio Lower Upper
 149 100
 167 25.2 20.3 30.5
 279 3.5 1.9 2.9#

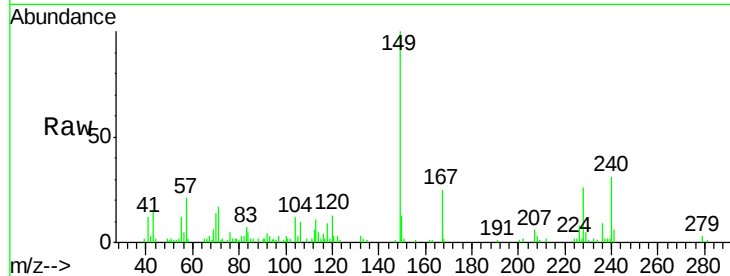


Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 167.00 (166.70 to 167.70): E
 Ion 279.00 (278.70 to 279.70): E

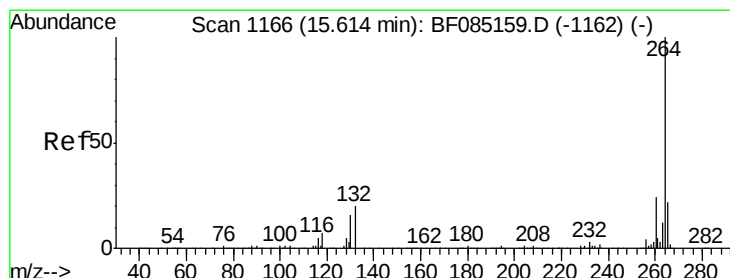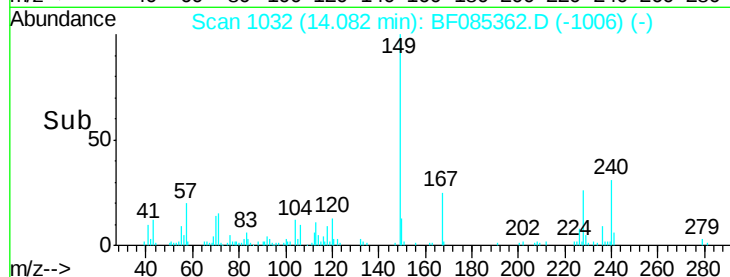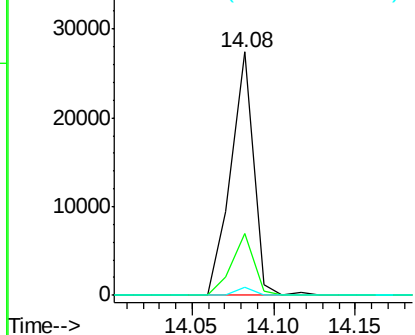

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.56 min Scan# 1161
 Delta R.T. -0.01 min
 Lab File: BF085362.D
 Acq: 11 Mar 2016 5:05

Tgt Ion:264 Resp: 268741
 Ion Ratio Lower Upper
 264 100
 260 23.5 19.2 28.8
 265 20.9 17.3 25.9

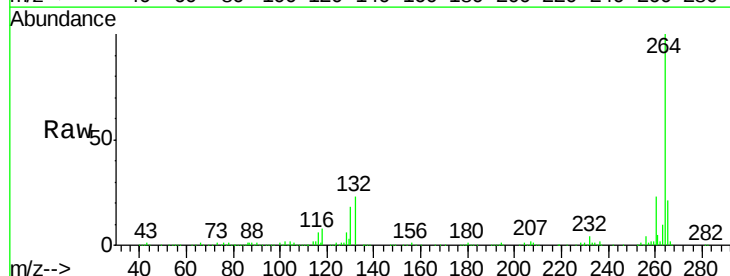

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

