


Data Path : S:\HPCHEM1\BNA_F\DATA\BF031016\
 Data File : BF085328.D
 Acq On : 10 Mar 2016 12:11
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 04 00:54:58 2016

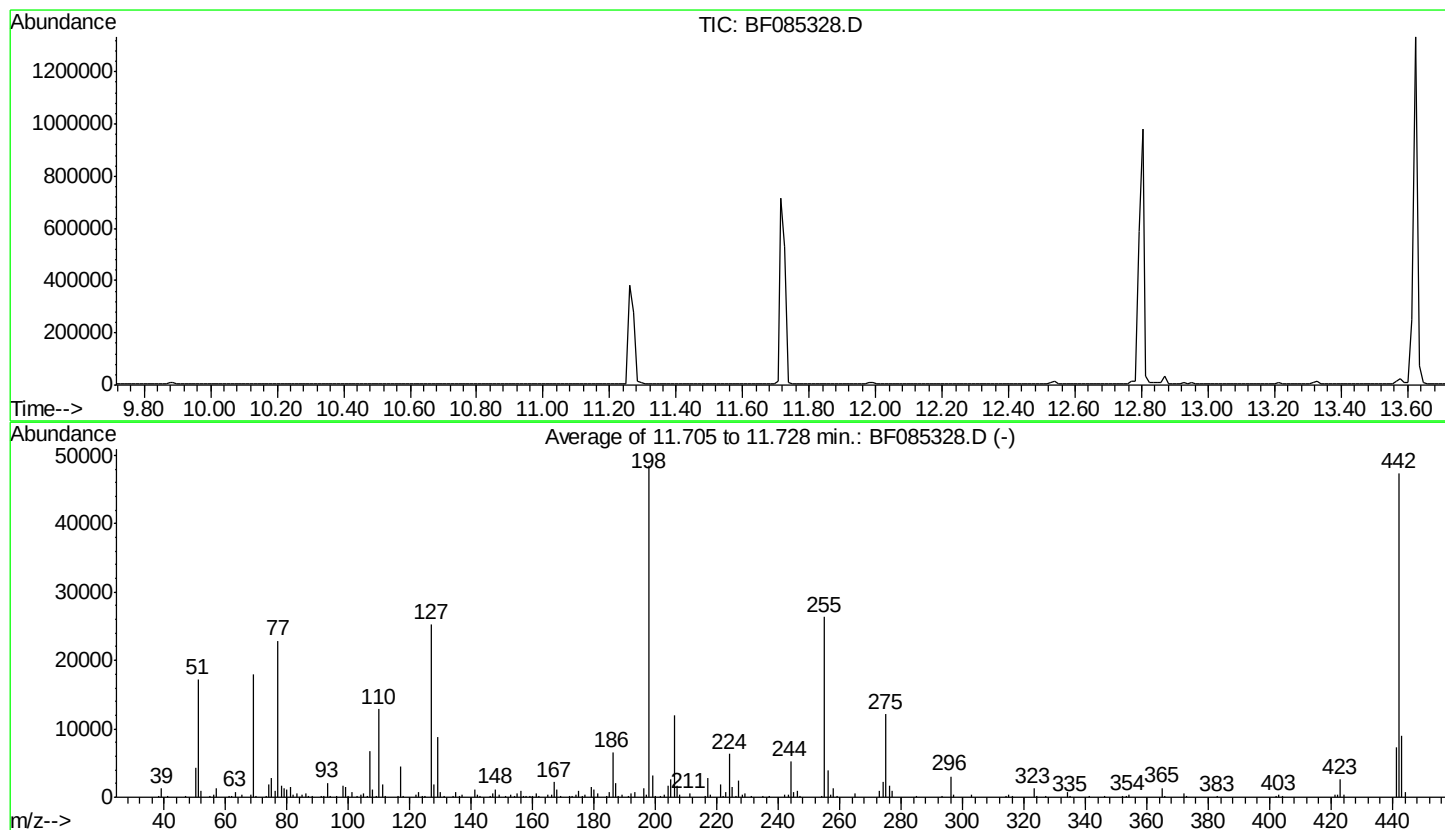

AutoFind: Scans 824, 825, 826; Background Corrected with Scan 821

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	17150	PASS
68	69	0.00	2	1.7	312	PASS
69	198	0.00	100	37.1	17986	PASS
70	69	0.00	2	0.6	100	PASS
127	198	10	80	52.1	25246	PASS
197	198	0.00	2	0.7	319	PASS
198	198	100	100	100.0	48478	PASS
199	198	5	9	6.6	3222	PASS
275	198	10	60	25.0	12132	PASS
365	198	1	100	2.8	1378	PASS
441	442	0.01	24	15.5	7358	PASS
442	198	50	100	97.9	47441	PASS
443	442	15	24	18.8	8931	PASS