

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031017\
 Data File : BF093534.D
 Acq On : 10 Mar 2017 20:51
 Operator : SJ/MA
 Sample : I2172-26
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 D-51

Quant Time: Mar 10 22:18:11 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 07 15:55:22 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.74	152	173424	20.00	ng	-0.02
21) Naphthalene-d8	8.02	136	730625	20.00	ng	-0.03
38) Acenaphthene-d10	9.77	164	341447	20.00	ng	-0.03
63) Phenanthrene-d10	11.26	188	632864	20.00	ng	-0.02
75) Chrysene-d12	13.90	240	540661	20.00	ng	-0.02
86) Perylene-d12	15.31	264	360672	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.36	112	1397964	134.16	ng	0.01
7) Phenol-d6	6.41	99	1704784	129.74	ng	0.00
23) Nitrobenzene-d5	7.32	82	1161521	88.21	ng	-0.02
41) 2,4,6-Tribromophenol	10.57	330	350702	157.65	ng	-0.02
44) 2-Fluorobiphenyl	9.10	172	1656248	90.22	ng	-0.03
78) Terphenyl-d14	12.85	244	1664897	80.06	ng	-0.02
Target Compounds						
9) Benzaldehyde	6.41	77	2614	Below Cal	#	1
19) n-Nitroso-di-n-propylamine	7.32	70	155094	17.17	ng	# 80
25) Isophorone	7.32	82	1163673	43.82	ng	# 65
50) 2,6-Dinitrotoluene	9.77	165	43933	8.84	ng	# 31
56) 2,4-Dinitrotoluene	9.77	165	43934	7.20	ng	# 20
66) 4-Bromophenyl-phenylether	10.57	248	26194	3.91	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031017\
Data File : BF093534.D
Acq On : 10 Mar 2017 20:51
Operator : SJ/MA
Sample : I2172-26
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
D-51

Quant Time: Mar 10 22:18:11 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 15:55:22 2017
Response via : Initial Calibration

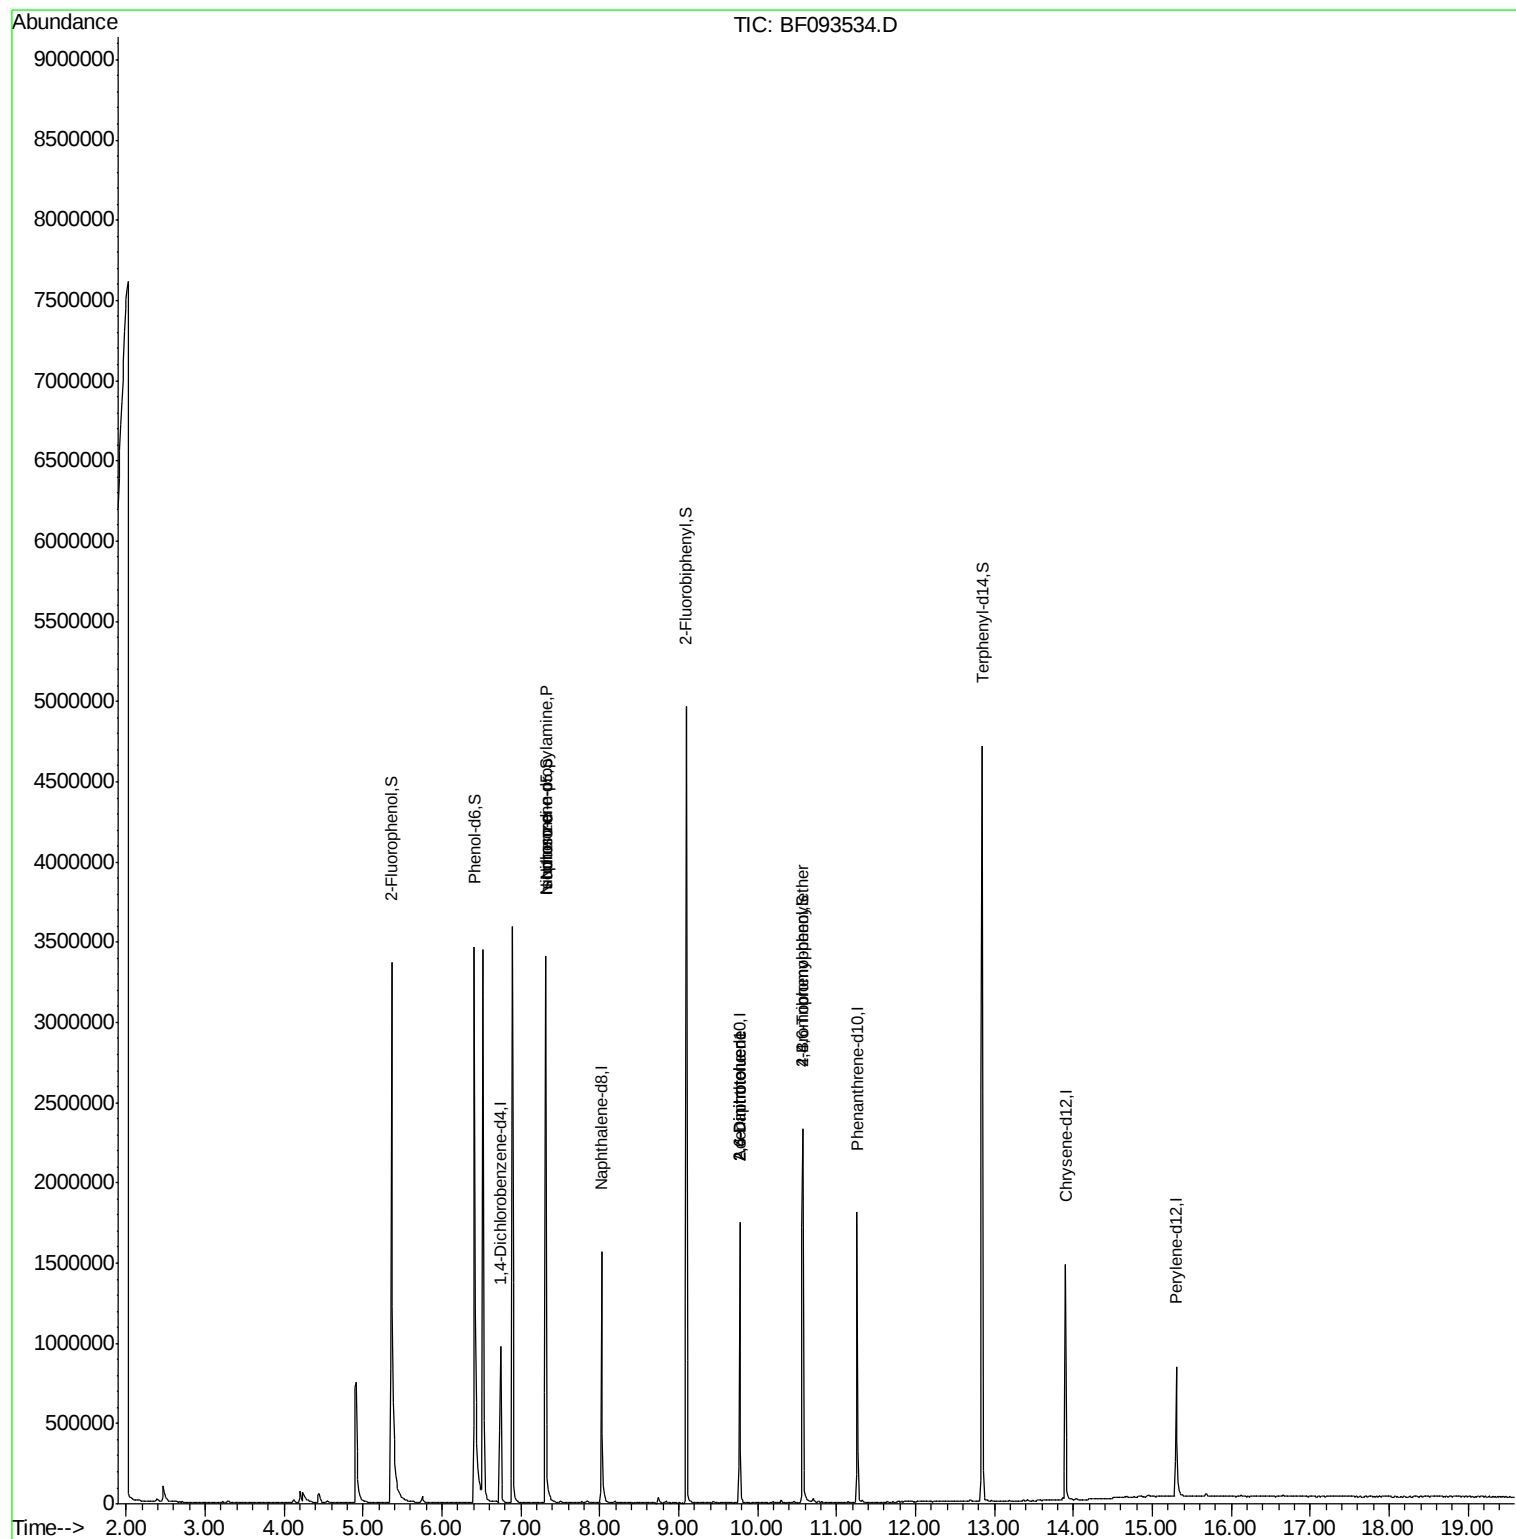




#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.74 min Scan# 425
Delta R.T. -0.02 min
Lab File: BF093534.D
Acq: 10 Mar 2017 20:51

Instrument :
BNA_F
ClientSampleID :
D-51

Tot Ion:152 Resp: 173424
Ion Ratio Lower Upper
152 100
150 157.5 124.9 187.3
115 56.0 46.0 69.0

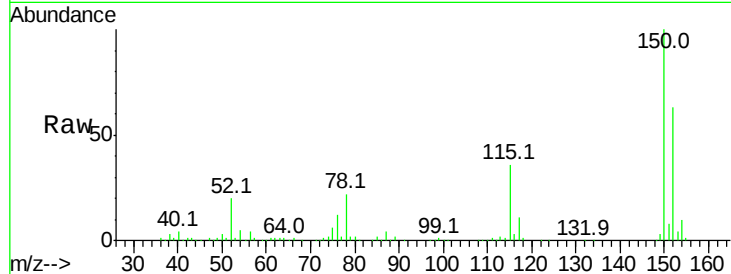


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

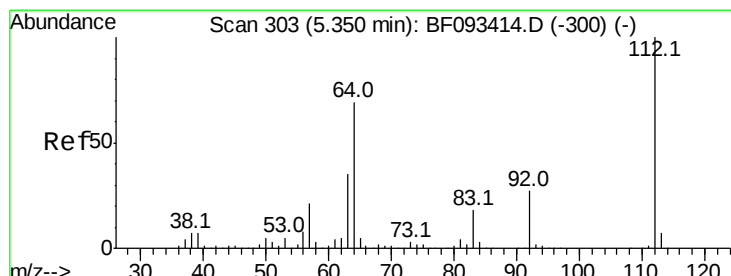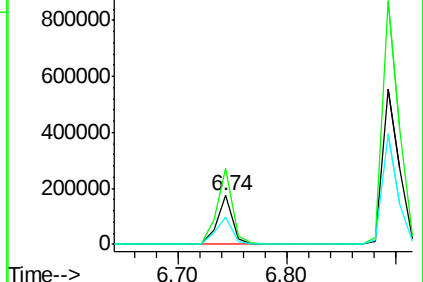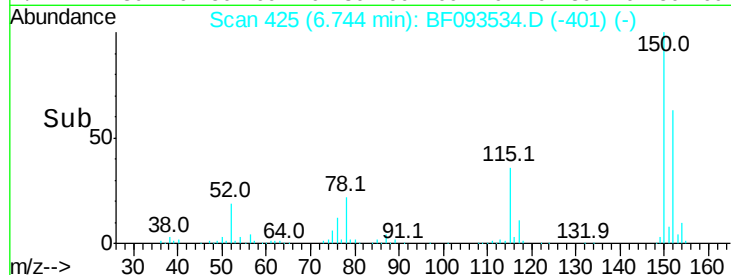



#5


2-Fluorophenol
Concen: 134.16 ng
RT: 5.36 min Scan# 304
Delta R.T. 0.01 min
Lab File: BF093534.D
Acq: 10 Mar 2017 20:51

Tgt Ion:112 Resp: 1397964
Ion Ratio Lower Upper
112 100
64 61.5 46.1 69.1
63 31.4 23.8 35.6

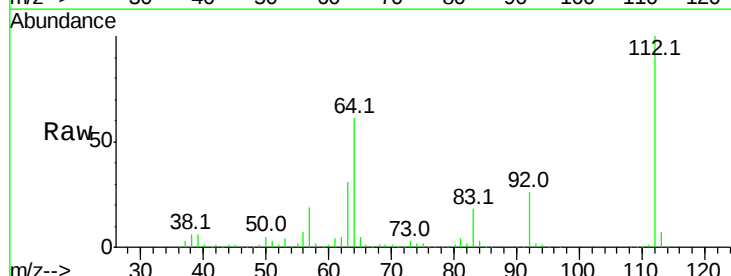

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

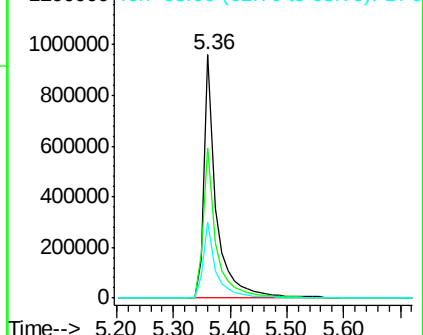

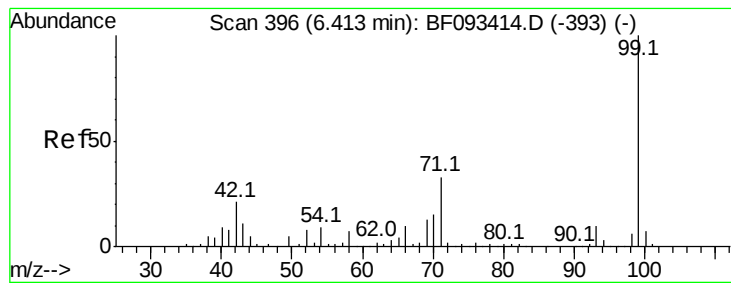

#7

Phenol-d6

Concen: 129.74 ng

RT: 6.41 min Scan# 396

Delta R.T. -0.00 min

Lab File: BF093534.D

Acq: 10 Mar 2017 20:51

Instrument :

BNA_F

ClientSampleId :

D-51


Tot Ion: 99 Resp: 1704784

Ion Ratio Lower Upper

99 100

42 19.2 15.6 23.4




71 32.2 27.5 41.3



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

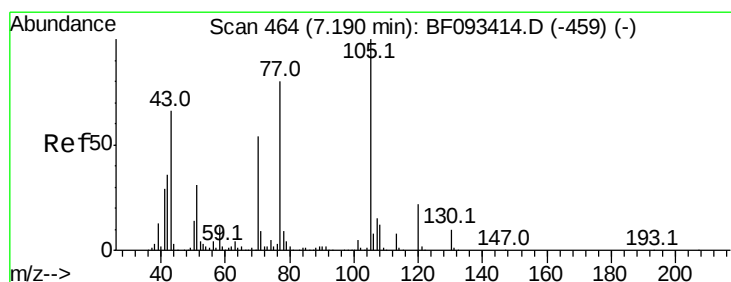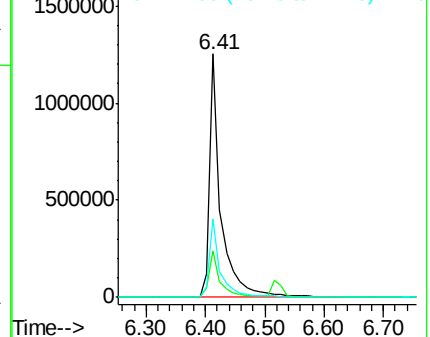

#19

n-Nitroso-di-n-propylamine

Concen: 17.17 ng

RT: 7.32 min Scan# 475

Delta R.T. 0.13 min

Lab File: BF093534.D

Acq: 10 Mar 2017 20:51

Tgt Ion: 70 Resp: 155094


Ion Ratio Lower Upper

70 100

42 50.5 49.4 74.0

101 0.0 7.4 11.2#

130 1.9 14.2 21.4#


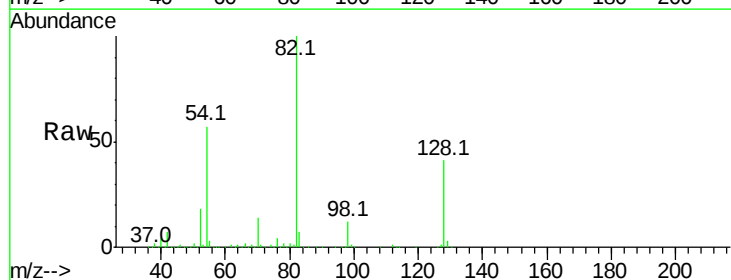



Abundance Ion 70.00 (69.70 to 70.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 101.00 (100.70 to 101.70): BF0

Ion 130.00 (129.70 to 130.70): BF0



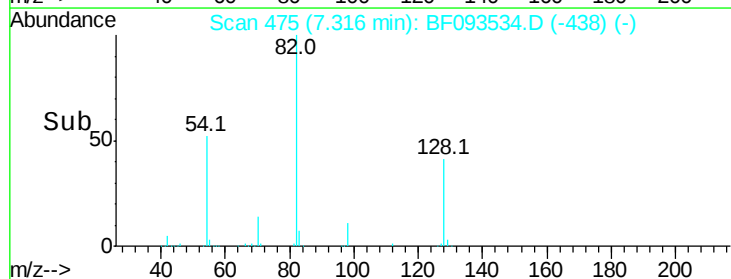
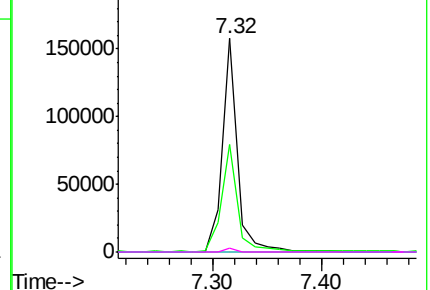


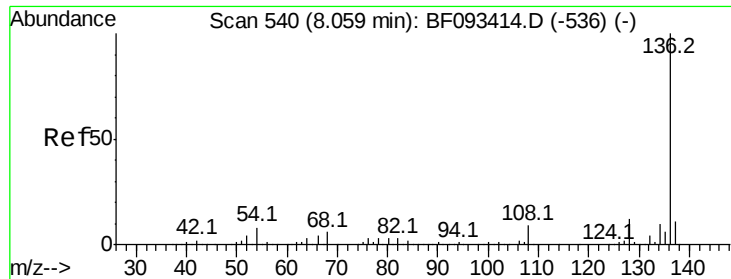

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.02 min Scan# 537
Delta R.T. -0.03 min
Lab File: BF093534.D
Acq: 10 Mar 2017 20:51




Instrument :
BNA_F
ClientSampleId :
D-51


Tot Ion:	136	Resp:	730625
Ion	Ratio	Lower	Upper
136	100		
137	11.2	8.4	12.6
54	11.1	4.5	6.7#
68	7.8	3.6	5.4#

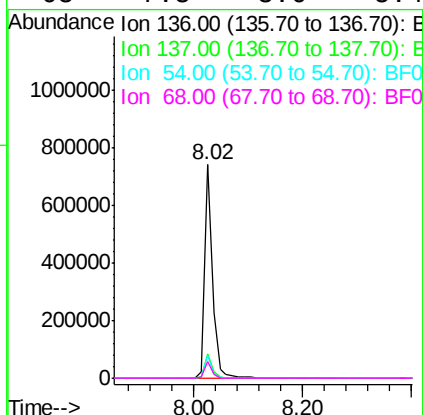

#23
Nitrobenzene-d5
Concen: 88.21 ng
RT: 7.32 min Scan# 475
Delta R.T. -0.02 min
Lab File: BF093534.D
Acq: 10 Mar 2017 20:51

Tgt Ion:	82	Resp:	1161521
Ion	Ratio	Lower	Upper
82	100		
128	41.3	34.6	52.0
54	57.0	39.5	59.3

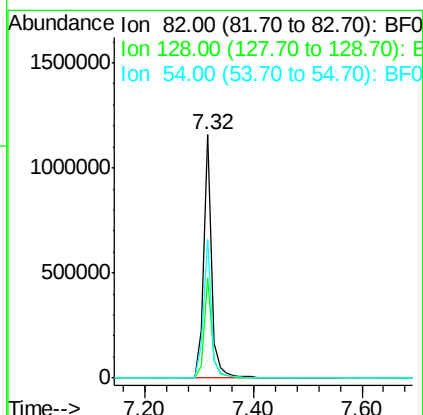



#25

Isophorone

Concen: 43.82 ng

RT: 7.32 min Scan# 475

Delta R.T. -0.29 min

Lab File: BF093534.D

Acq: 10 Mar 2017 20:51

Instrument :

BNA_F

ClientSampleId :

D-51





Tot Ion: 82 Resp: 1163673

Ion Ratio Lower Upper

82 100

95 0.0 5.6 8.4#

138 0.0 14.6 22.0#

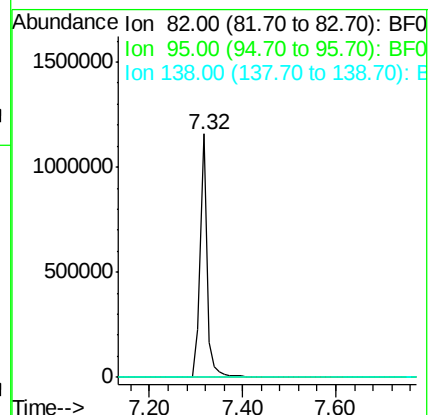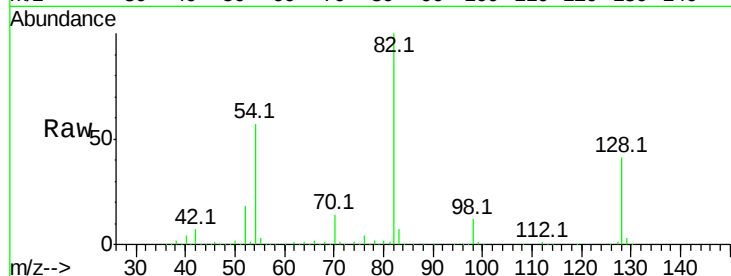

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.77 min Scan# 690

Delta R.T. -0.03 min

Lab File: BF093534.D

Acq: 10 Mar 2017 20:51




Tgt Ion:164 Resp: 341447


Ion Ratio Lower Upper

164 100

162 100.9 80.2 120.2

160 45.3 36.9 55.3

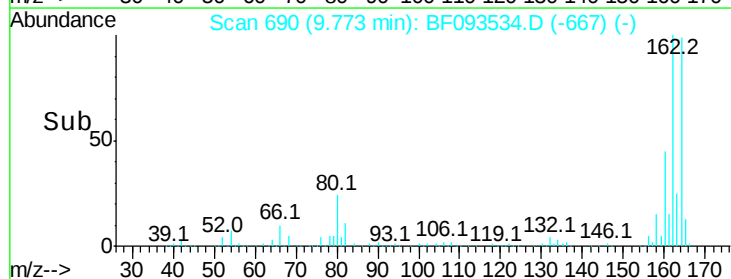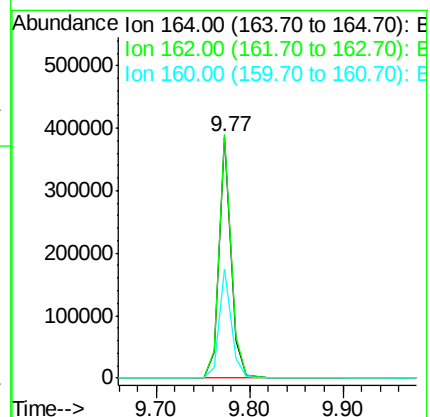


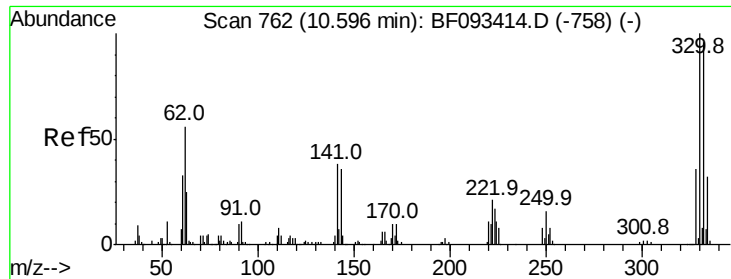




#41
 2,4,6-Tribromophenol
 Concen: 157.65 ng
 RT: 10.57 min Scan# 760
 Delta R.T. -0.02 min
 Lab File: BF093534.D
 Acq: 10 Mar 2017 20:51

Instrument :
 BNA_F
 ClientSampled :
 D-51

Tot Ion:330 Resp: 350702
 Ion Ratio Lower Upper
 330 100
 332 96.2 77.4 116.2
 141 40.4 34.1 51.1




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


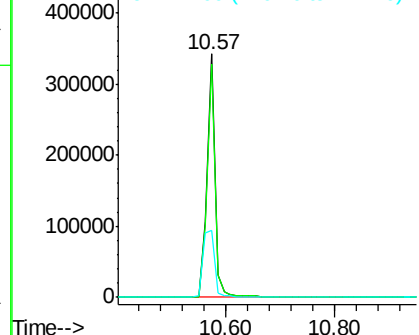



#44
 2-Fluorobiphenyl
 Concen: 90.22 ng
 RT: 9.10 min Scan# 631
 Delta R.T. -0.03 min
 Lab File: BF093534.D
 Acq: 10 Mar 2017 20:51

Tgt Ion:172 Resp: 1656248
 Ion Ratio Lower Upper
 172 100
 171 36.8 29.4 44.0
 170 24.7 20.2 30.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E




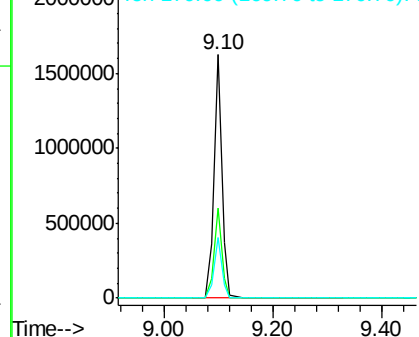


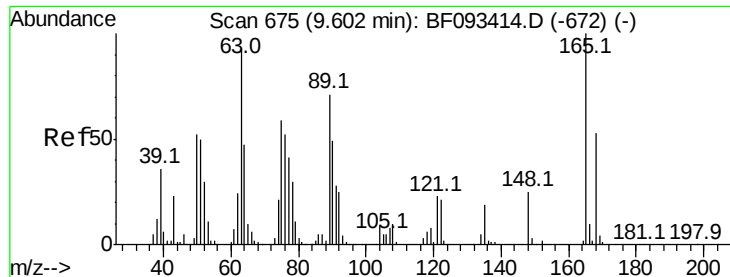

#50
2,6-Dinitrotoluene
Concen: 8.84 ng
RT: 9.77 min Scan# 690
Delta R.T. 0.17 min
Lab File: BF093534.D
Acq: 10 Mar 2017 20:51




Instrument :
BNA_F
ClientSampleId :
D-51


Tot Ion:165 Resp: 43933
Ion Ratio Lower Upper
165 100
63 1.0 36.2 54.4#
89 1.1 40.2 60.4#

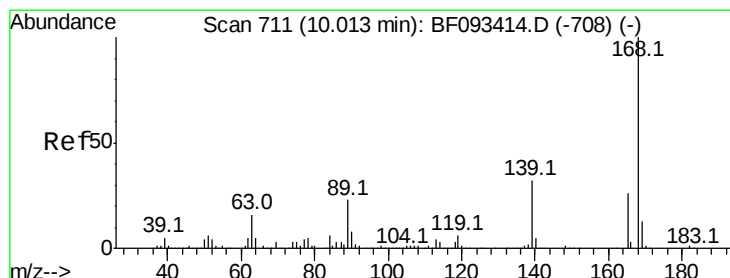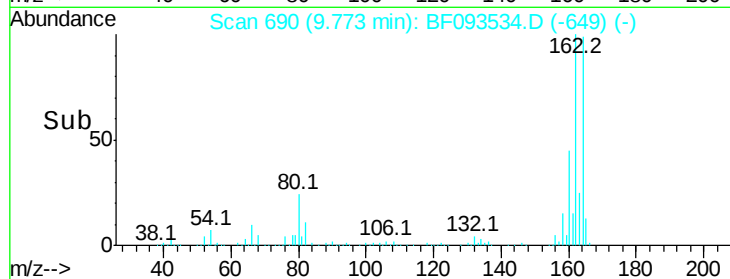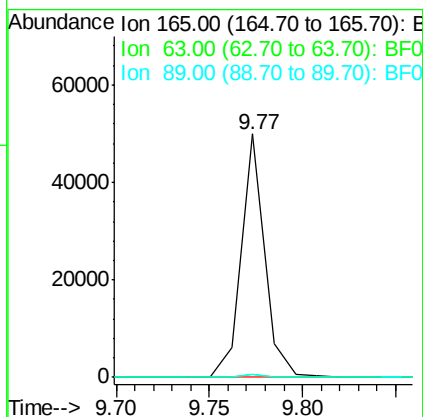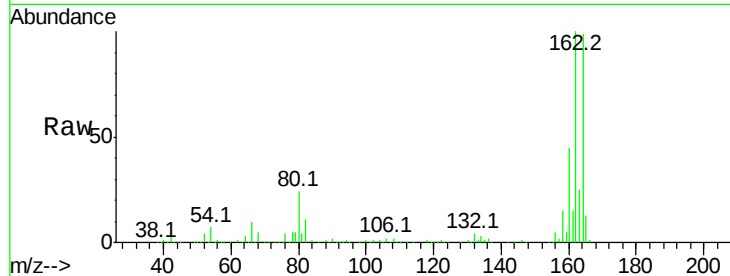

#56
2,4-Dinitrotoluene
Concen: 7.20 ng
RT: 9.77 min Scan# 690
Delta R.T. -0.24 min
Lab File: BF093534.D
Acq: 10 Mar 2017 20:51

Tgt Ion:165 Resp: 43934
Ion Ratio Lower Upper
165 100
63 1.0 40.2 60.4#
89 1.1 62.5 93.7#
182 0.0 1.8 2.8#

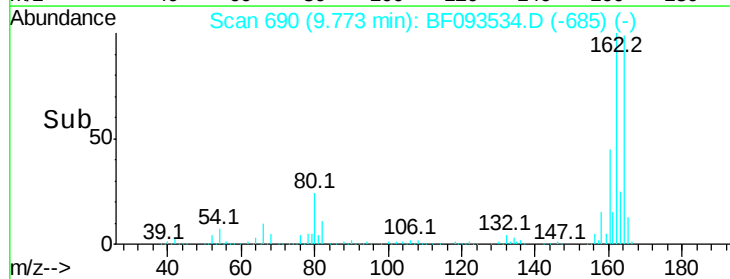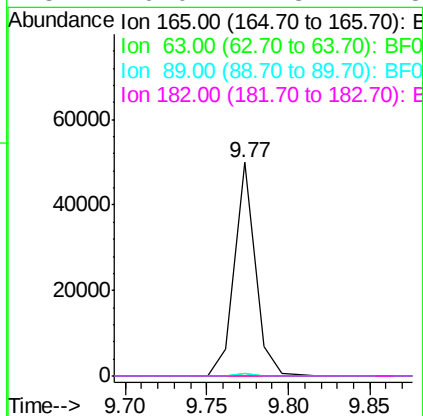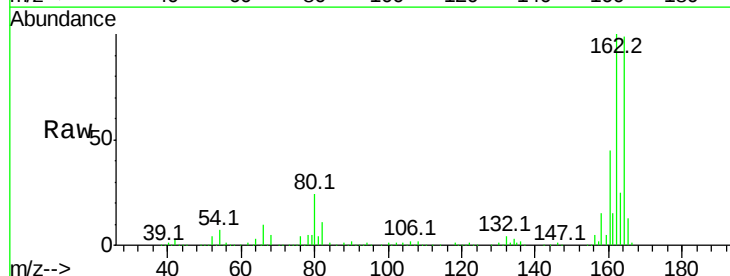


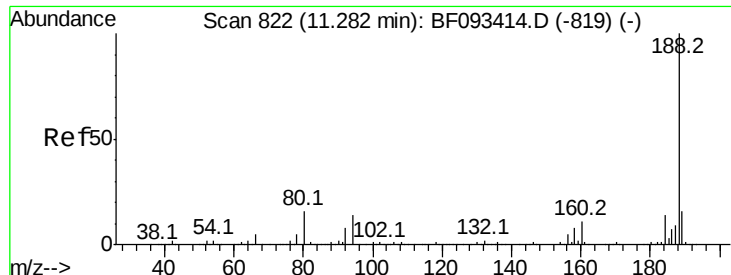




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.26 min Scan# 820
Delta R.T. -0.02 min
Lab File: BF093534.D
Acq: 10 Mar 2017 20:51

Instrument :
BNA_F
ClientSampleId :
D-51

Tot Ion:188 Resp: 632864
Ion Ratio Lower Upper
188 100
94 11.4 10.0 15.0
80 12.4 11.2 16.8

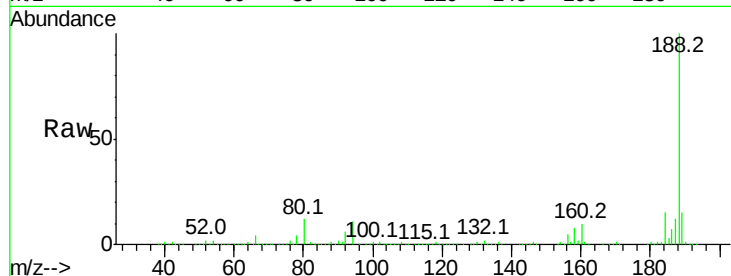


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

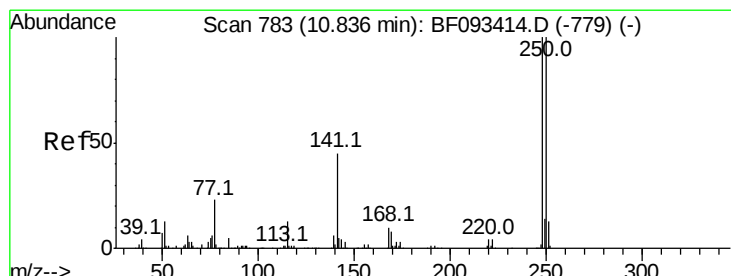
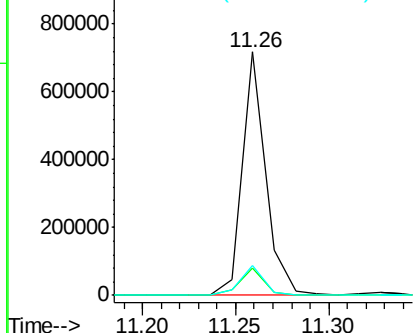



#66
4-Bromophenyl-phenylether
Concen: 3.91 ng
RT: 10.57 min Scan# 760
Delta R.T. -0.26 min
Lab File: BF093534.D
Acq: 10 Mar 2017 20:51

Tgt Ion:248 Resp: 26194
Ion Ratio Lower Upper
248 100
250 196.1 76.9 115.3#
141 395.6 68.2 102.4#

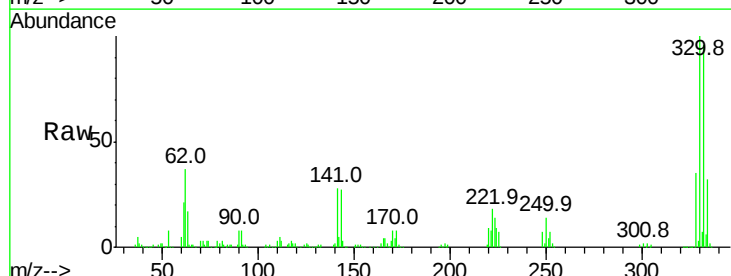

Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

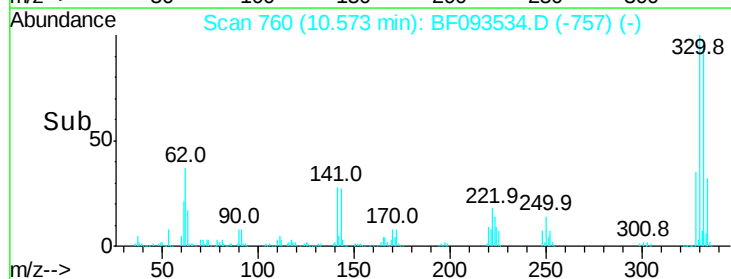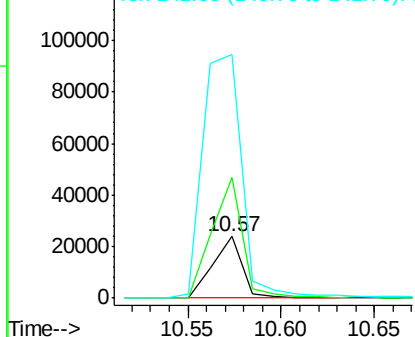



#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.90 min Scan# 1051

Delta R.T. -0.02 min

Lab File: BF093534.D

Acq: 10 Mar 2017 20:51

Instrument :

BNA_F

ClientSampleId :

D-51


Tot Ion:240 Resp: 540661

Ion Ratio Lower Upper

240 100

120 13.8 12.9 19.3




236 25.7 20.9 31.3



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

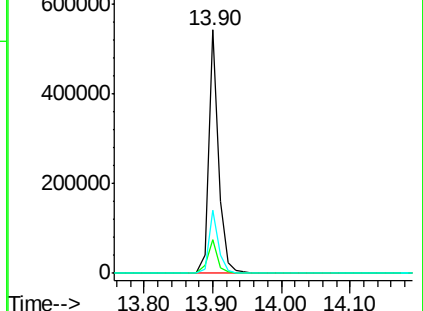

#78

Terphenyl-d14

Concen: 80.06 ng

RT: 12.85 min Scan# 959

Delta R.T. -0.02 min

Lab File: BF093534.D

Acq: 10 Mar 2017 20:51


Tgt Ion:244 Resp: 1664897

Ion Ratio Lower Upper

244 100

212 7.8 6.2 9.2



122 12.3 11.4 17.2




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

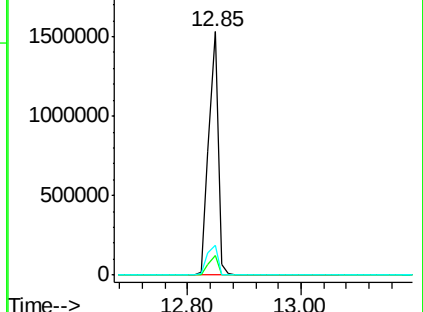

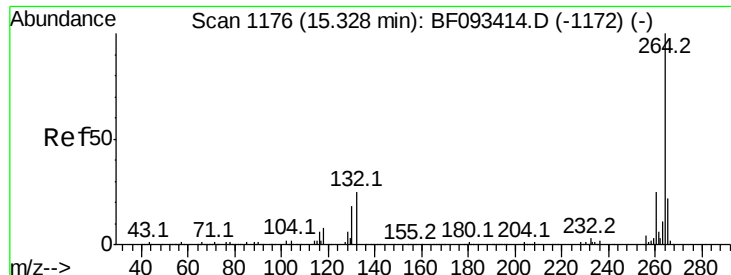


#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.31 min Scan# 1174
Delta R.T. -0.02 min
Lab File: BF093534.D
Acq: 10 Mar 2017 20:51

Instrument :
BNA_F
ClientSampleId :
D-51

Tot Ion: 264 Resp: 360672

Ion	Ratio	Lower	Upper
264	100		
260	24.5	19.2	28.8
265	21.4	17.4	26.0

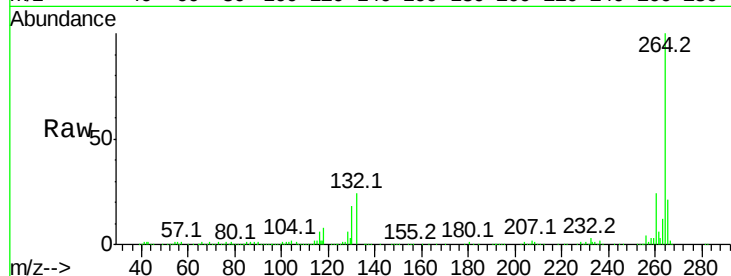

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

