

Data Path : Z:\HPCHEM1\BNA F\Data\BF031017\
 Data File : BF093555.D
 Acq On : 11 Mar 2017 6:45
 Operator : SJ/MA
 Sample : I2195-05
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Mar 13 14:02:02 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 07 15:55:22 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.74	152	176971	20.00	ng	-0.02
21) Naphthalene-d8	8.02	136	726507	20.00	ng	-0.03
38) Acenaphthene-d10	9.77	164	338514	20.00	ng	-0.03
63) Phenanthrene-d10	11.26	188	638031	20.00	ng	-0.02
75) Chrysene-d12	13.90	240	485554	20.00	ng	-0.02
86) Perylene-d12	15.31	264	248631	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.36	112	1361569	128.05	ng	0.01
7) Phenol-d6	6.41	99	1680166	125.30	ng	0.00
23) Nitrobenzene-d5	7.32	82	1209887	92.40	ng	-0.02
41) 2,4,6-Tribromophenol	10.57	330	339053	153.73	ng	-0.02
44) 2-Fluorobiphenyl	9.10	172	1667312	91.61	ng	-0.03
78) Terphenyl-d14	12.85	244	1697043	90.87	ng	-0.02
Target Compounds						
9) Benzaldehyde	6.41	77	2528	Below Cal	#	14
19) n-Nitroso-di-n-propylamine	7.32	70	161452	17.51	ng	# 82
25) Isophorone	7.32	82	1211705	45.89	ng	# 65
50) 2,6-Dinitrotoluene	9.77	165	42207	8.57	ng	# 31
56) 2,4-Dinitrotoluene	9.77	165	42200	6.98	ng	# 20
66) 4-Bromophenyl-phenylether	10.57	248	25063	3.71	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\Data\BF031017\
Data File : BF093555.D
Acq On : 11 Mar 2017 6:45
Operator : SJ/MA
Sample : I2195-05
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Mar 13 14:02:02 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 15:55:22 2017
Response via : Initial Calibration

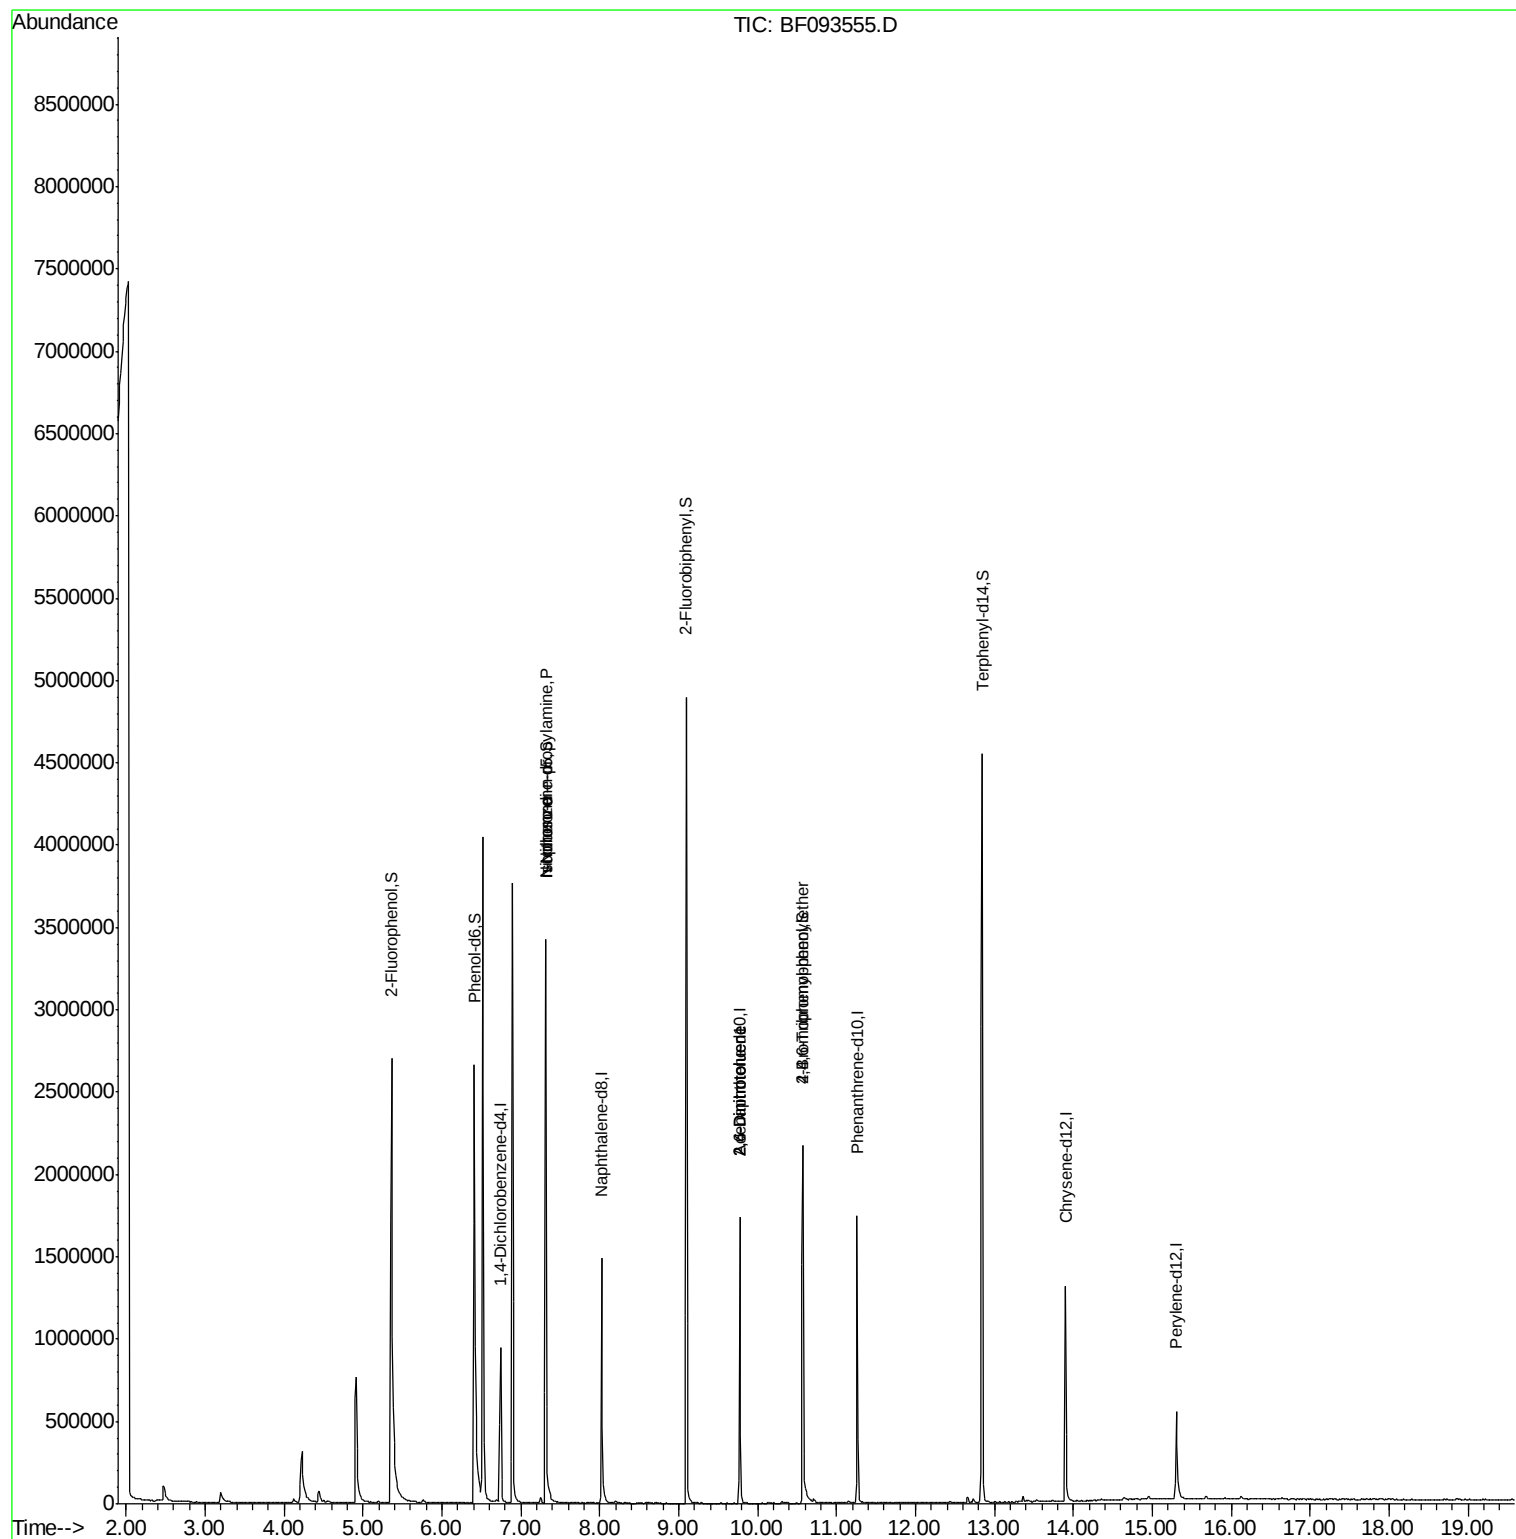

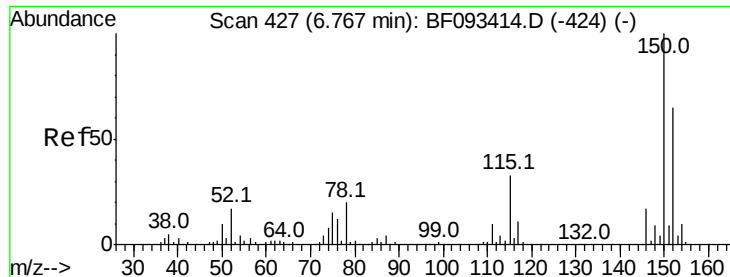

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.74 min Scan# 425

Delta R.T. -0.02 min

Lab File: BF093555.D

Acq: 11 Mar 2017 6:45

Instrument :

BNA_F

ClientSampleId :


Tot Ion:152 Resp: 176971

Ion Ratio Lower Upper

152 100

150 155.5 124.9 187.3




115 54.8 46.0 69.0

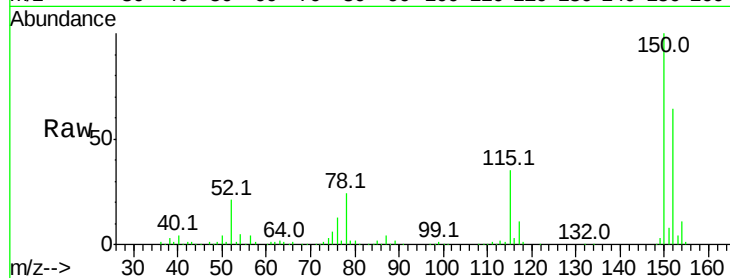

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

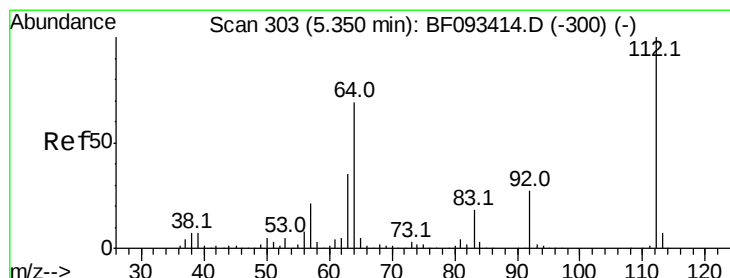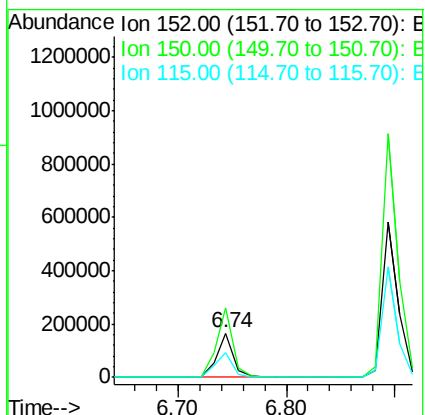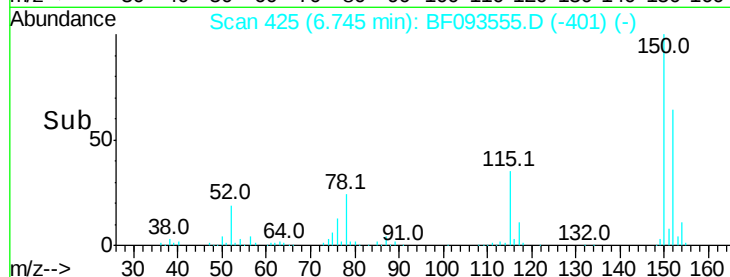

#5

2-Fluorophenol

Concen: 128.05 ng

RT: 5.36 min Scan# 304

Delta R.T. 0.01 min

Lab File: BF093555.D

Acq: 11 Mar 2017 6:45


Tgt Ion:112 Resp: 1361569

Ion Ratio Lower Upper

112 100

64 59.6 46.1 69.1



63 30.6 23.8 35.6

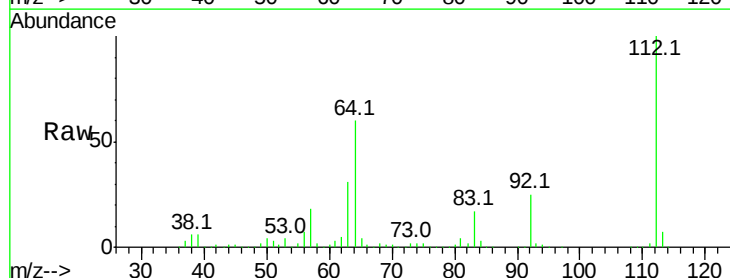


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

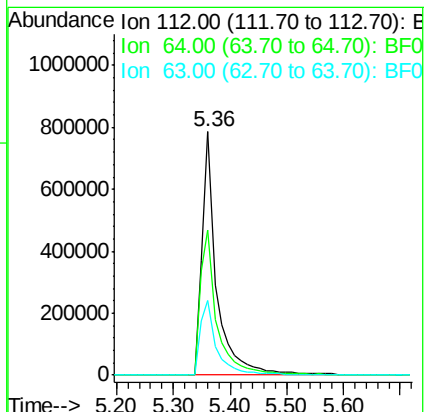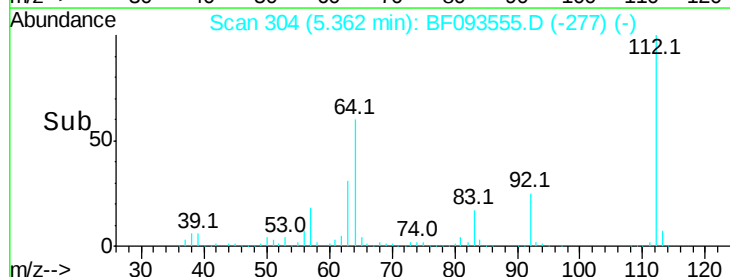

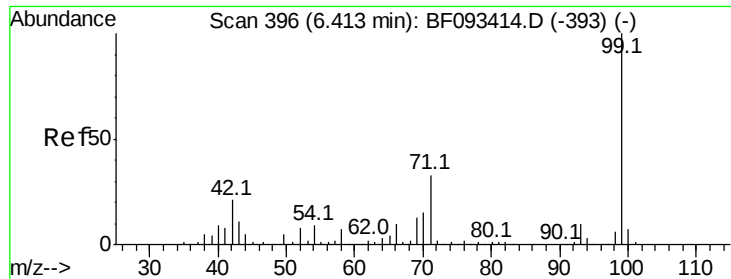

#7

Phenol-d6

Concen: 125.30 ng

RT: 6.41 min Scan# 396

Delta R.T. 0.00 min

Lab File: BF093555.D

Acq: 11 Mar 2017 6:45

Instrument :

BNA_F

ClientSampled :


Tot Ion: 99 Resp: 1680166

Ion Ratio Lower Upper

99 100

42 17.5 15.6 23.4




71 30.0 27.5 41.3



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

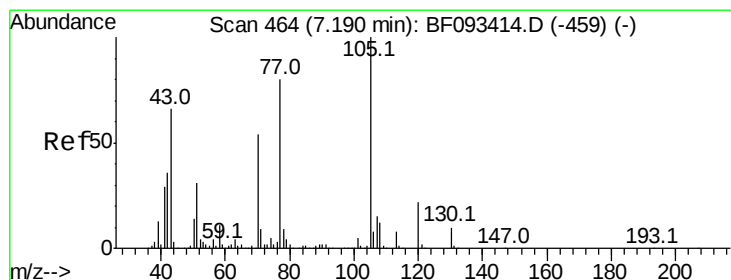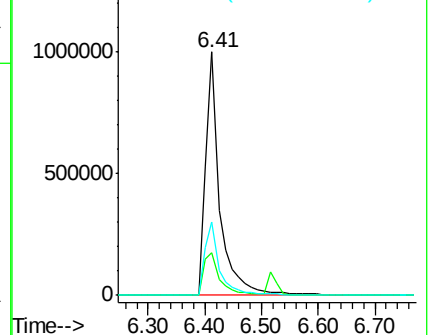

#19

n-Nitroso-di-n-propylamine

Concen: 17.51 ng

RT: 7.32 min Scan# 475

Delta R.T. 0.13 min

Lab File: BF093555.D

Acq: 11 Mar 2017 6:45

Tgt Ion: 70 Resp: 161452


Ion Ratio Lower Upper

70 100

42 52.6 49.4 74.0

101 0.0 7.4 11.2#

130 1.8 14.2 21.4#






Abundance Ion 70.00 (69.70 to 70.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 101.00 (100.70 to 101.70): BF0

Ion 130.00 (129.70 to 130.70): BF0

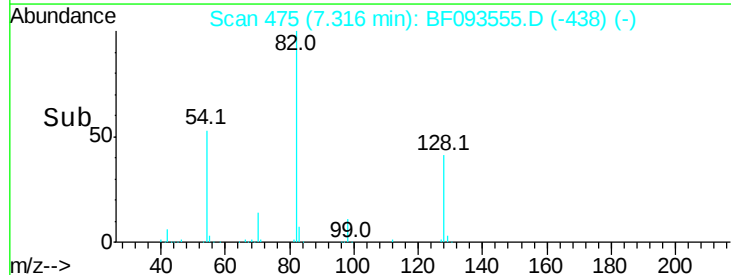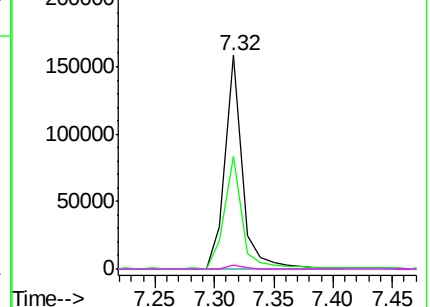


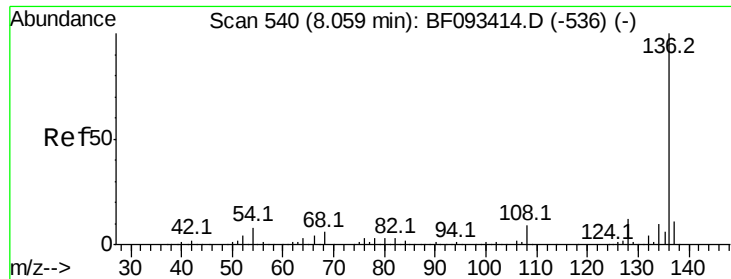




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.02 min Scan# 537
Delta R.T. -0.03 min
Lab File: BF093555.D
Acq: 11 Mar 2017 6:45

Instrument :
BNA_F
ClientSampleId :

Tot Ion:	136	Resp:	726507
Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.4	12.6
54	11.3	4.5	6.7#
68	8.3	3.6	5.4#

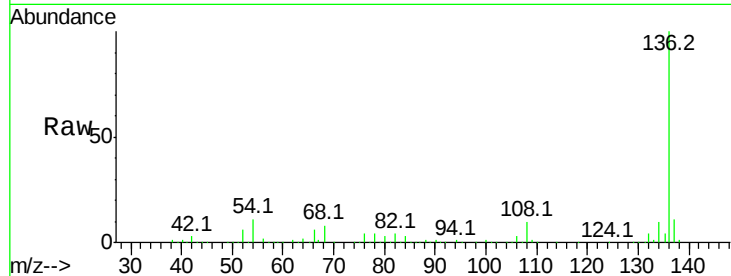


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

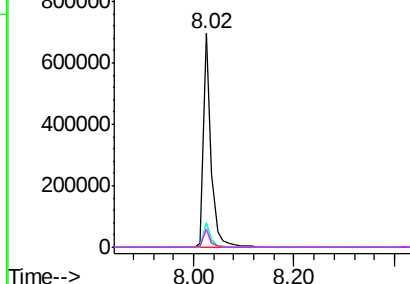




#23
Nitrobenzene-d5
Concen: 92.40 ng
RT: 7.32 min Scan# 475
Delta R.T. -0.02 min
Lab File: BF093555.D
Acq: 11 Mar 2017 6:45

Tgt Ion:	82	Resp:	1209887
Ion	Ratio	Lower	Upper
82	100		
128	41.0	34.6	52.0
54	57.9	39.5	59.3



Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

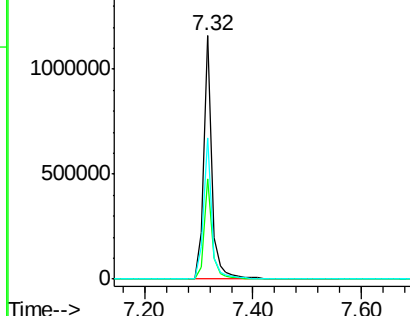



#25

Isophorone

Concen: 45.89 ng

RT: 7.32 min Scan# 475

Delta R.T. -0.29 min

Lab File: BF093555.D

Acq: 11 Mar 2017 6:45

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 1211705

Ion Ratio Lower Upper




82 100

95 0.0 5.6 8.4#

138 0.0 14.6 22.0#

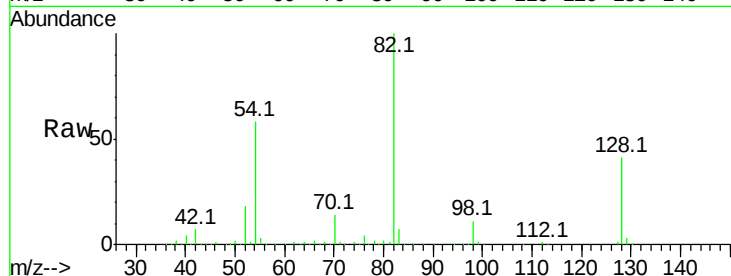

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 95.00 (94.70 to 95.70): BF0
Ion 138.00 (137.70 to 138.70): E

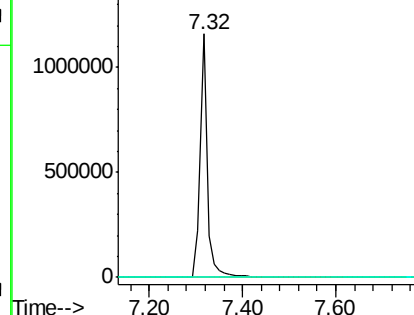

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.77 min Scan# 690

Delta R.T. -0.03 min

Lab File: BF093555.D

Acq: 11 Mar 2017 6:45


Tgt Ion: 164 Resp: 338514

Ion Ratio Lower Upper



164 100


162 103.2 80.2 120.2

160 45.0 36.9 55.3



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

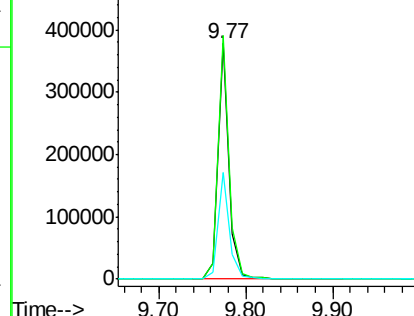







#41
 2,4,6-Tribromophenol
 Concen: 153.73 ng
 RT: 10.57 min Scan# 760
 Delta R.T. -0.02 min
 Lab File: BF093555.D
 Acq: 11 Mar 2017 6:45

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:330 Resp: 339053
 Ion Ratio Lower Upper
 330 100
 332 95.7 77.4 116.2
 141 40.6 34.1 51.1

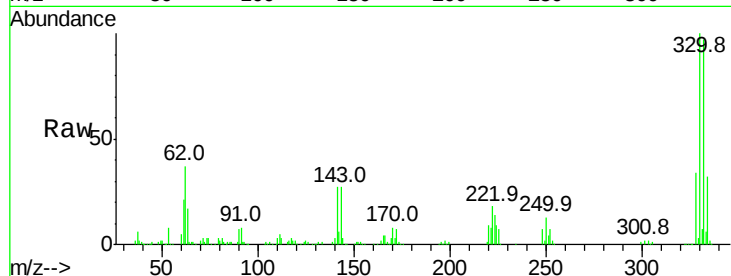


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


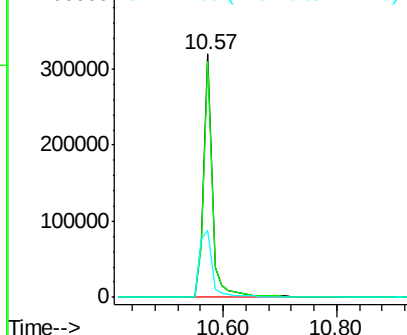



#44
 2-Fluorobiphenyl
 Concen: 91.61 ng
 RT: 9.10 min Scan# 631
 Delta R.T. -0.03 min
 Lab File: BF093555.D
 Acq: 11 Mar 2017 6:45

Tgt Ion:172 Resp: 1667312
 Ion Ratio Lower Upper
 172 100
 171 36.9 29.4 44.0
 170 25.1 20.2 30.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E




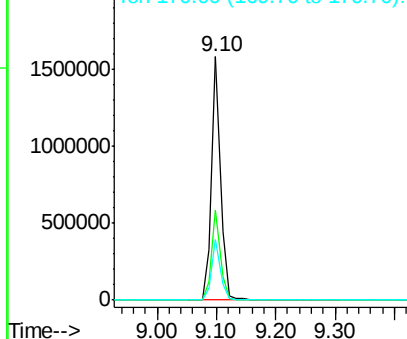


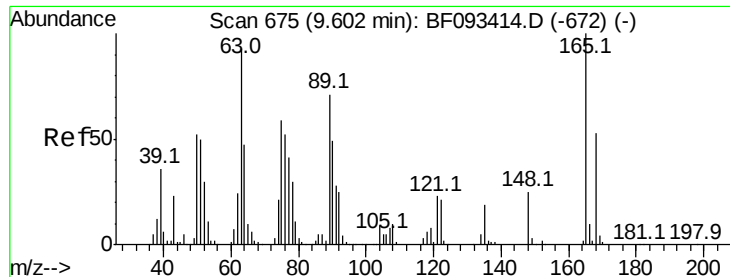

#50
2,6-Dinitrotoluene
Concen: 8.57 ng
RT: 9.77 min Scan# 690
Delta R.T. 0.17 min
Lab File: BF093555.D
Acq: 11 Mar 2017 6:45




Instrument :
BNA_F
ClientSampleId :


Tot Ion:165 Resp: 42207
Ion Ratio Lower Upper
165 100
63 1.4 36.2 54.4#
89 1.4 40.2 60.4#

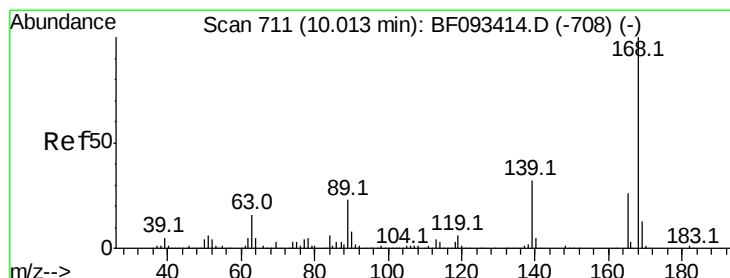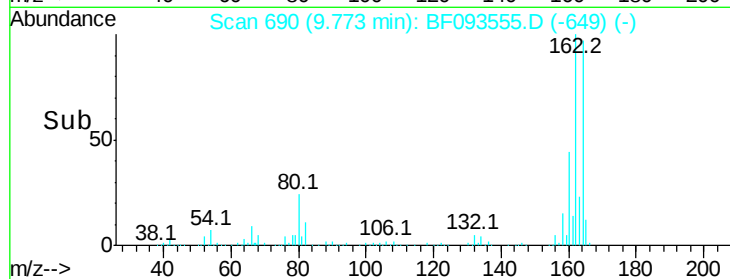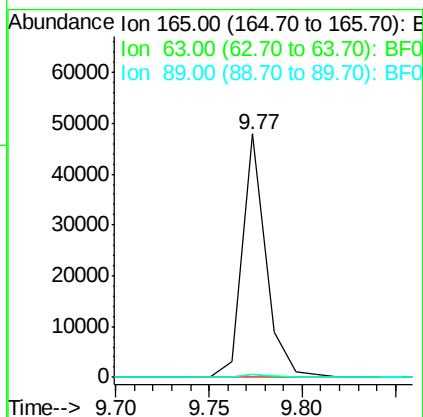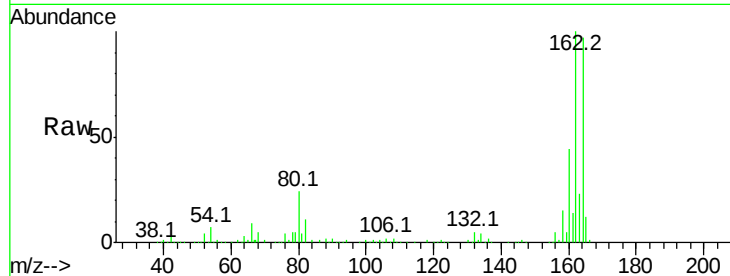

#56
2,4-Dinitrotoluene
Concen: 6.98 ng
RT: 9.77 min Scan# 690
Delta R.T. -0.24 min
Lab File: BF093555.D
Acq: 11 Mar 2017 6:45

Tgt Ion:165 Resp: 42200
Ion Ratio Lower Upper
165 100
63 1.4 40.2 60.4#
89 1.4 62.5 93.7#
182 0.0 1.8 2.8#

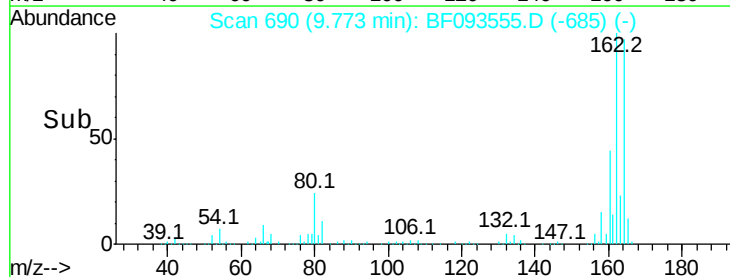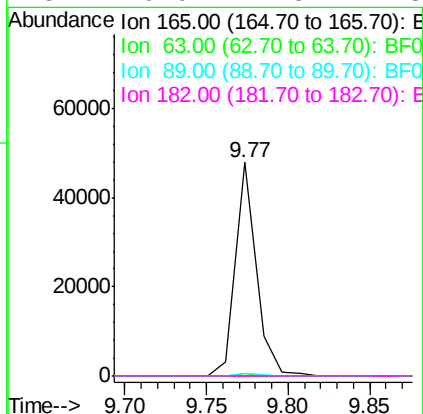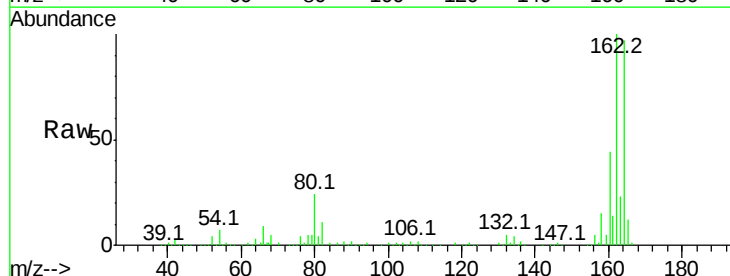


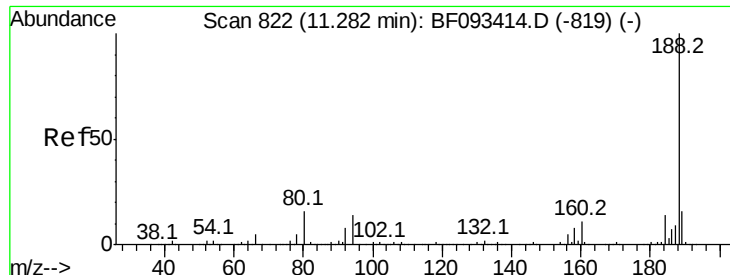




#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.26 min Scan# 820
 Delta R.T. -0.02 min
 Lab File: BF093555.D
 Acq: 11 Mar 2017 6:45

Instrument :
 BNA_F
 ClientSampled :

Tot Ion:188 Resp: 638031
 Ion Ratio Lower Upper
 188 100
 94 11.9 10.0 15.0
 80 12.9 11.2 16.8

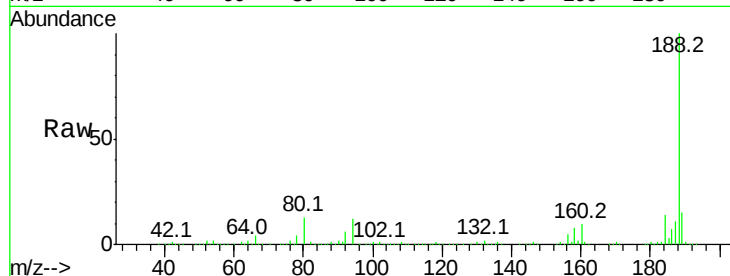


Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF0
 Ion 80.00 (79.70 to 80.70): BF0

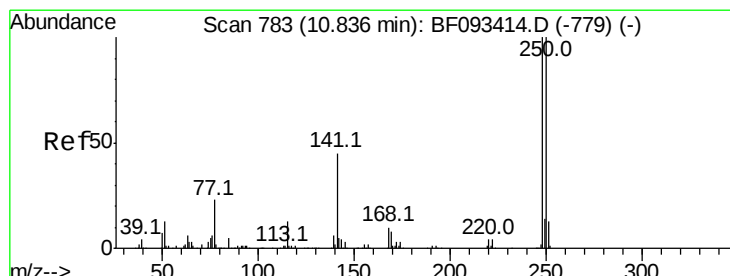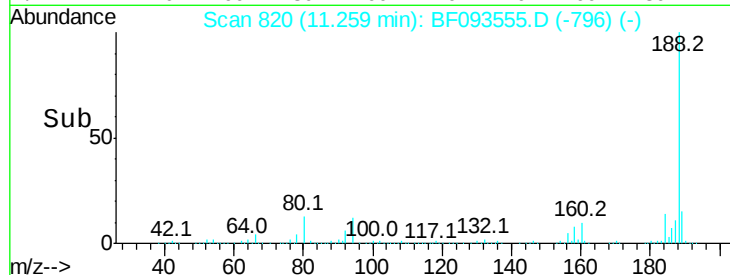
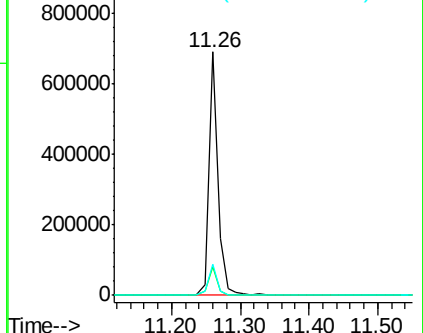



#66
 4-Bromophenyl-phenylether
 Concen: 3.71 ng
 RT: 10.57 min Scan# 760
 Delta R.T. -0.26 min
 Lab File: BF093555.D
 Acq: 11 Mar 2017 6:45

Tgt Ion:248 Resp: 25063
 Ion Ratio Lower Upper
 248 100
 250 199.7 76.9 115.3#
 141 408.2 68.2 102.4#

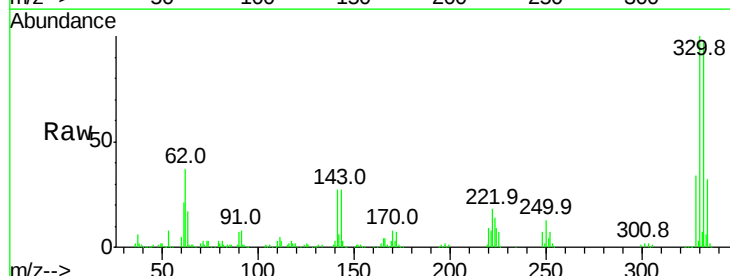

Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

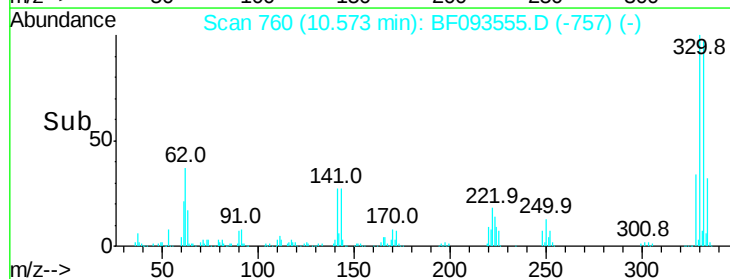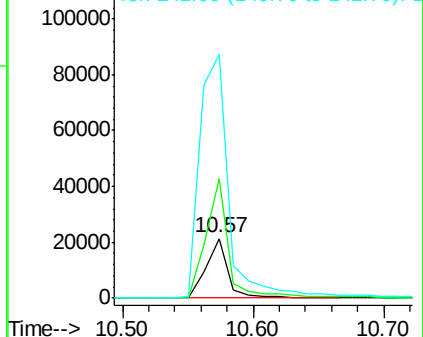

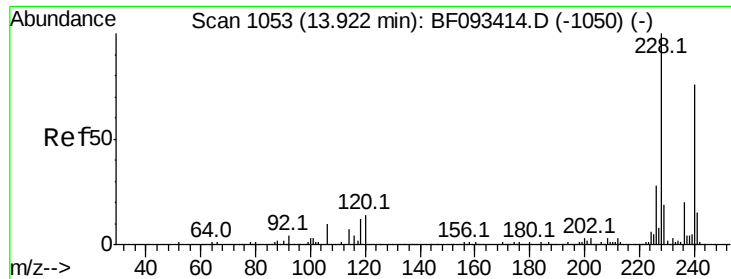

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.90 min Scan# 1051

Delta R.T. -0.02 min

Lab File: BF093555.D

Acq: 11 Mar 2017 6:45

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 485554

Ion Ratio Lower Upper

240 100

120 14.6 12.9 19.3




236 26.4 20.9 31.3

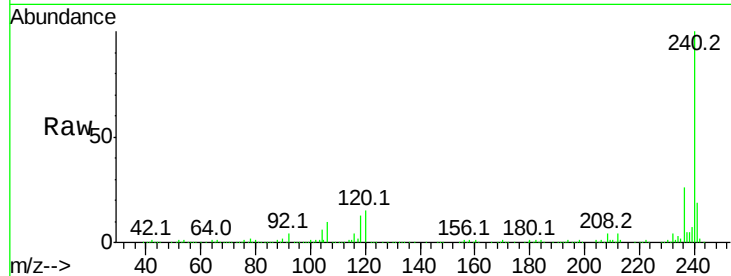

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

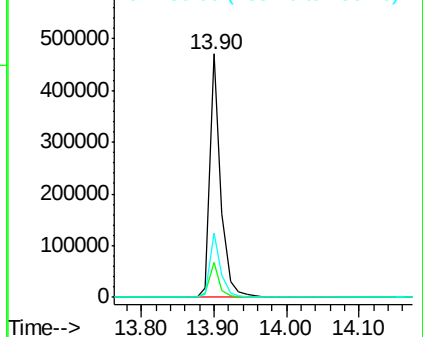

#78

Terphenyl-d14

Concen: 90.87 ng

RT: 12.85 min Scan# 959

Delta R.T. -0.02 min

Lab File: BF093555.D

Acq: 11 Mar 2017 6:45


Tgt Ion:244 Resp: 1697043

Ion Ratio Lower Upper

244 100

212 7.8 6.2 9.2



122 11.2 11.4 17.2#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

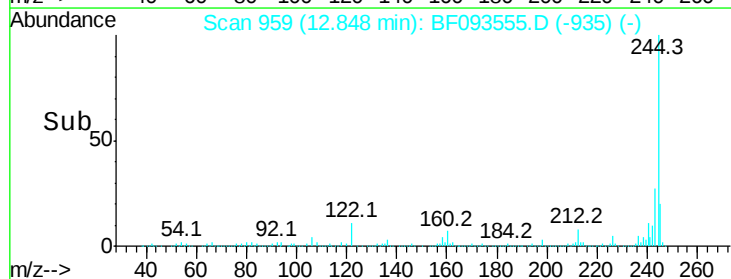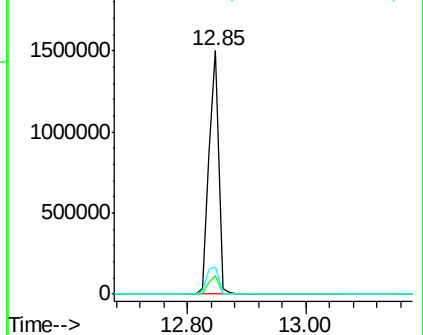


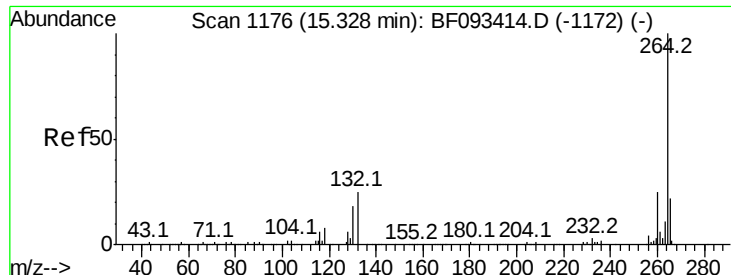

#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.31 min Scan# 1174
Delta R.T. -0.02 min
Lab File: BF093555.D
Acq: 11 Mar 2017 6:45

Instrument :
BNA_F
ClientSampleId :

Tot Ion: 264 Resp: 248631
Ion Ratio Lower Upper
264 100
260 24.6 19.2 28.8
265 21.2 17.4 26.0



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

