
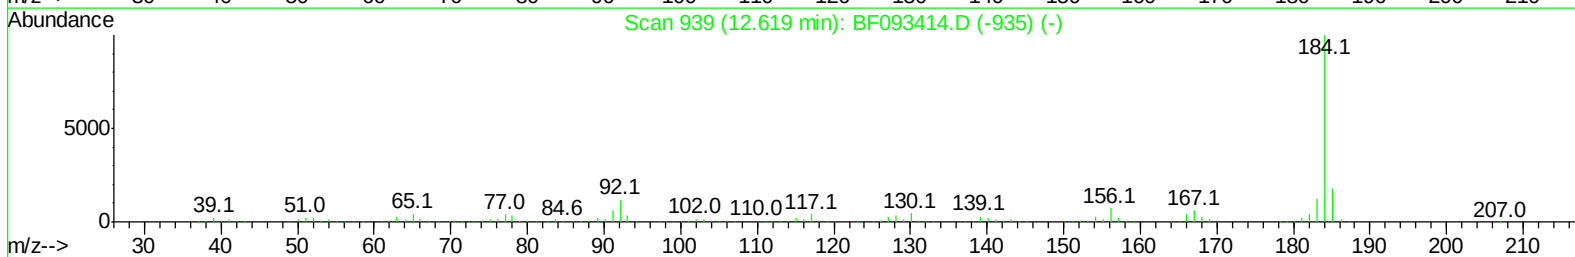
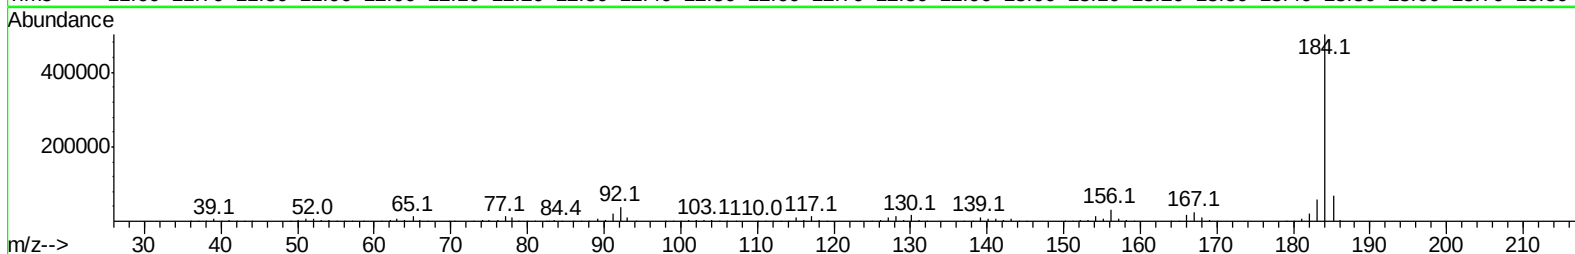


Data Path : Z:\HPCHEM1\BNA F\DATA\BF031017\
Data File : BF093544.D
Acq On : 11 Mar 2017 1:28
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 11 04:38:42 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 15:55:22 2017
Response via : Initial Calibration

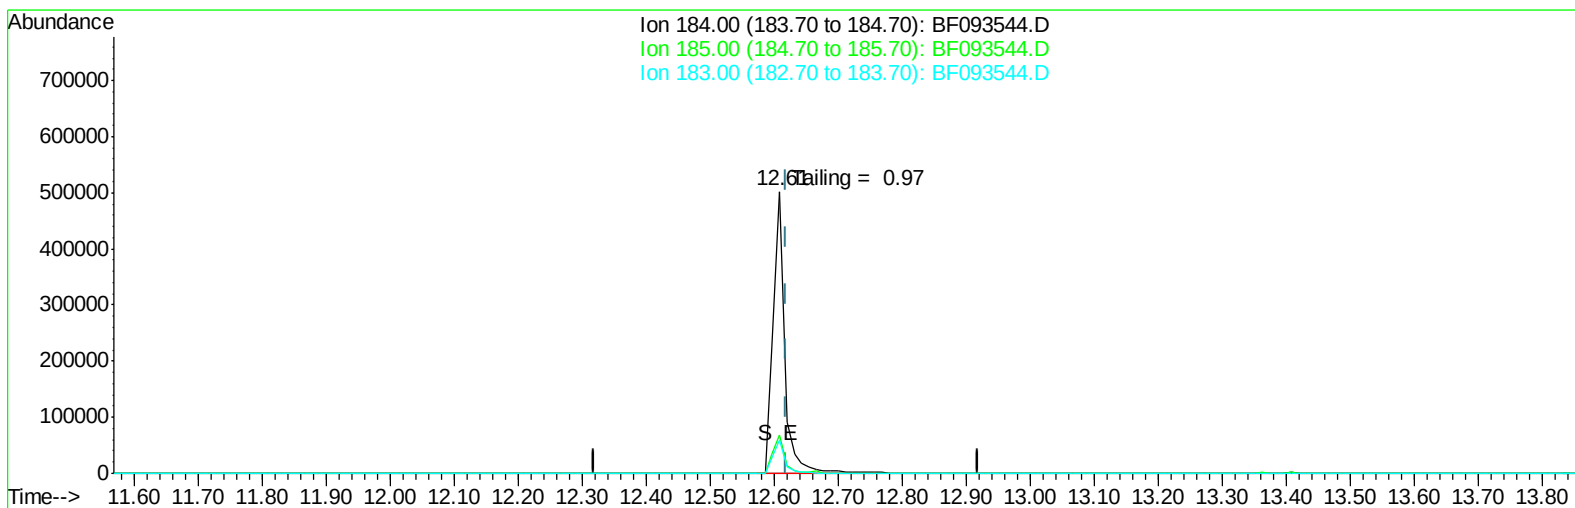

TIC: BF093544.D

(76) Benzidine




12.608min (-0.012) 0.00ng

response 631248

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	13.88
183.00	11.50	11.83
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031017\
Data File : BF093544.D
Acq On : 11 Mar 2017 1:28
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 11 04:38:42 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 15:55:22 2017
Response via : Initial Calibration

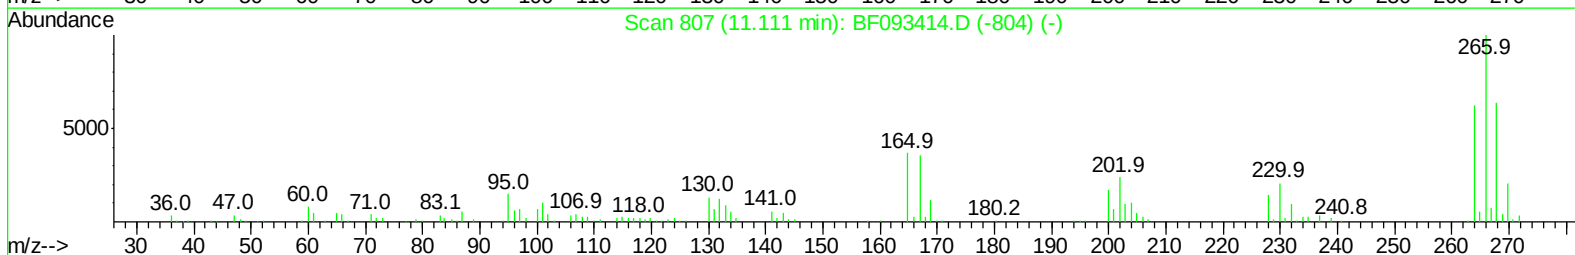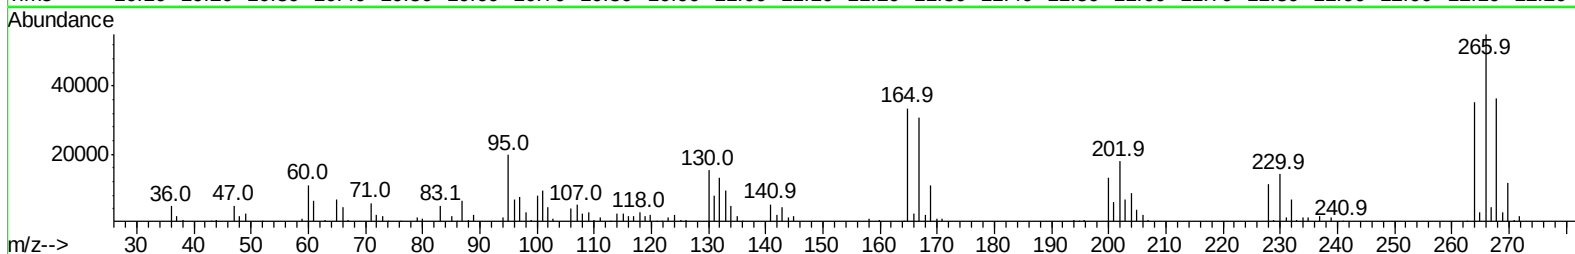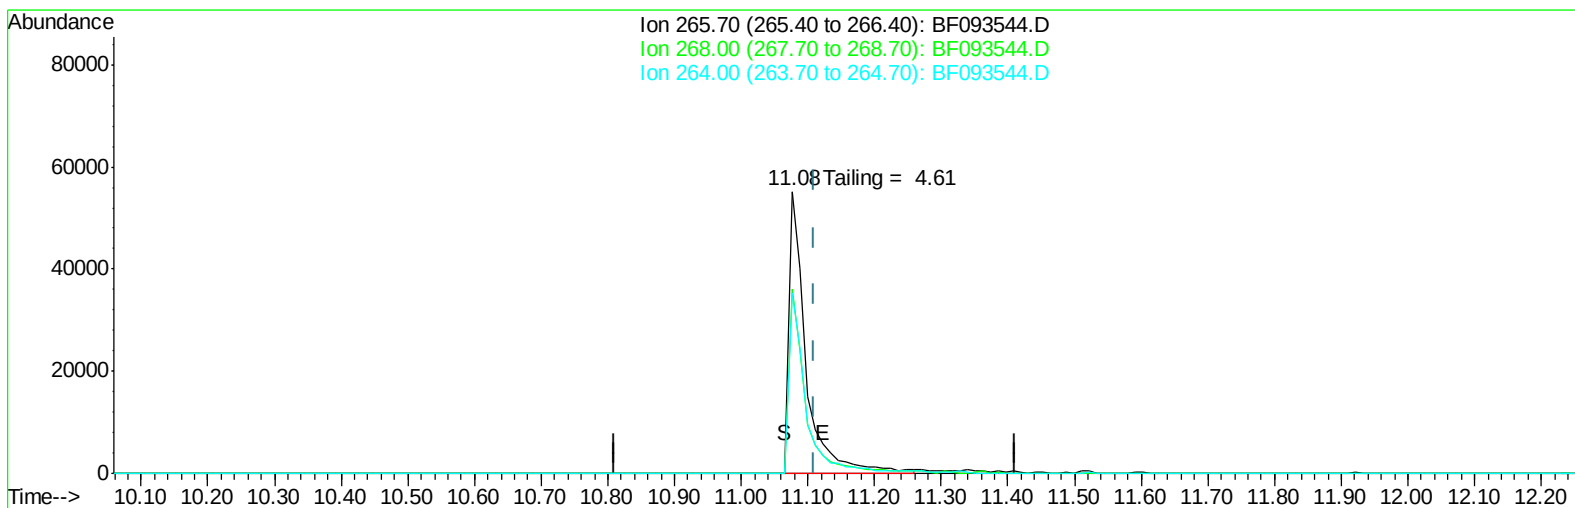

TIC: BF093544.D

(69) Pentachlorophenol (C)

11.076min (-0.034) 35113.42ng

response 98421

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	65.69
264.00	62.90	64.10
0.00	0.00	0.00