

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031017\
 Data File : BF093542.D
 Acq On : 11 Mar 2017 00:32
 Operator : SJ/MA
 Sample : I2198-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FIELDBLANK

Quant Time: Mar 11 03:42:30 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 07 15:55:22 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.74	152	182910	20.00	ng	-0.02
21) Naphthalene-d8	8.02	136	782411	20.00	ng	-0.03
38) Acenaphthene-d10	9.77	164	353817	20.00	ng	-0.03
63) Phenanthrene-d10	11.26	188	657310	20.00	ng	-0.02
75) Chrysene-d12	13.90	240	581945	20.00	ng	-0.02
86) Perylene-d12	15.31	264	430385	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.35	112	675955	61.51	ng	0.00
7) Phenol-d6	6.40	99	568438	41.02	ng	-0.01
23) Nitrobenzene-d5	7.32	82	1162512	82.44	ng	-0.02
41) 2,4,6-Tribromophenol	10.57	330	324571	140.80	ng	-0.02
44) 2-Fluorobiphenyl	9.10	172	1583551	83.25	ng	-0.03
78) Terphenyl-d14	12.85	244	1666911	74.47	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031017\
Data File : BF093542.D
Acq On : 11 Mar 2017 00:32
Operator : SJ/MA
Sample : I2198-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FIELDBLANK

Quant Time: Mar 11 03:42:30 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 15:55:22 2017
Response via : Initial Calibration

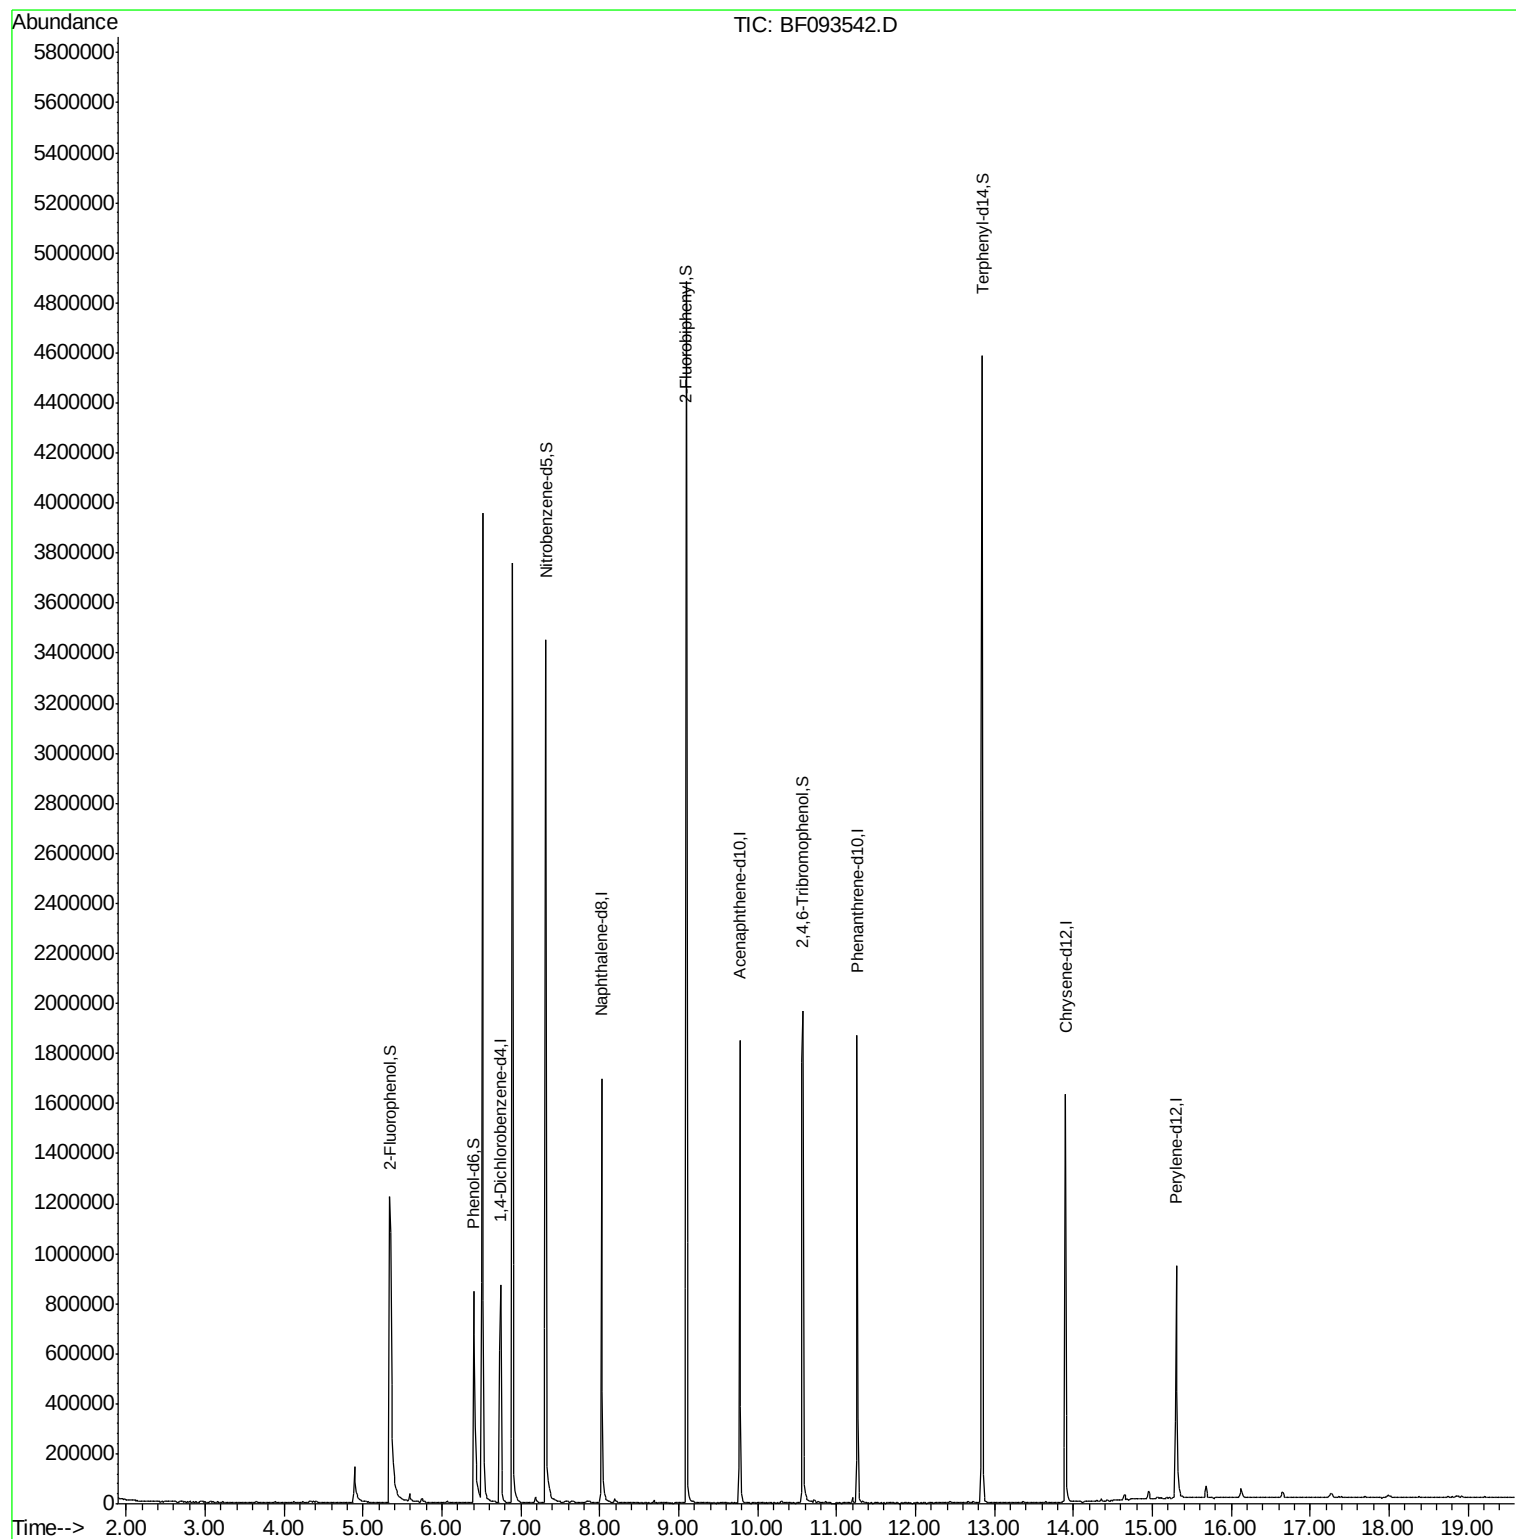

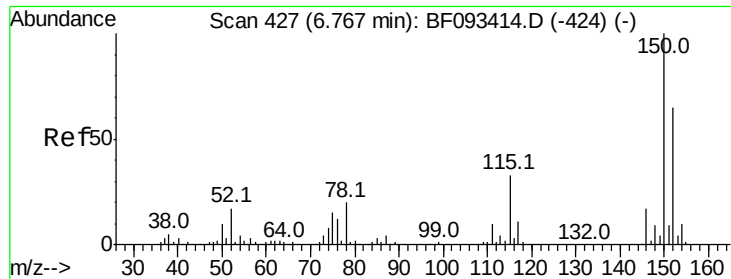

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.74 min Scan# 425

Delta R.T. -0.02 min

Lab File: BF093542.D

Acq: 11 Mar 2017 00:32

Instrument :

BNA_F

ClientSampleId :

FIELDBLANK


Tot Ion:152 Resp: 182910

Ion Ratio Lower Upper

152 100

150 154.8 124.9 187.3




115 54.0 46.0 69.0

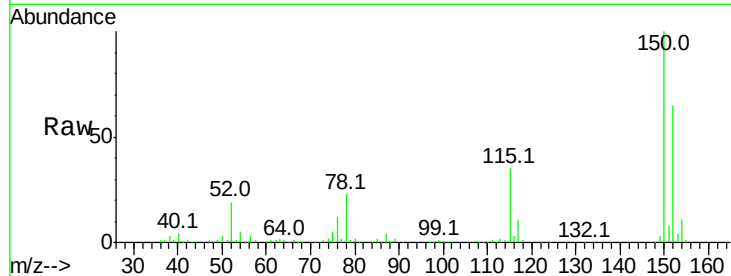

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

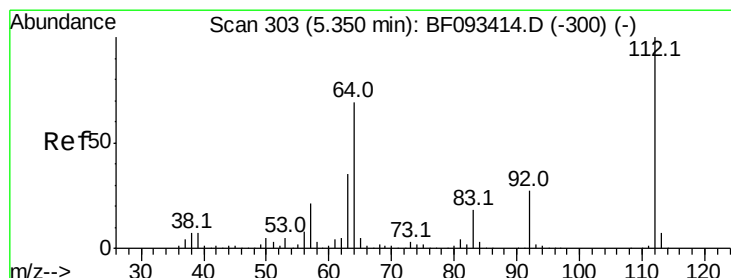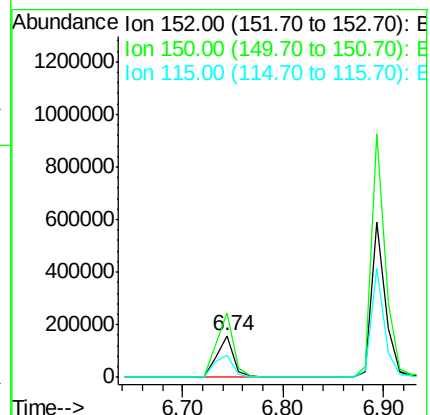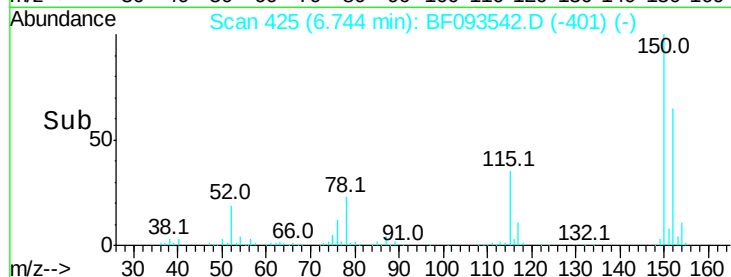

#5

2-Fluorophenol

Concen: 61.51 ng

RT: 5.35 min Scan# 303

Delta R.T. -0.00 min

Lab File: BF093542.D

Acq: 11 Mar 2017 00:32


Tgt Ion:112 Resp: 675955

Ion Ratio Lower Upper

112 100

64 61.7 46.1 69.1



63 31.5 23.8 35.6

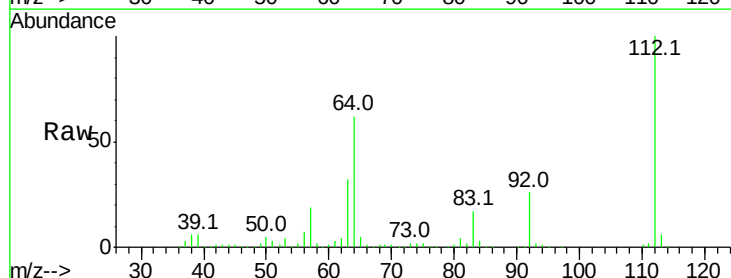


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

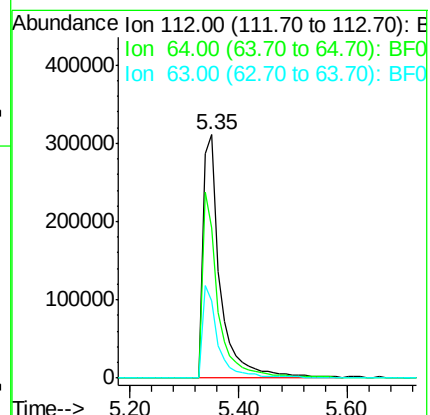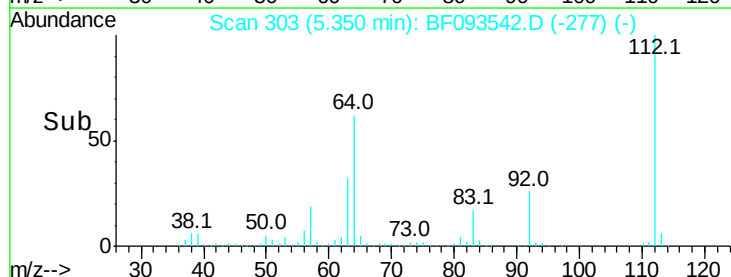

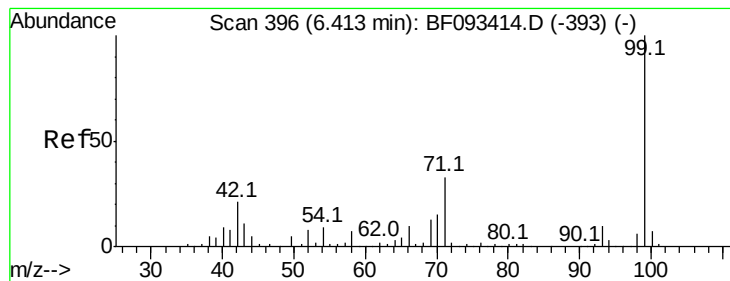

#7

Phenol-d6

Concen: 41.02 ng

RT: 6.40 min Scan# 395

Delta R.T. -0.01 min

Lab File: BF093542.D

Acq: 11 Mar 2017 00:32

Instrument :


BNA_F

ClientSampleId :

FIELDBLANK

Tot Ion: 99 Resp: 568438




Ion	Ratio	Lower	Upper
99	100		
42	24.5	15.6	23.4#
71	34.1	27.5	41.3

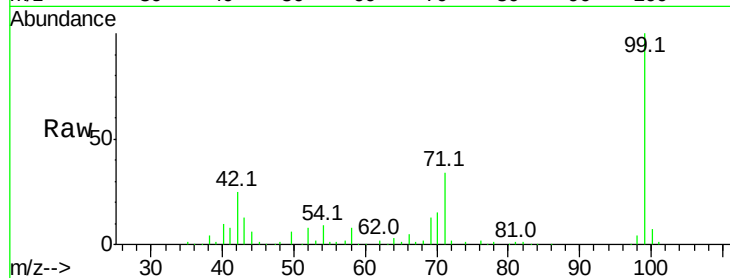

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

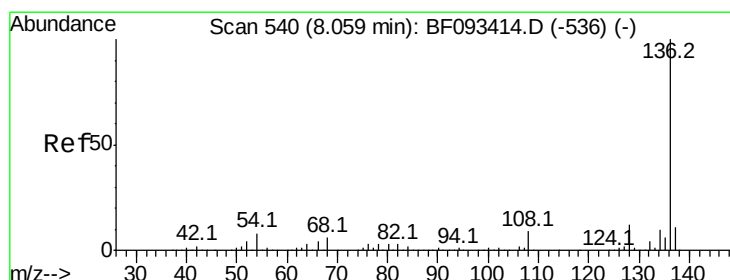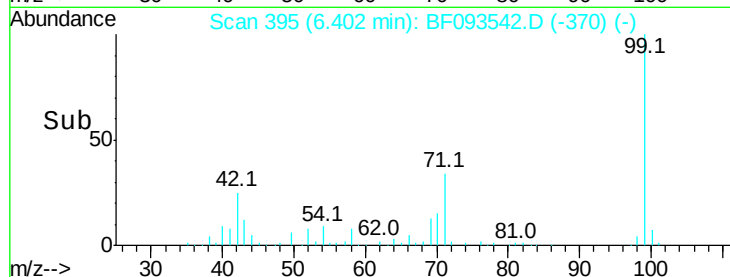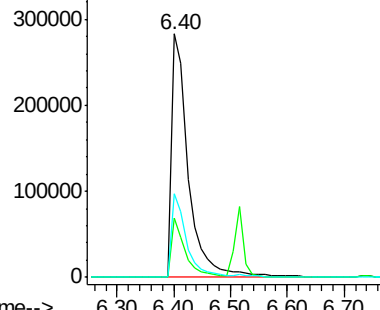

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.02 min Scan# 537


Delta R.T. -0.03 min

Lab File: BF093542.D

Acq: 11 Mar 2017 00:32

Tgt Ion: 136 Resp: 782411

Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.4	12.6
54	11.0	4.5	6.7#
68	7.8	3.6	5.4#


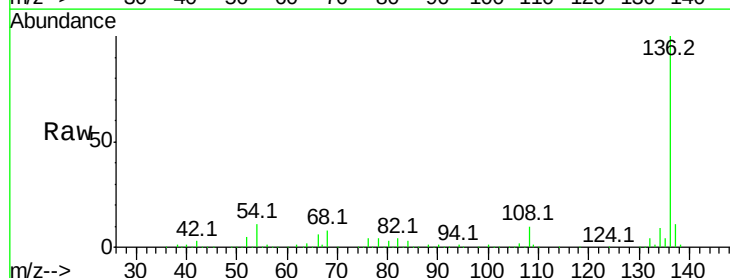



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

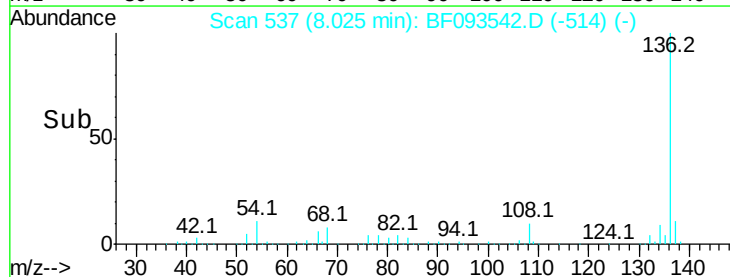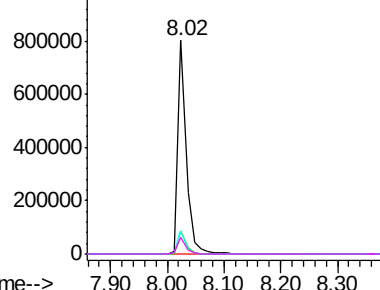


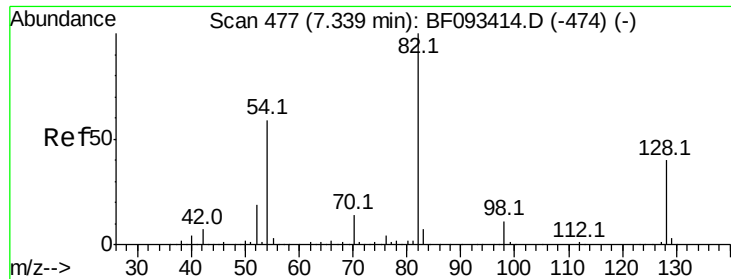




#23
Nitrobenzene-d5
Concen: 82.44 ng
RT: 7.32 min Scan# 475
Delta R.T. -0.02 min
Lab File: BF093542.D
Acq: 11 Mar 2017 00:32

Instrument :
BNA_F
ClientSampleId :
FIELDBLANK

Tot Ion: 82 Resp: 1162512
Ion Ratio Lower Upper
82 100
128 40.5 34.6 52.0
54 57.5 39.5 59.3

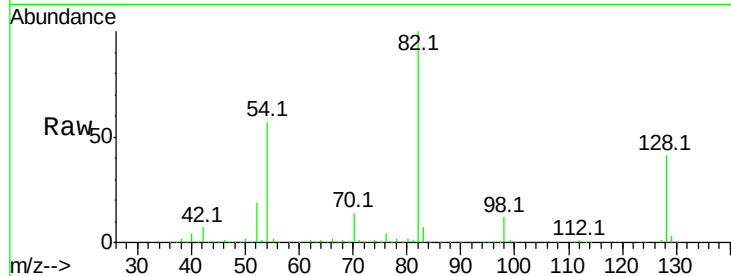


Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): B
Ion 54.00 (53.70 to 54.70): BF0

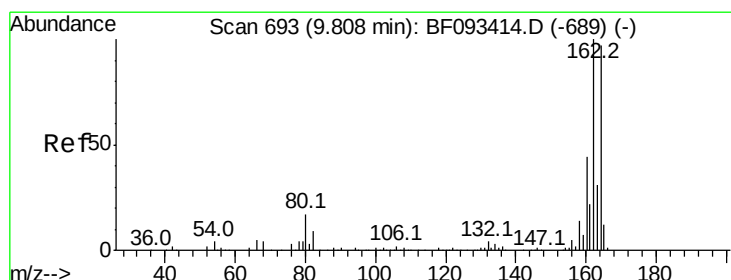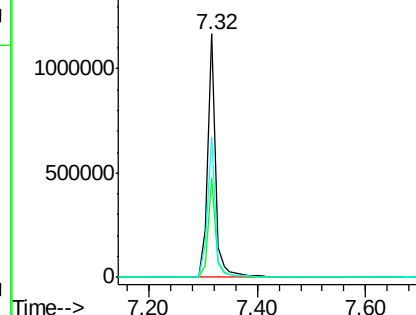
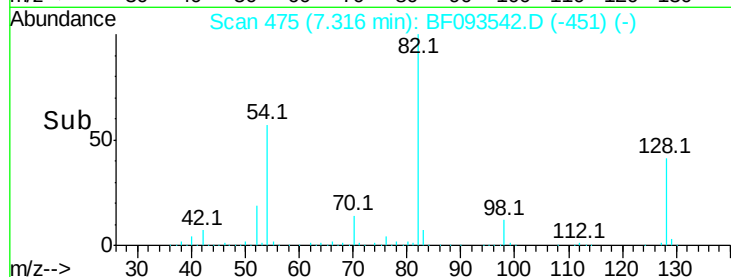



#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.77 min Scan# 690
Delta R.T. -0.03 min
Lab File: BF093542.D
Acq: 11 Mar 2017 00:32

Tgt Ion:164 Resp: 353817
Ion Ratio Lower Upper
164 100
162 102.1 80.2 120.2
160 43.8 36.9 55.3

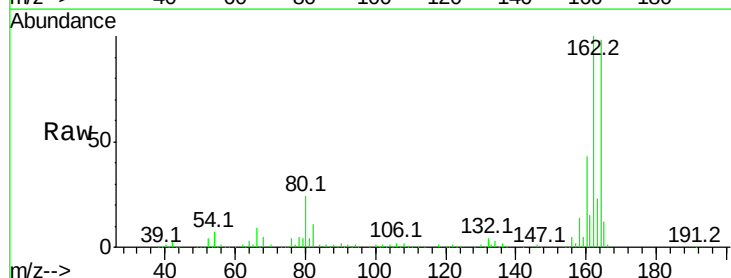

Abundance Ion 164.00 (163.70 to 164.70): B
Ion 162.00 (161.70 to 162.70): B
Ion 160.00 (159.70 to 160.70): B

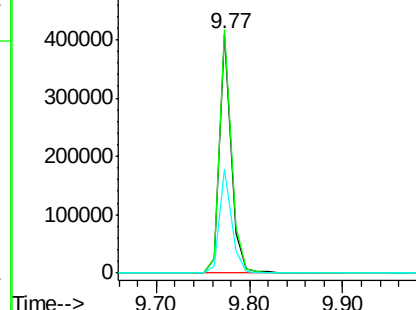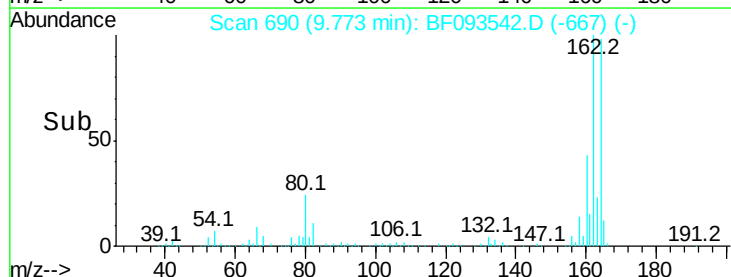


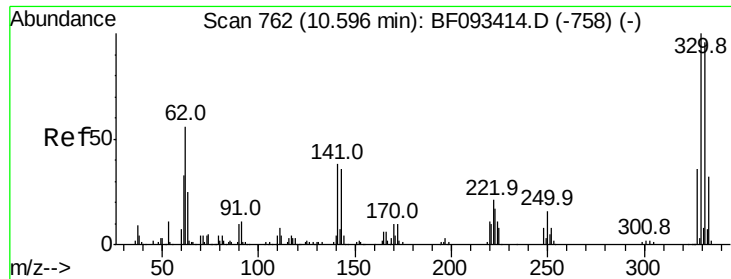




#41
 2,4,6-Tribromophenol
 Concen: 140.80 ng
 RT: 10.57 min Scan# 760
 Delta R.T. -0.02 min
 Lab File: BF093542.D
 Acq: 11 Mar 2017 00:32

Instrument :
 BNA_F
 ClientSampleId :
 FIELDBLANK

Tot Ion:330 Resp: 324571
 Ion Ratio Lower Upper
 330 100
 332 97.1 77.4 116.2
 141 39.3 34.1 51.1

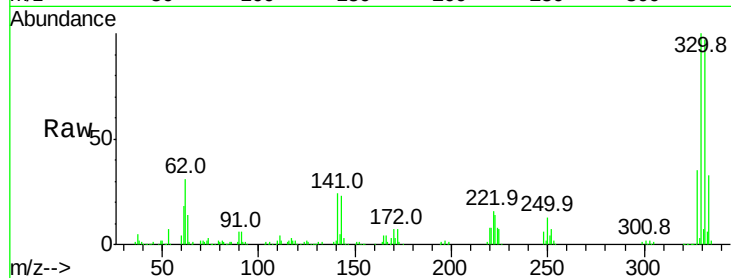


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

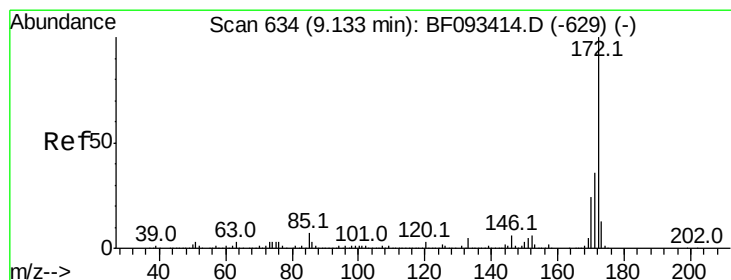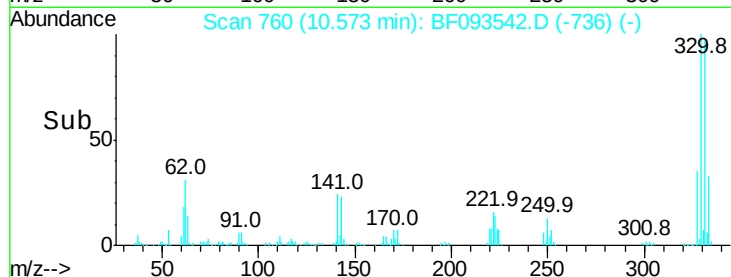
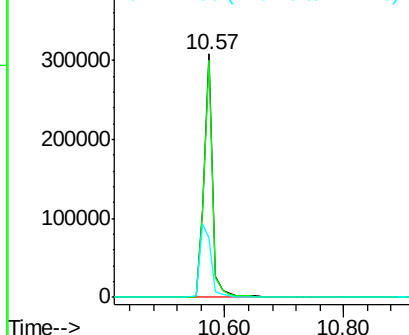



#44
 2-Fluorobiphenyl
 Concen: 83.25 ng
 RT: 9.10 min Scan# 631
 Delta R.T. -0.03 min
 Lab File: BF093542.D
 Acq: 11 Mar 2017 00:32

Tgt Ion:172 Resp: 1583551
 Ion Ratio Lower Upper
 172 100
 171 36.8 29.4 44.0
 170 24.5 20.2 30.4

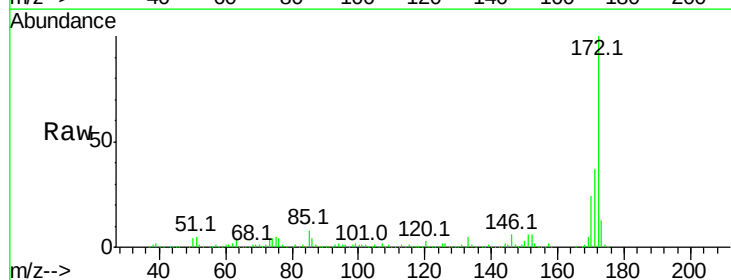

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

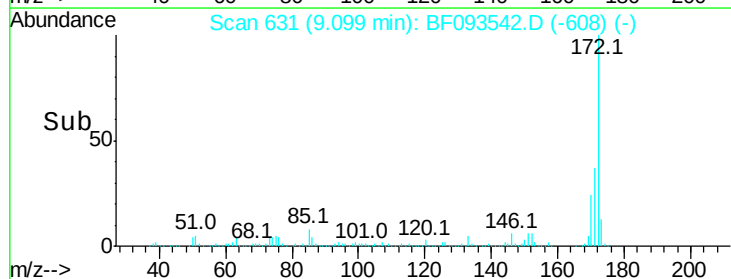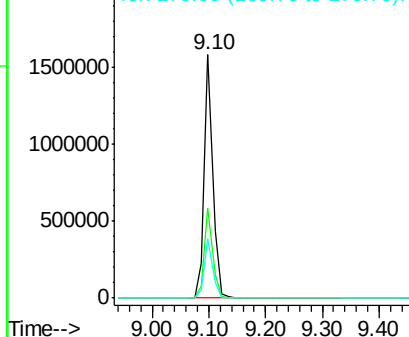


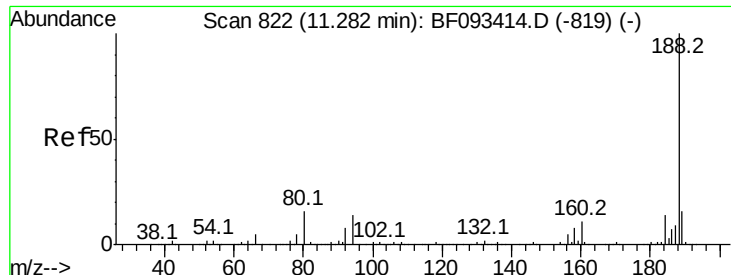




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.26 min Scan# 820
Delta R.T. -0.02 min
Lab File: BF093542.D
Acq: 11 Mar 2017 00:32

Instrument :
BNA_F
ClientSampleId :
FIELDBLANK

Tot Ion:188 Resp: 657310
Ion Ratio Lower Upper
188 100
94 11.7 10.0 15.0
80 12.7 11.2 16.8

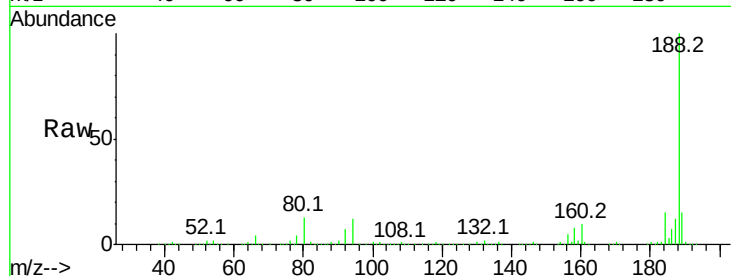


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

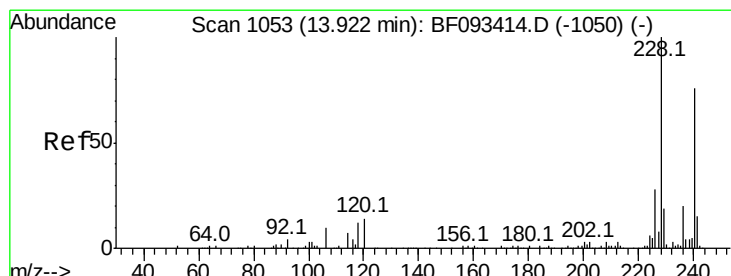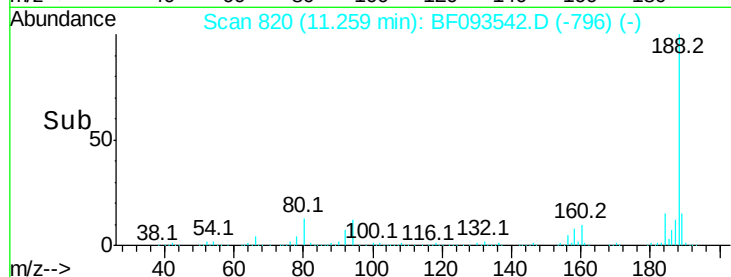
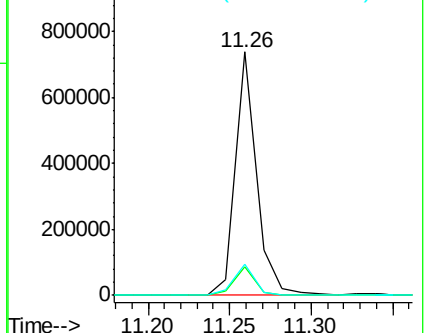



#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.90 min Scan# 1051
Delta R.T. -0.02 min
Lab File: BF093542.D
Acq: 11 Mar 2017 00:32

Tgt Ion:240 Resp: 581945
Ion Ratio Lower Upper
240 100
120 13.3 12.9 19.3
236 26.1 20.9 31.3

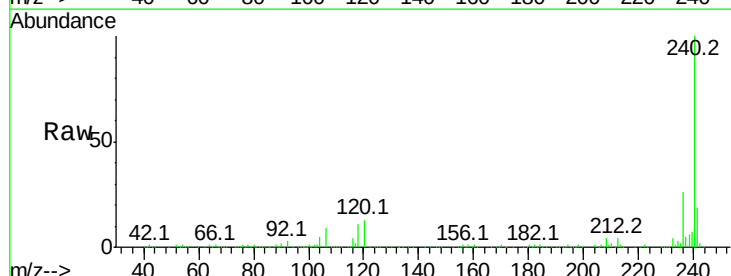

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

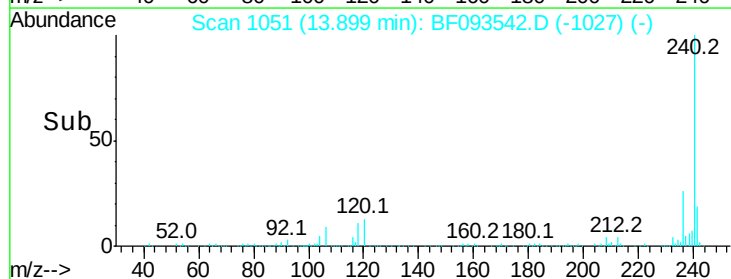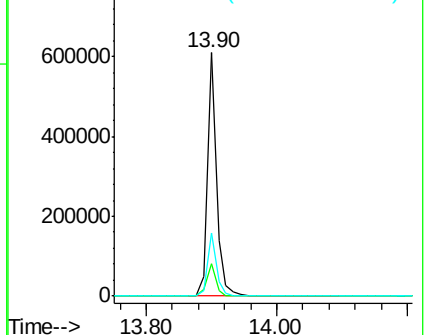

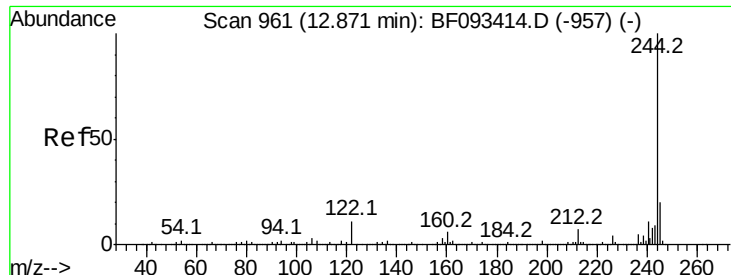

#78

Terphenyl-d14

Concen: 74.47 ng

RT: 12.85 min Scan# 959

Delta R.T. -0.02 min

Lab File: BF093542.D

Acq: 11 Mar 2017 00:32

Instrument :

BNA_F

ClientSampleId :

FIELDBLANK


Tot Ion:244 Resp: 1666911

Ion Ratio Lower Upper

244 100

212 7.7 6.2 9.2




122 11.2 11.4 17.2#

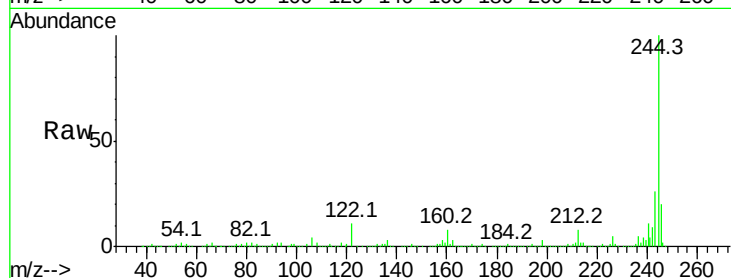

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

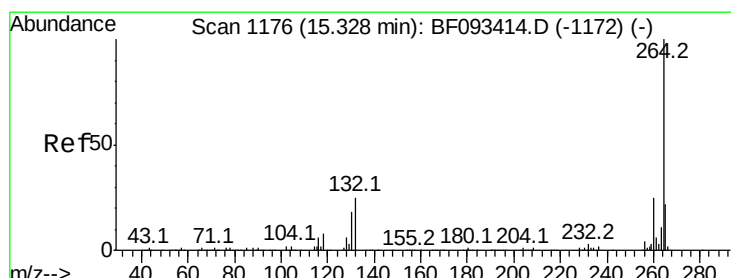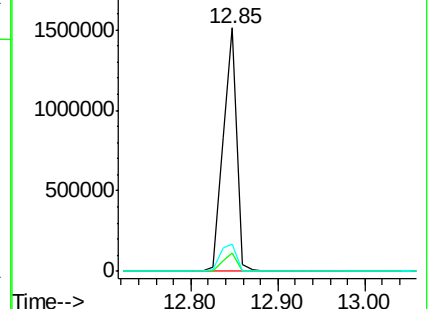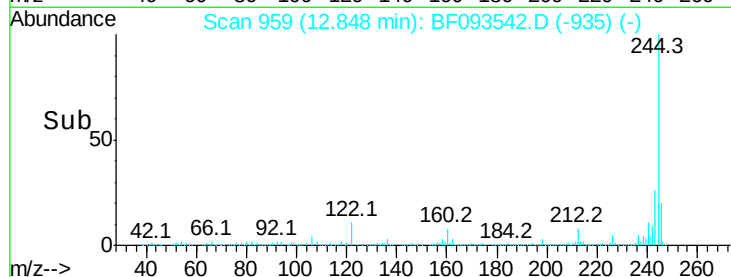

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.31 min Scan# 1174

Delta R.T. -0.02 min

Lab File: BF093542.D

Acq: 11 Mar 2017 00:32


Tgt Ion:264 Resp: 430385

Ion Ratio Lower Upper

264 100

260 23.8 19.2 28.8

265 21.5 17.4 26.0

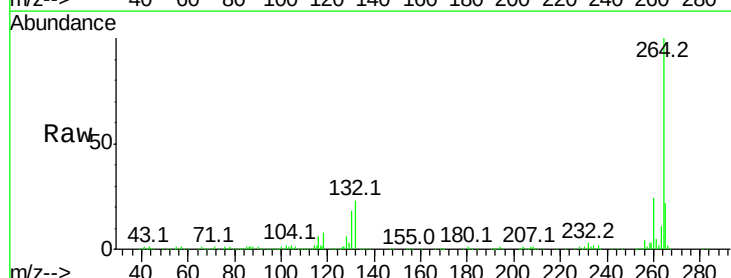

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

