

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031017\
 Data File : BF093540.D
 Acq On : 10 Mar 2017 23:37
 Operator : SJ/MA
 Sample : I2198-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 W-23

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.893	261	263	277	rBV	129718	246227	4.79%	0.650%
2	5.350	301	303	323	rBV	1118150	2507439	48.74%	6.623%
3	6.413	394	396	403	rBV	782020	1509004	29.34%	3.986%
4	6.516	403	405	419	rVB	4106033	4192609	81.50%	11.075%
5	6.744	422	425	427	rBV	899560	1097617	21.34%	2.899%
6	6.893	436	438	441	rBV	3974115	3749013	72.88%	9.903%
7	7.316	472	475	477	rBV	3548808	3338684	64.90%	8.819%
8	8.025	535	537	548	rVB	1556796	1523164	29.61%	4.023%
9	9.099	629	631	634	rBV	4977923	5048404	98.14%	13.335%
10	9.499	664	666	669	rBV	82858	111282	2.16%	0.294%
11	9.773	688	690	693	rBV	1807485	1624123	31.57%	4.290%
12	10.208	726	728	729	rVB	55333	60666	1.18%	0.160%
13	10.573	757	760	762	rBV	2455011	2990188	58.13%	7.898%
14	10.676	767	769	771	rBV	98284	106633	2.07%	0.282%
15	11.122	806	808	809	rBV	88735	80558	1.57%	0.213%
16	11.259	818	820	823	rBV	1841667	1647825	32.03%	4.353%
17	11.545	843	845	847	rVB	62260	51483	1.00%	0.136%
18	12.848	956	959	961	rBV	4656284	5144031	100.00%	13.588%
19	13.739	1034	1037	1045	rBV	45319	122006	2.37%	0.322%
20	13.899	1049	1051	1054	rBV	1631439	1515074	29.45%	4.002%
21	15.305	1171	1174	1182	rVB	927406	1191690	23.17%	3.148%


Sum of corrected areas: 37857720

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031017\
Data File : BF093540.D
Acq On : 10 Mar 2017 23:37
Operator : SJ/MA
Sample : I2198-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
W-23

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

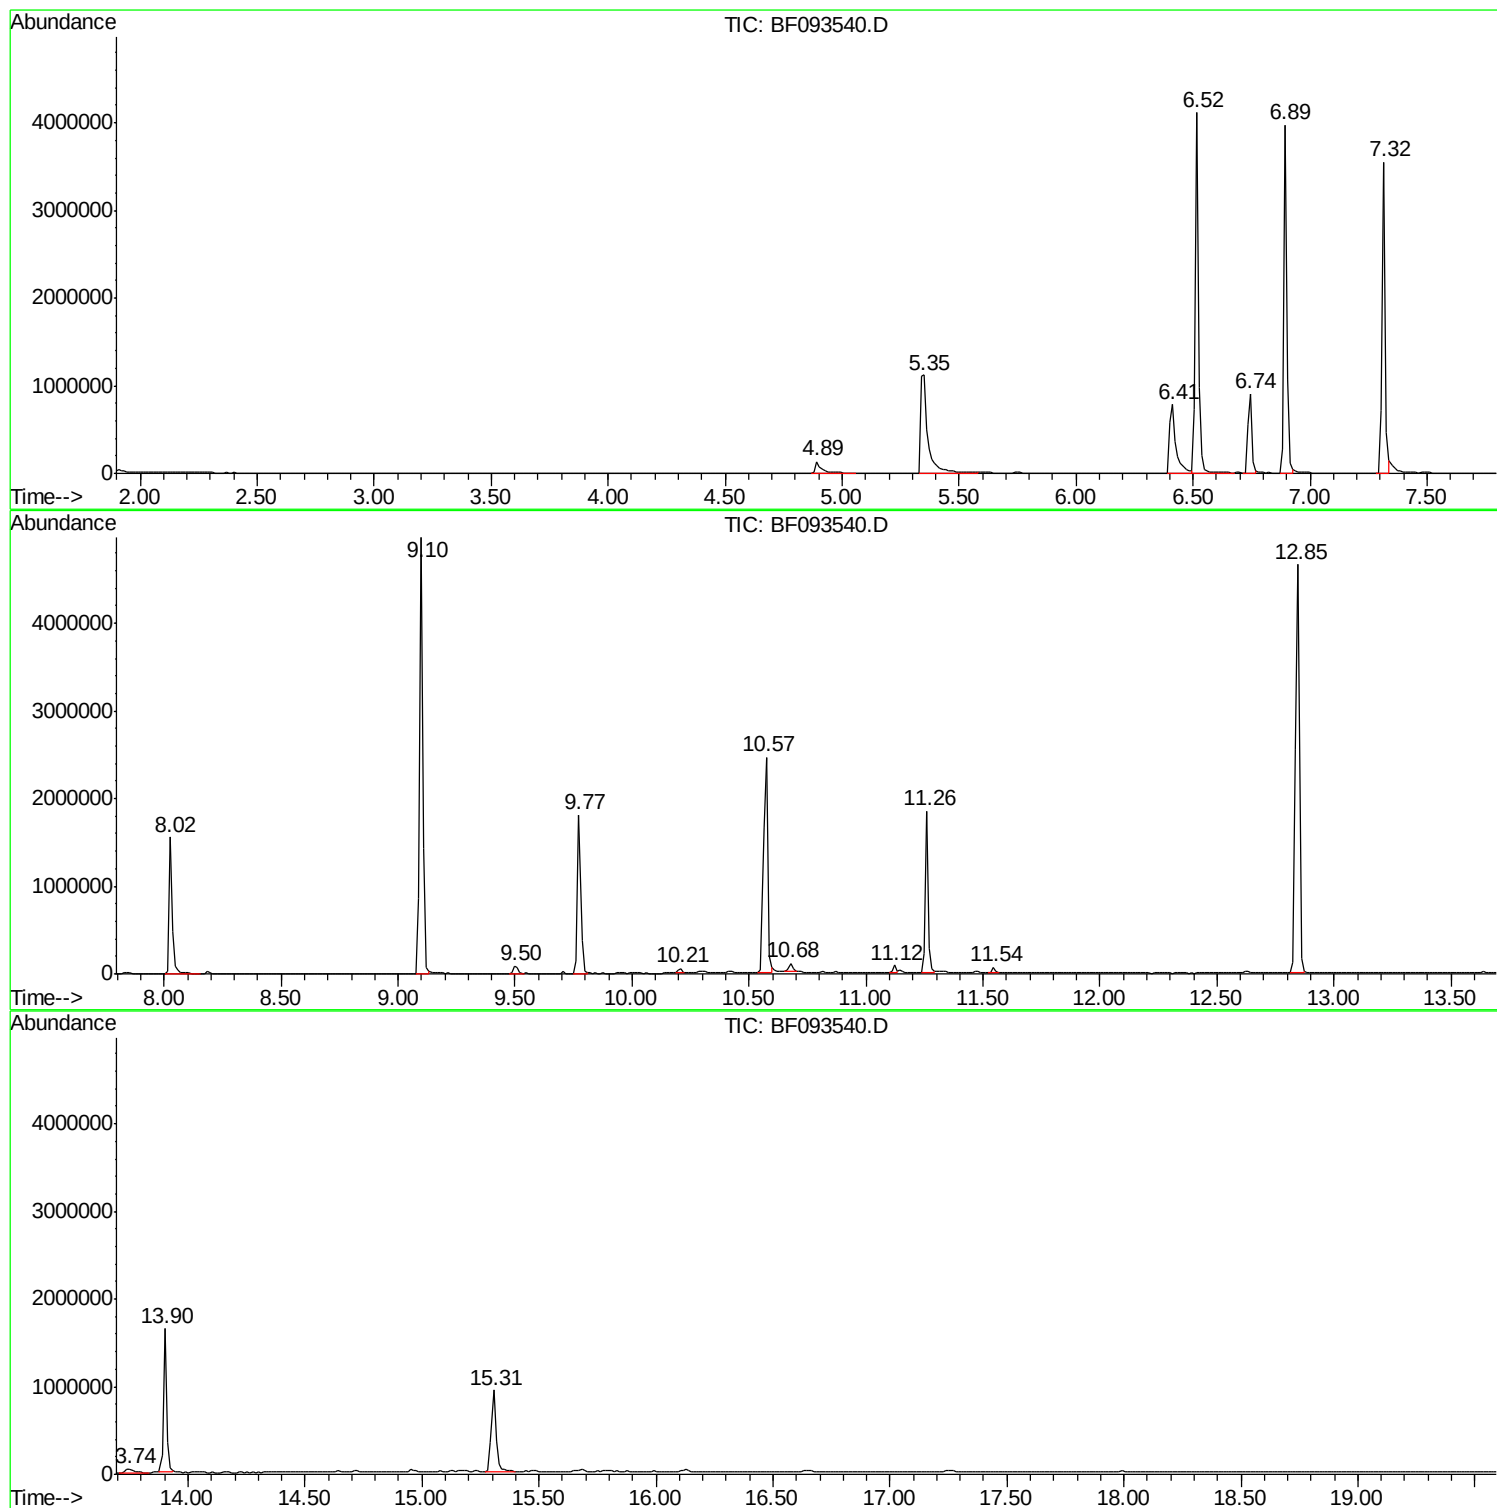

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031017\
Data File : BF093540.D
Acq On : 10 Mar 2017 23:37
Operator : SJ/MA
Sample : I2198-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
W-23










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.89	4.49 ng	246227	1,4-Dichlorobenzene-d4	6.74

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2		2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	38
3		3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33
4		Acetic acid, cyano-, 1,1-dimethyl...	141	C7H11NO2	001116-98-9	25
5		2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9

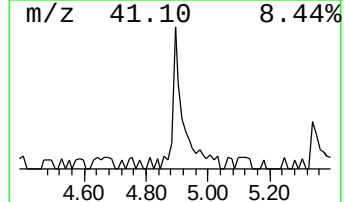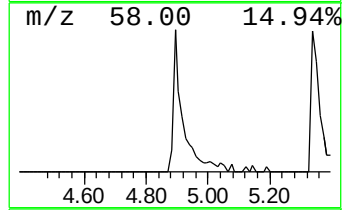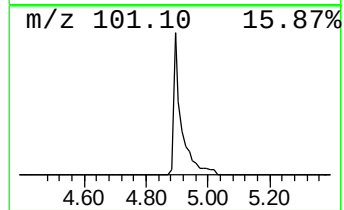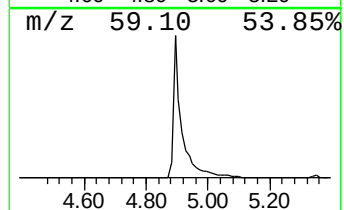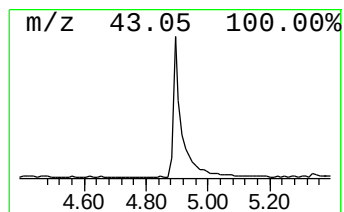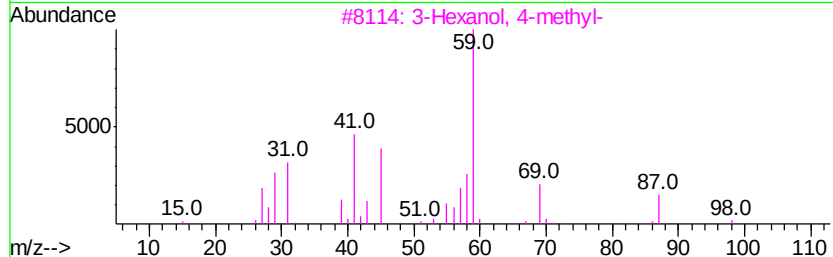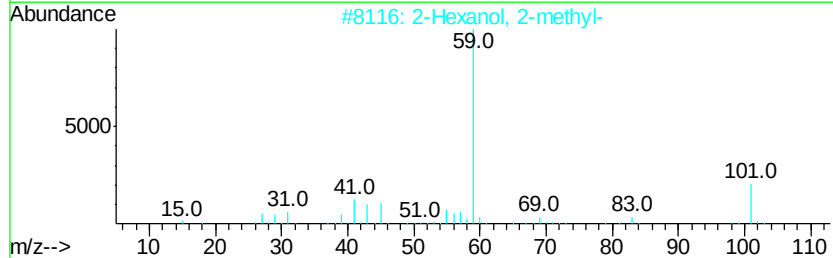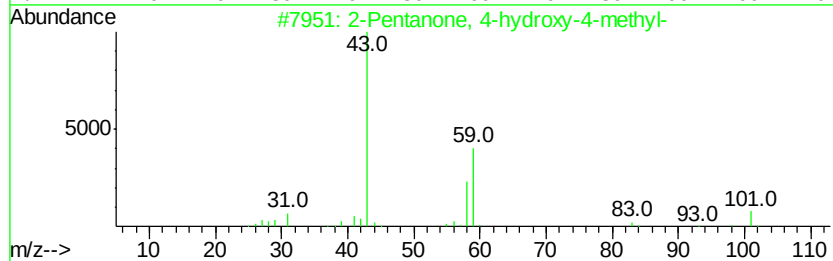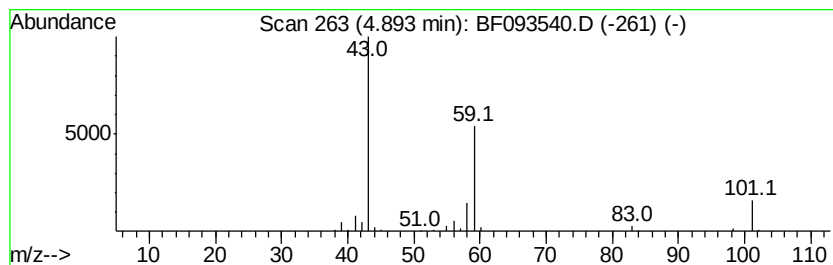

Data Path : Z:\HPCHEM1\BNA F\DATA\BF031017\
Data File : BF093540.D
Acq On : 10 Mar 2017 23:37
Operator : SJ/MA
Sample : I2198-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
W-23










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.52 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.52	76.39 ng	4192610	1,4-Dichlorobenzene-d4	6.74

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Aminoindole	132	C8H8N2	005192-03-0	12
3		Tranvlcypromine-propionyl	189	C12H15NO	1000123-86-3	10
4		Imidazole, 4,5-dicyano-1-methyl-	132	C6H4N4	019485-35-9	9
5		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9

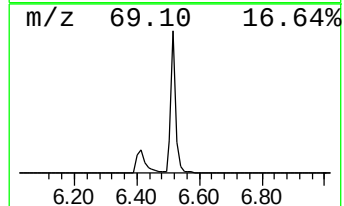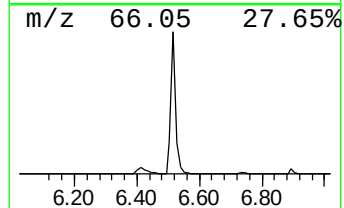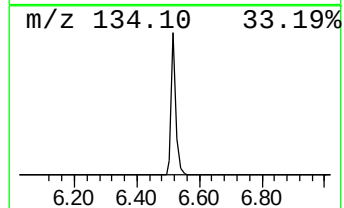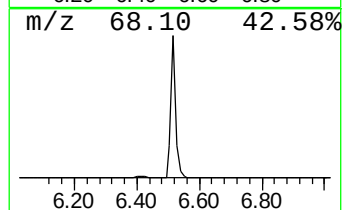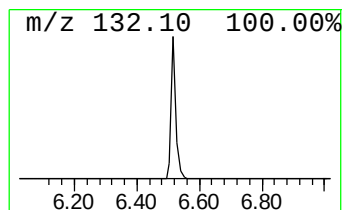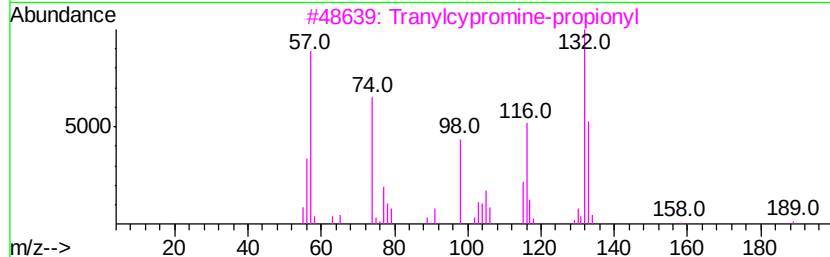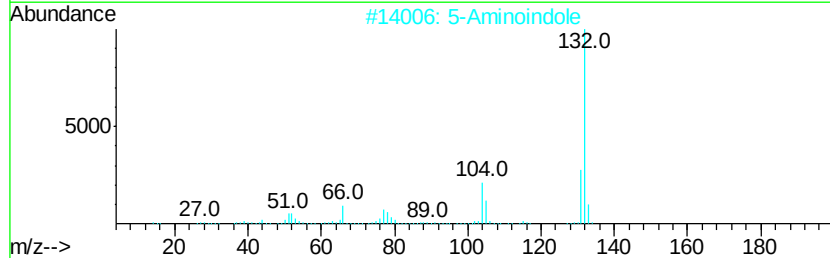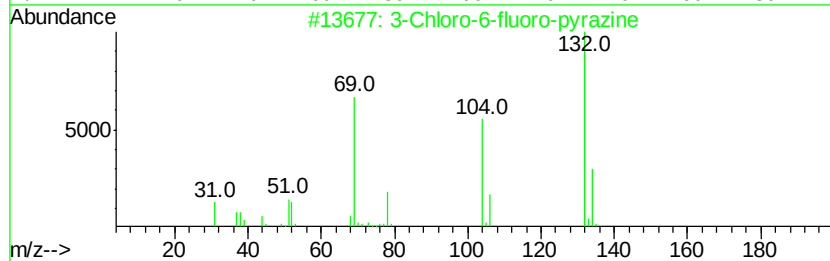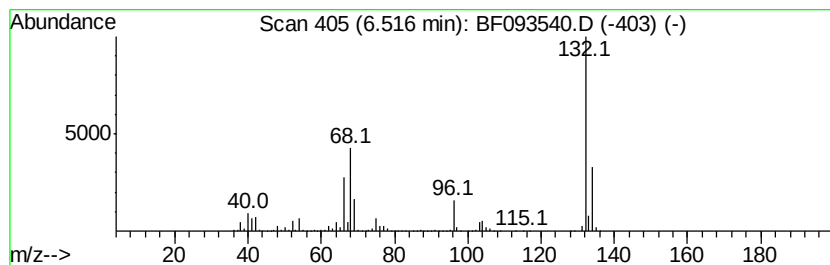

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031017\
Data File : BF093540.D
Acq On : 10 Mar 2017 23:37
Operator : SJ/MA
Sample : I2198-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
W-23

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.89	4.5	ng	246227	1	6.74	1097620	20.0
unknown6.52	6.52	76.4	ng	4192610	1	6.74	1097620	20.0