


Data Path : Z:\HPCHEM1\BNA F\Data\BF031017\
 Data File : BF093519.D
 Acq On : 10 Mar 2017 12:59
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 13 15:05:08 2017

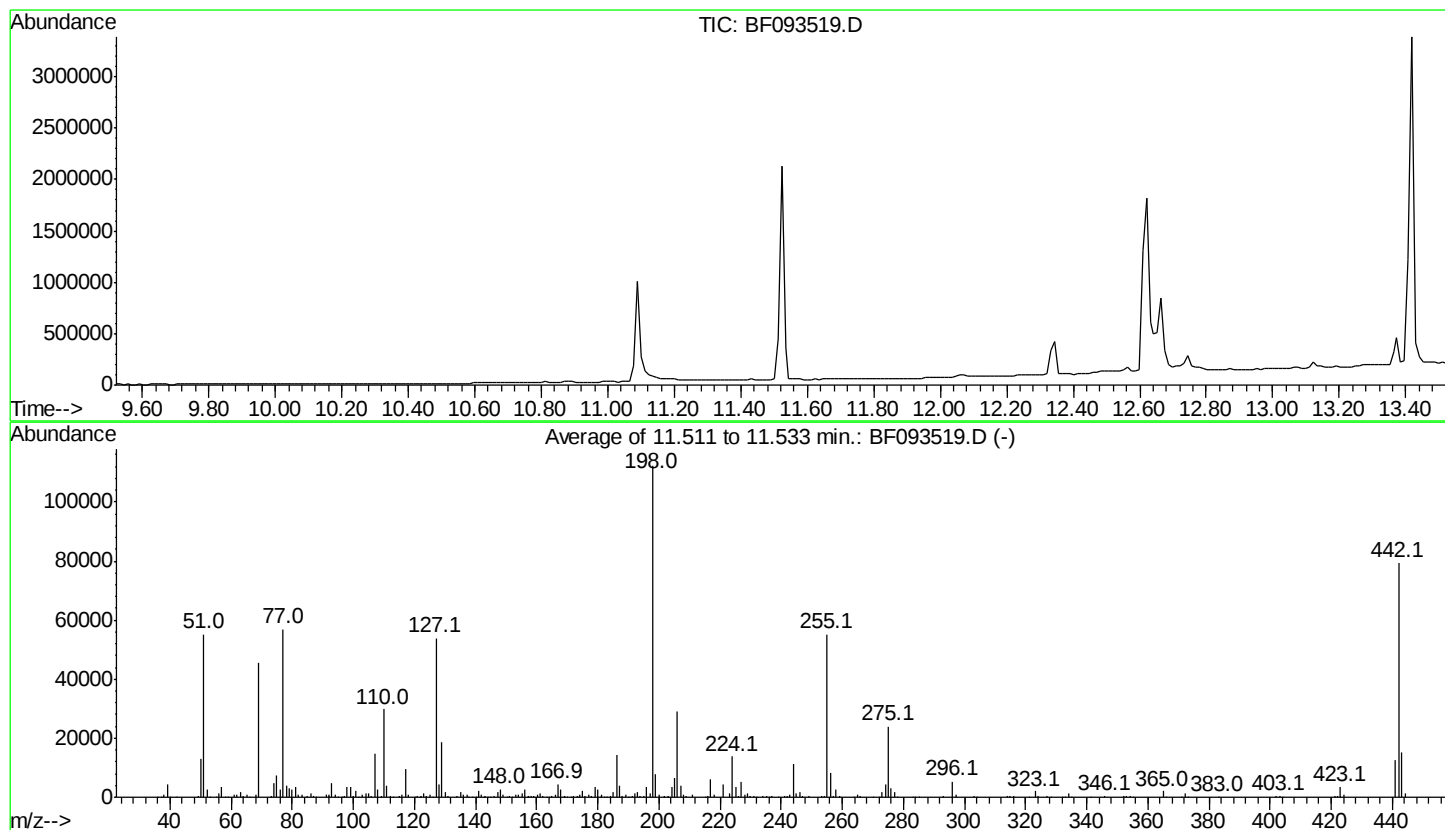

AutoFind: Scans 842, 843, 844; Background Corrected with Scan 838

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.2	55285	PASS
68	69	0.00	2	1.8	843	PASS
69	198	0.00	100	40.7	45700	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.0	53927	PASS
197	198	0.00	2	1.0	1106	PASS
198	198	100	100	100.0	112314	PASS
199	198	5	9	6.8	7651	PASS
275	198	10	60	21.3	23969	PASS
365	198	1	100	1.9	2167	PASS
441	442	0.01	24	15.6	12399	PASS
442	198	50	100	70.8	79540	PASS
443	442	15	24	19.1	15162	PASS