


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031017\
 Data File : BF093544.D
 Acq On : 11 Mar 2017 1:28
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 13 15:05:08 2017

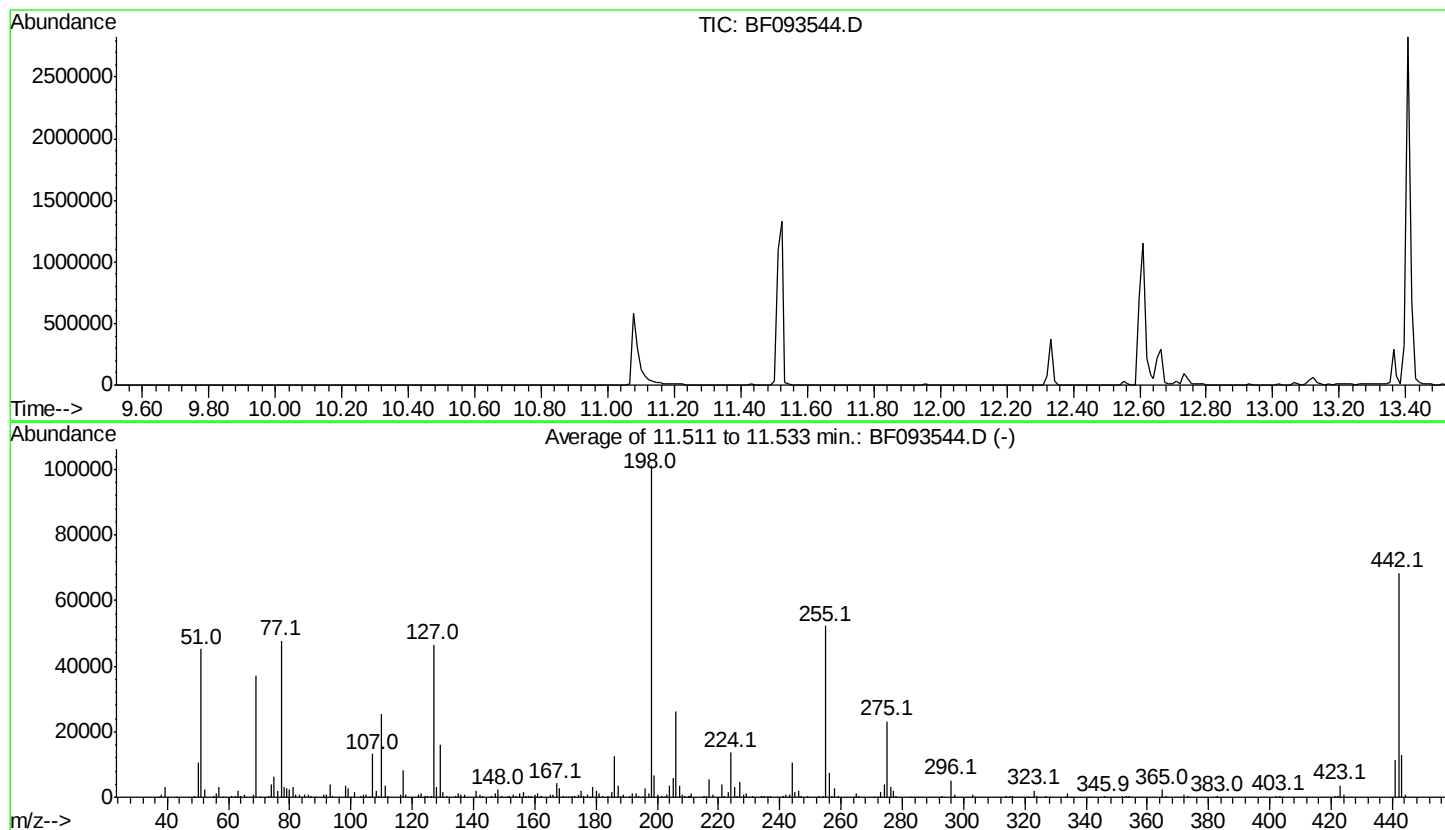

AutoFind: Scans 842, 843, 844; Background Corrected with Scan 838

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.7	45256	PASS
68	69	0.00	2	1.7	637	PASS
69	198	0.00	100	36.8	37236	PASS
70	69	0.00	2	0.4	135	PASS
127	198	10	80	46.1	46627	PASS
197	198	0.00	2	1.1	1079	PASS
198	198	100	100	100.0	101150	PASS
199	198	5	9	6.6	6655	PASS
275	198	10	60	22.8	23041	PASS
365	198	1	100	2.2	2246	PASS
441	442	0.01	24	16.3	11157	PASS
442	198	50	100	67.6	68373	PASS
443	442	15	24	19.1	13086	PASS