
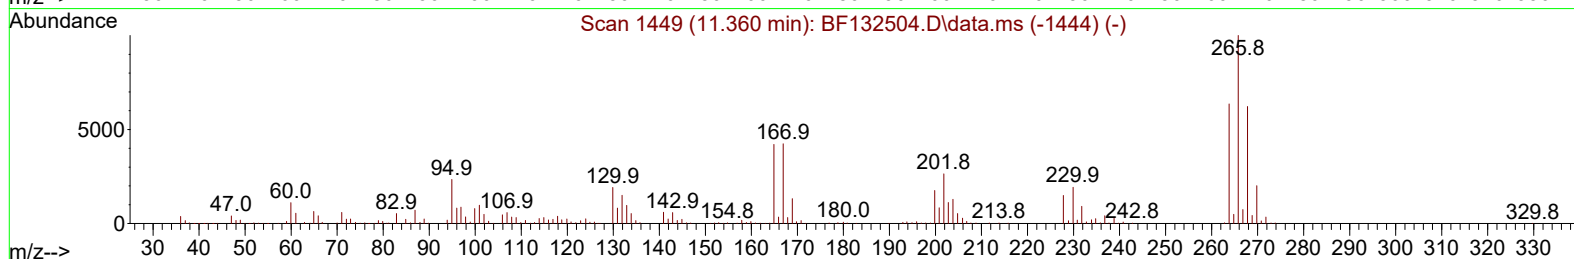
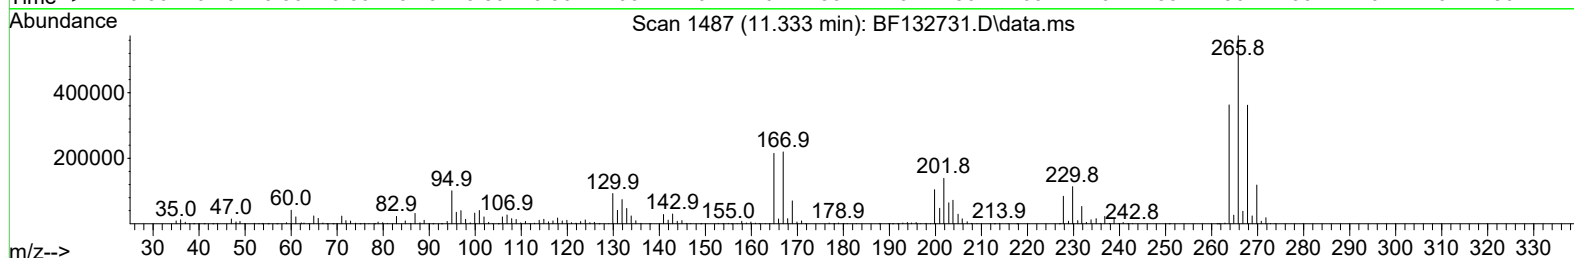


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF031023\  
Data File : BF132731.D  
Acq On : 10 Mar 2023 09:38  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 11 03:17:05 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF022223.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Mar 09 16:26:19 2023  
Response via : Initial Calibration

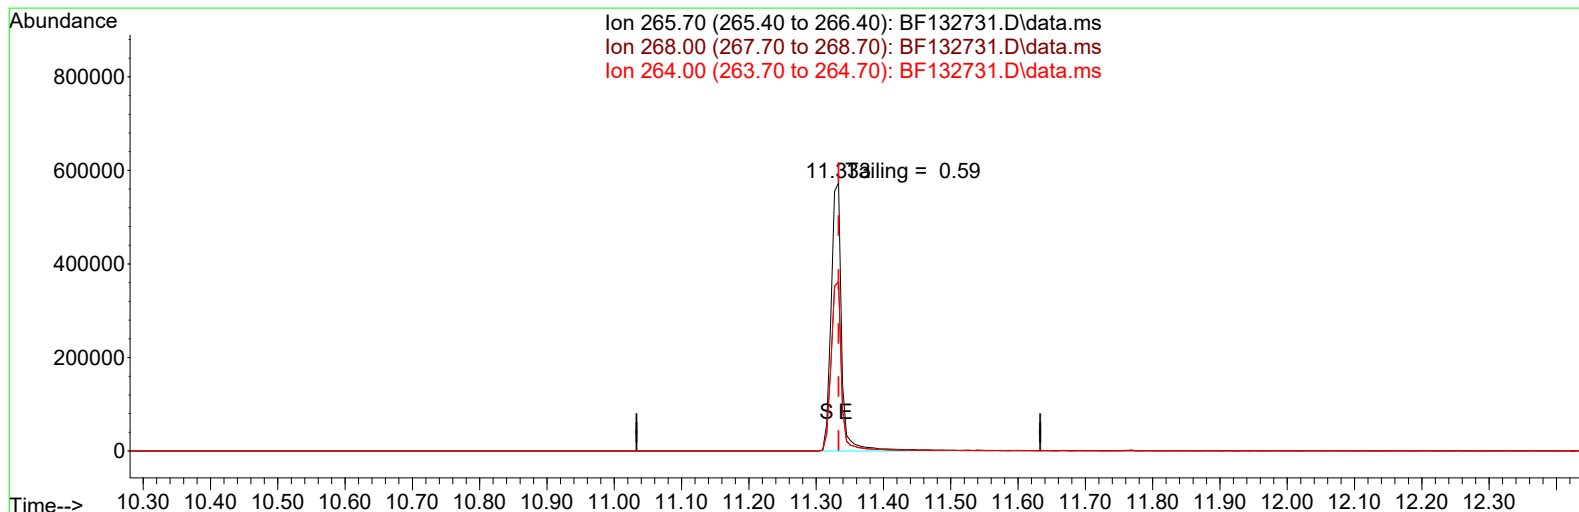




TIC: BF132731.D\data.ms

**(70) Pentachlorophenol (C)****11.333min (+ 0.000) 728789.30 ng****response 619311**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 63.11  |
| 264.00 | 63.60  | 63.27  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF031023\  
Data File : BF132731.D  
Acq On : 10 Mar 2023 09:38  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 11 03:17:05 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF022223.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Mar 09 16:26:19 2023  
Response via : Initial Calibration

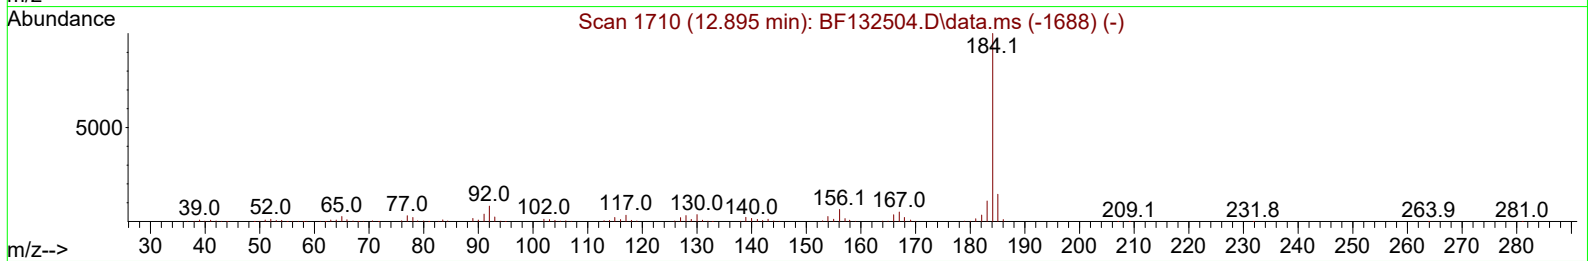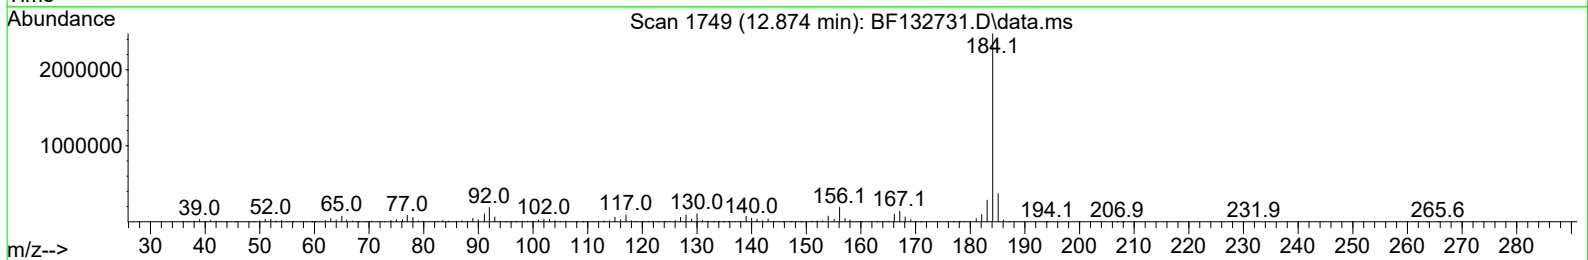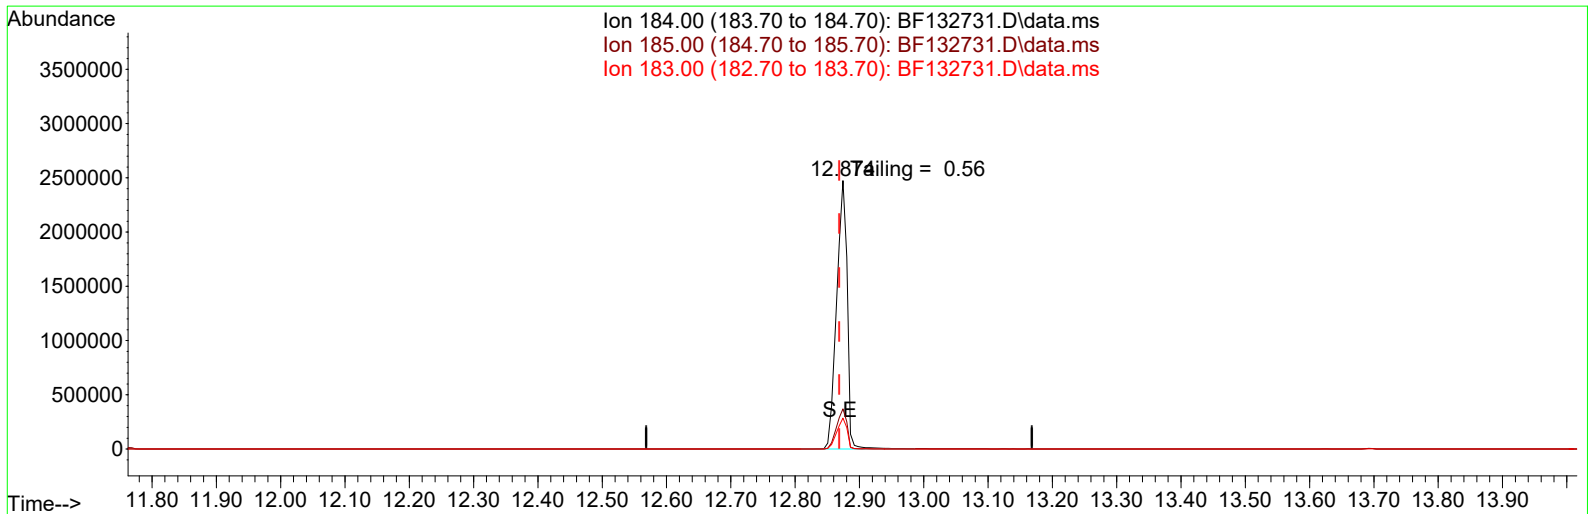

TIC: BF132731.D\data.ms

**(77) Benzidine****12.874min (+ 0.006) 314182.94 ng****response 2845097**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.60  | 14.96  |
| 183.00 | 10.90  | 11.50  |
| 0.00   | 0.00   | 0.00   |