
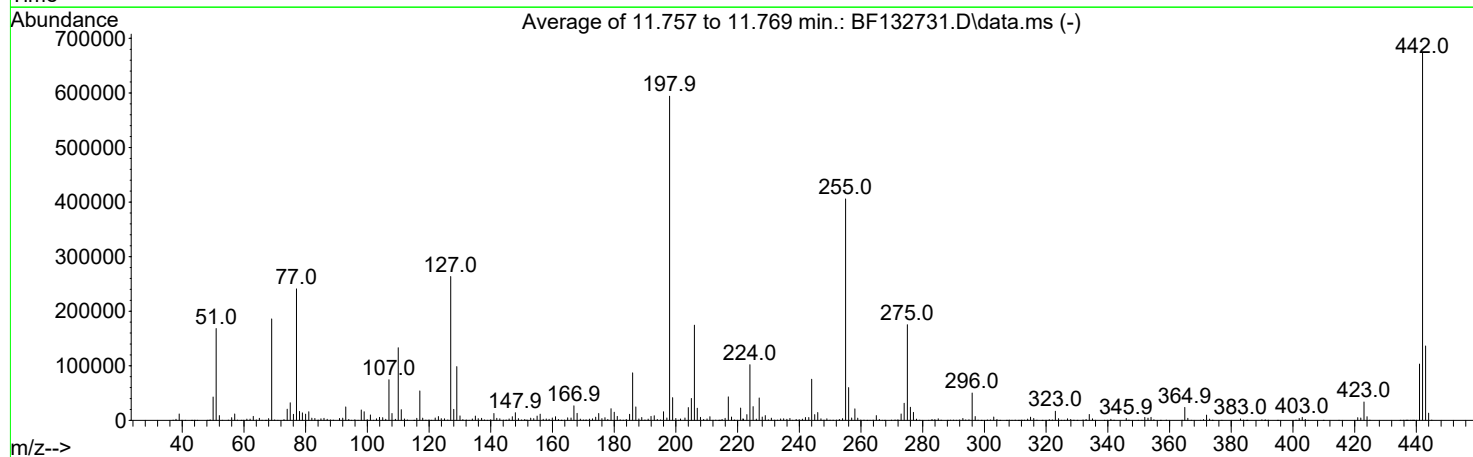


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031023\
Data File : BF132731.D
Acq On : 10 Mar 2023 09:38
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 09 16:26:19 2023

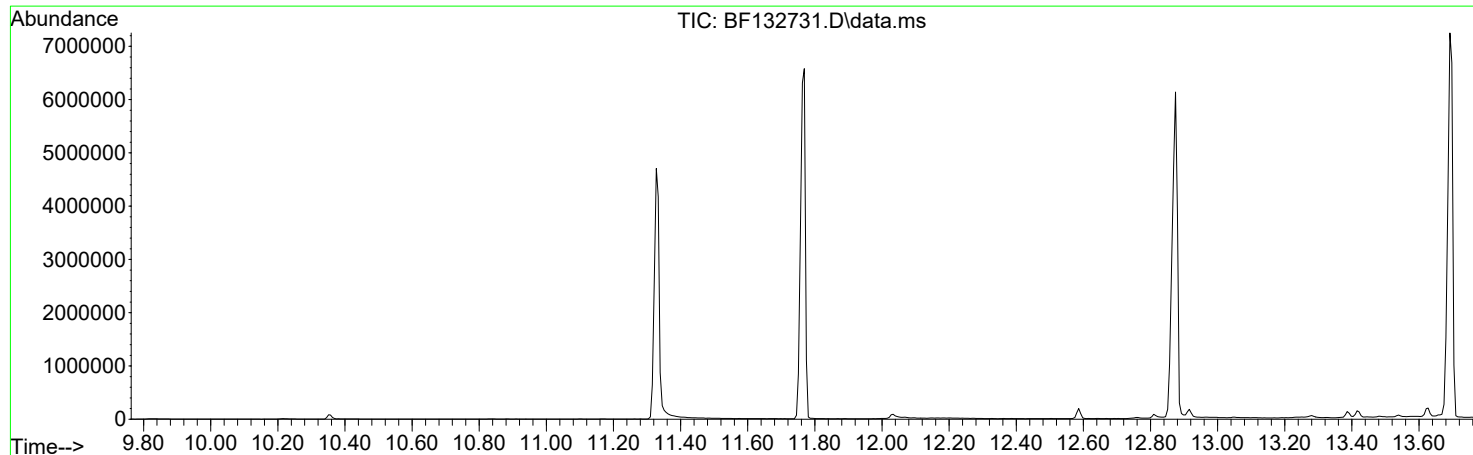

AutoFind: Scans 1559, 1560, 1561; Background Corrected with Scan 1554

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.4	168427	PASS
68	69	0.00	2	1.8	3312	PASS
69	198	0.00	100	31.3	186040	PASS
70	69	0.00	2	0.5	964	PASS
127	198	10	80	44.4	263659	PASS
197	198	0.00	2	0.8	4515	PASS
198	198	100	100	100.0	594005	PASS
199	198	5	9	7.0	41661	PASS
275	198	10	60	29.5	175280	PASS
365	198	1	100	4.0	23696	PASS
441	198	0.01	100	17.4	103331	PASS
442	442	50	100	100.0	674048	PASS
443	442	15	24	20.3	136504	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/10/2023	BNA_F	<u>BF132731.D</u>
Compound Name	Response	Retention Time
DDT	1534744	13.692
DDD	42723	13.386
DDE	3179	13.051
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
45902	1580646	2.90

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031023\
Data File : BF132731.D
Acq On : 10 Mar 2023 09:38
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 11 03:17:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 09 16:26:19 2023
Response via : Initial Calibration

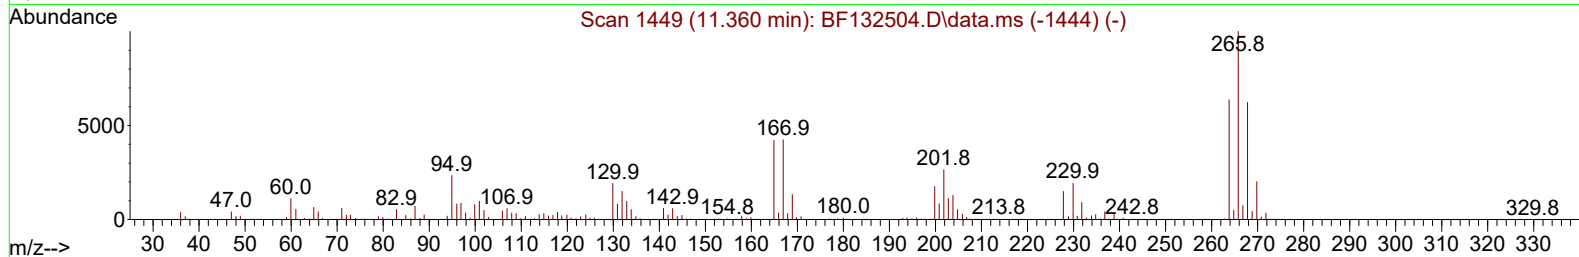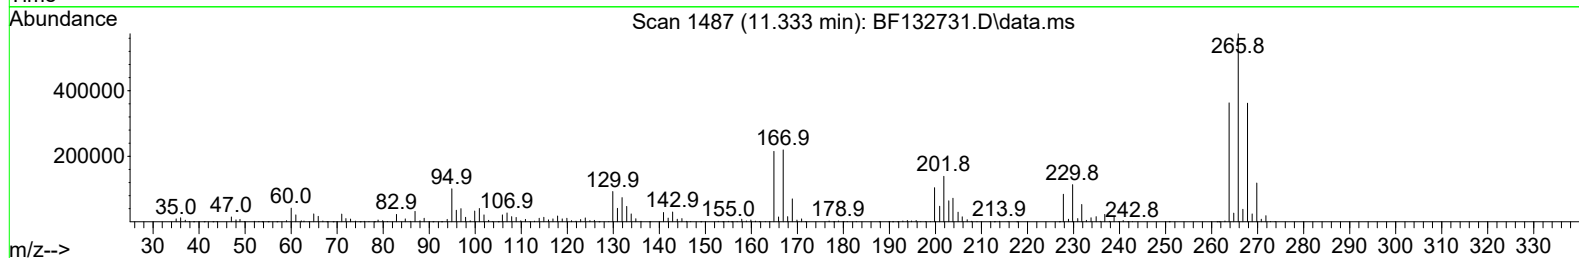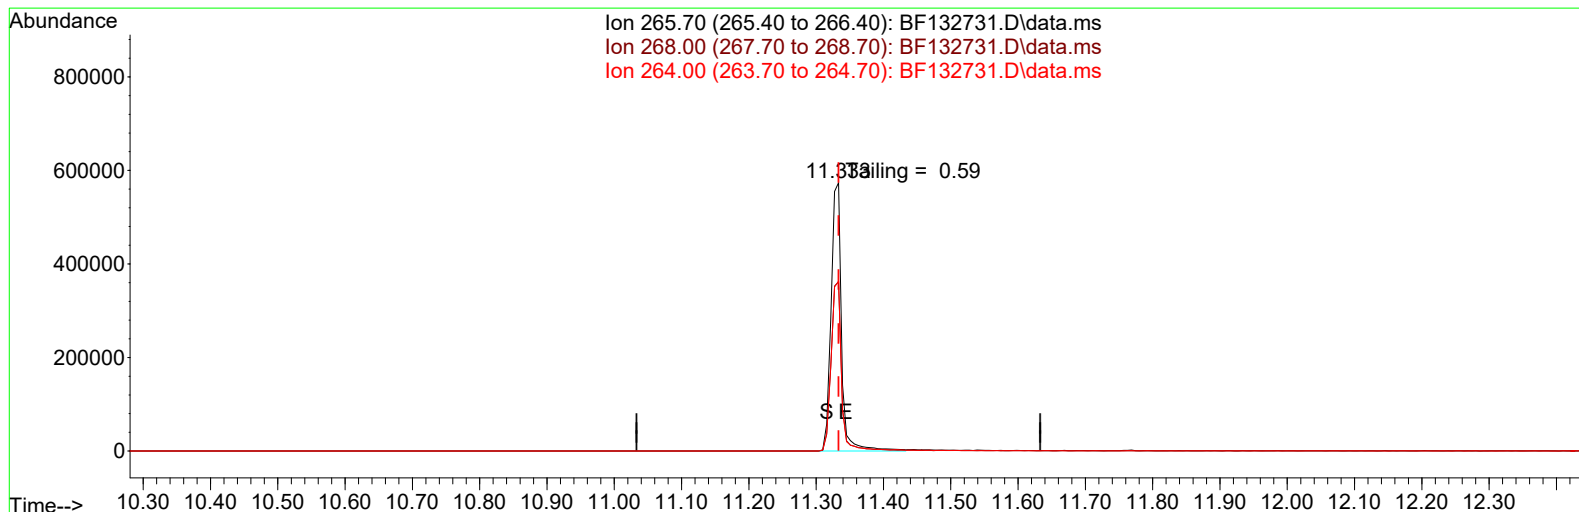

TIC: BF132731.D\data.ms

(70) Pentachlorophenol (C)

11.333min (+ 0.000) 728789.30 ng




response 619311

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.11
264.00	63.60	63.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031023\
 Data File : BF132731.D
 Acq On : 10 Mar 2023 09:38
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 11 03:17:05 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 16:26:19 2023
 Response via : Initial Calibration

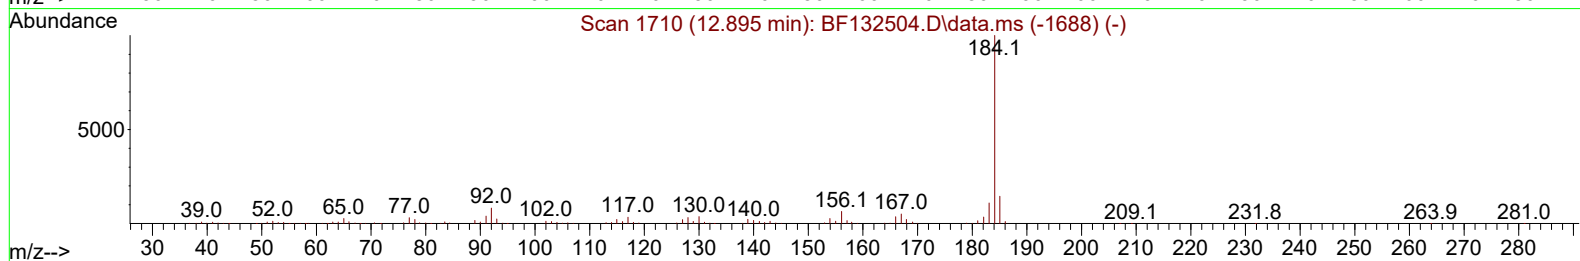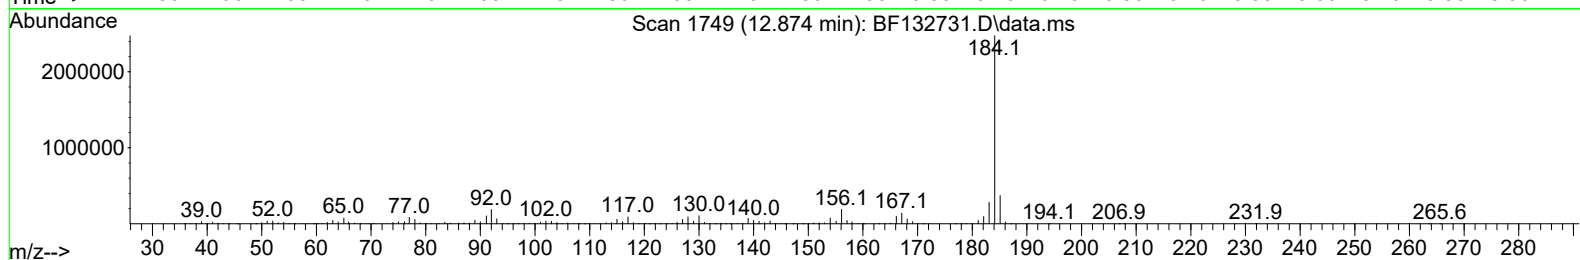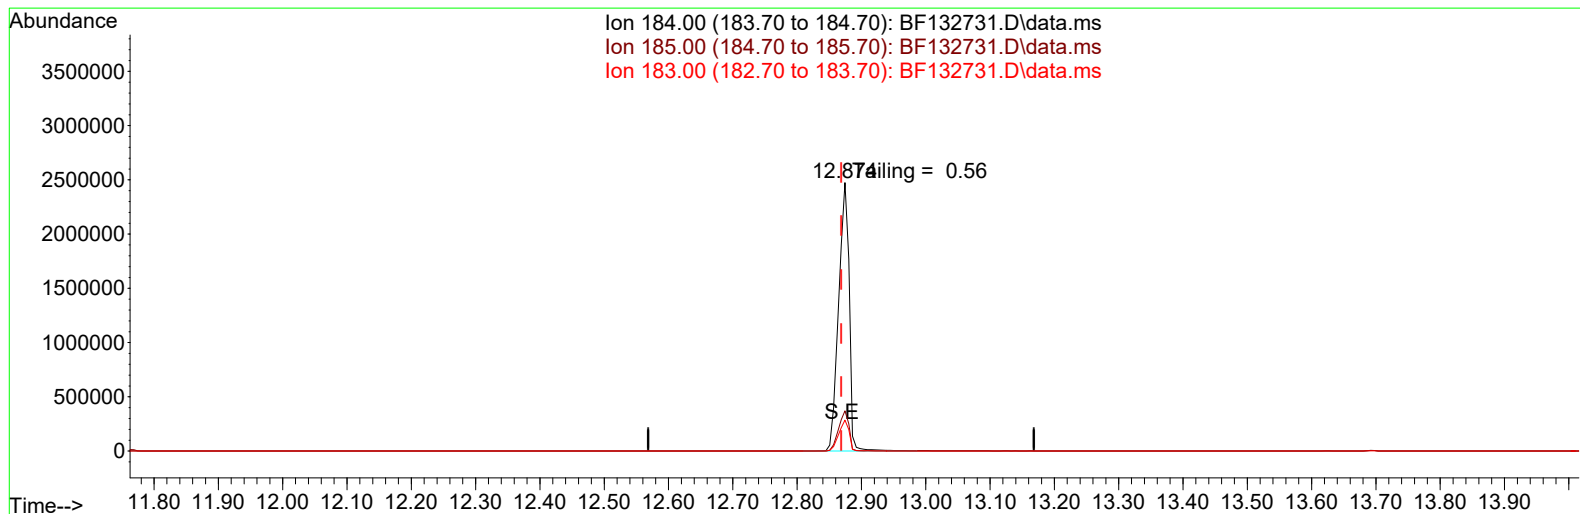

TIC: BF132731.D\data.ms

(77) Benzidine

12.874min (+ 0.006) 314182.94 ng

response 2845097

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.96
183.00	10.90	11.50
0.00	0.00	0.00