
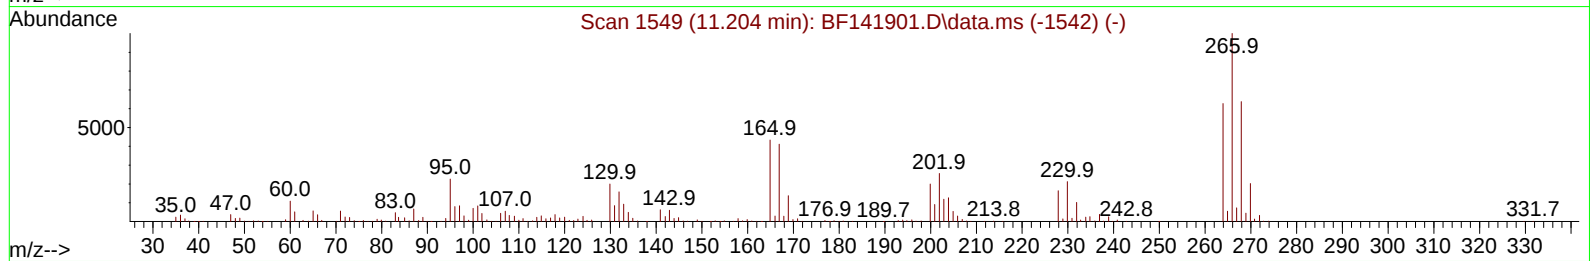
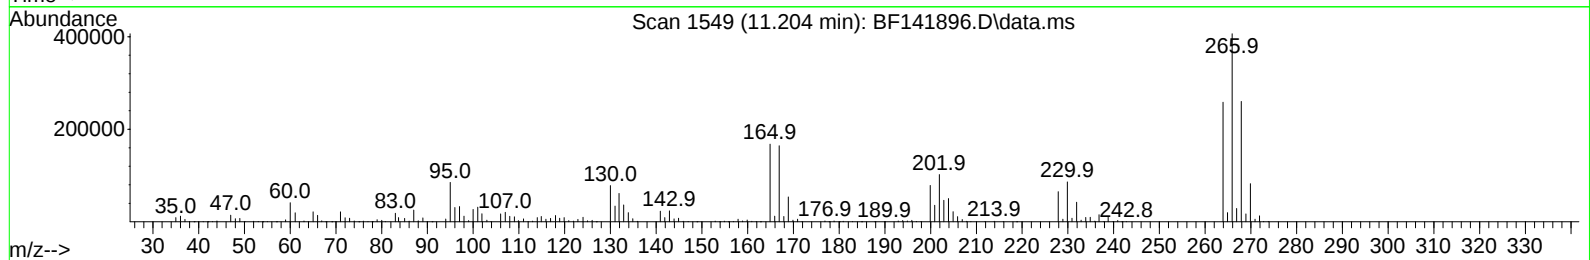


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031025\
Data File : BF141896.D
Acq On : 10 Mar 2025 10:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 16:16:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

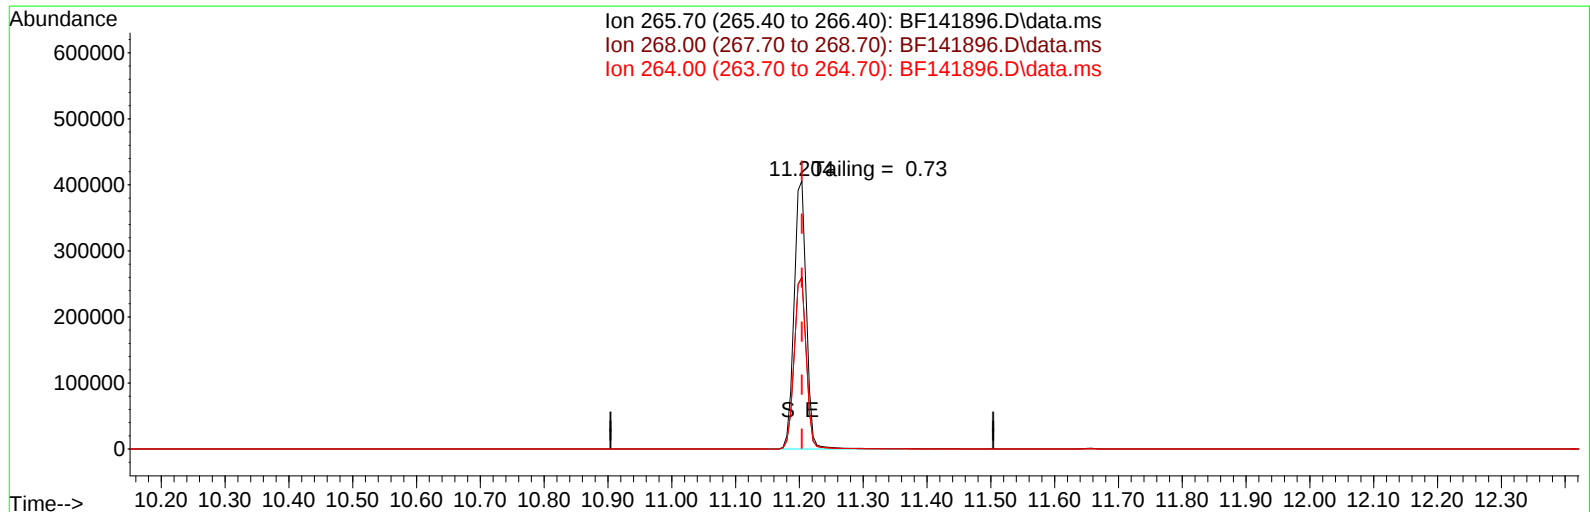

TIC: BF141896.D\data.ms

(70) Pentachlorophenol (C)




11.204min (-0.000) 118650.09 ng

response 544757

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.05
264.00	62.70	63.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031025\
Data File : BF141896.D
Acq On : 10 Mar 2025 10:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 16:16:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

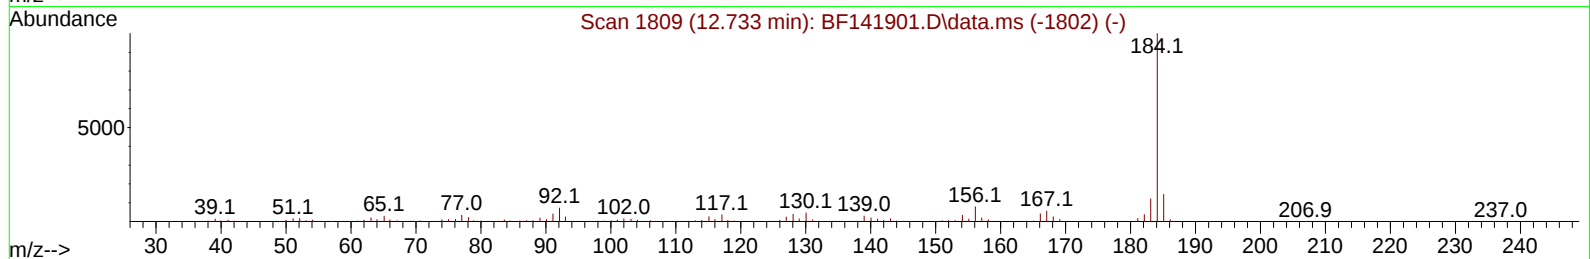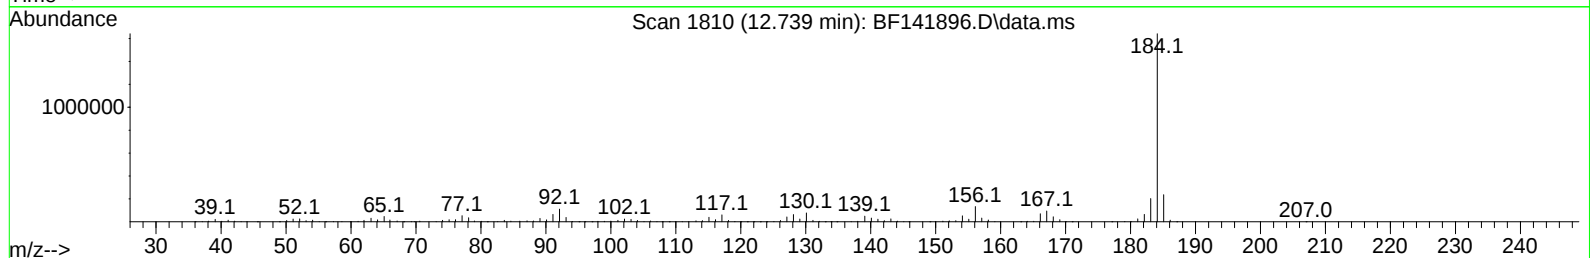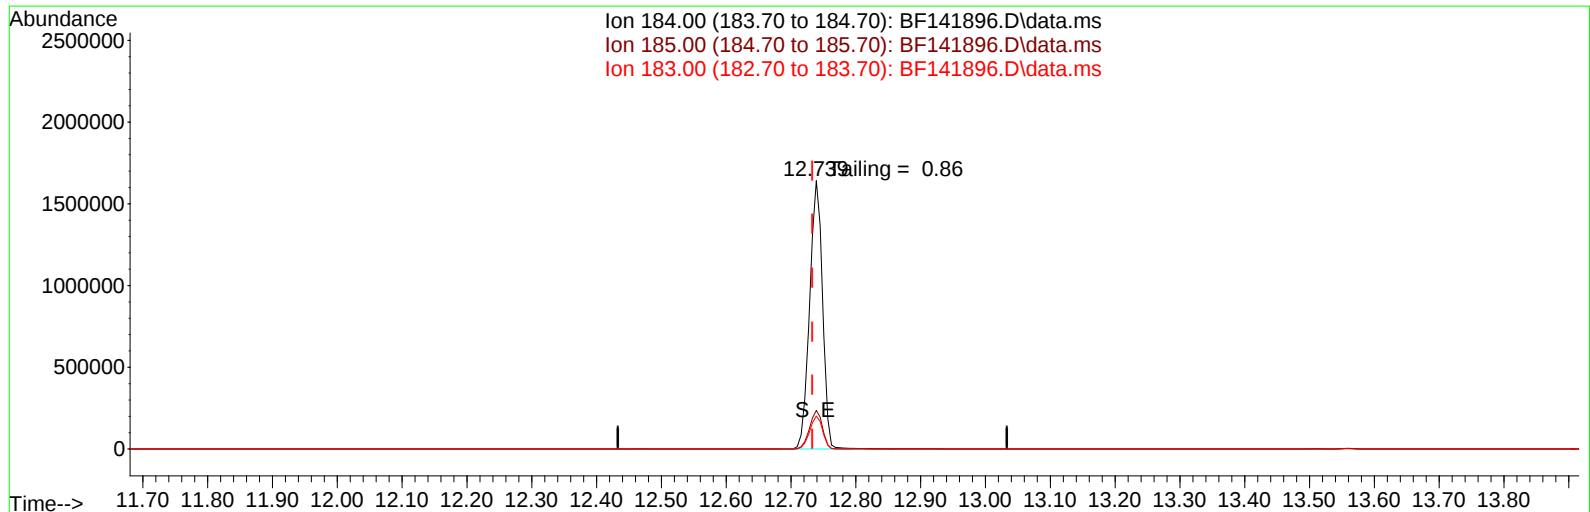

TIC: BF141896.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 203796.44 ng

response 2274676

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.38
183.00	12.10	12.32
0.00	0.00	0.00