

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031025\
 Data File : BF141907.D
 Acq On : 10 Mar 2025 17:09
 Operator : RC/JU
 Sample : PB167012BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB167012BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141907.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.263	22	29	39	rVB	56377	102696	1.09%	0.220%
2	5.504	573	580	586	rBV	3550145	5166667	54.87%	11.066%
3	6.498	742	749	755	rBV	3393065	5152688	54.72%	11.036%
4	6.881	808	814	819	rBV	989612	1279058	13.58%	2.739%
5	7.439	901	909	914	rBV	2445475	3537292	37.57%	7.576%
6	8.157	1025	1031	1042	rBV	1291655	1715042	18.21%	3.673%
7	9.233	1207	1214	1219	rBV	5374492	7444032	79.06%	15.943%
8	9.910	1323	1329	1345	rBV	1606953	2129910	22.62%	4.562%
9	10.704	1456	1464	1469	rBV	3895343	5394672	57.29%	11.554%
10	11.398	1576	1582	1587	rBV	1896011	2382653	25.30%	5.103%
11	12.986	1845	1852	1858	rBV	6797542	9415750	100.00%	20.166%
12	14.033	2025	2030	2041	rVB	1364012	1754967	18.64%	3.759%
13	15.504	2274	2280	2297	rVB	775825	1215164	12.91%	2.603%




Sum of corrected areas: 46690591

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031025\
Data File : BF141907.D
Acq On : 10 Mar 2025 17:09
Operator : RC/JU
Sample : PB167012BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB167012BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

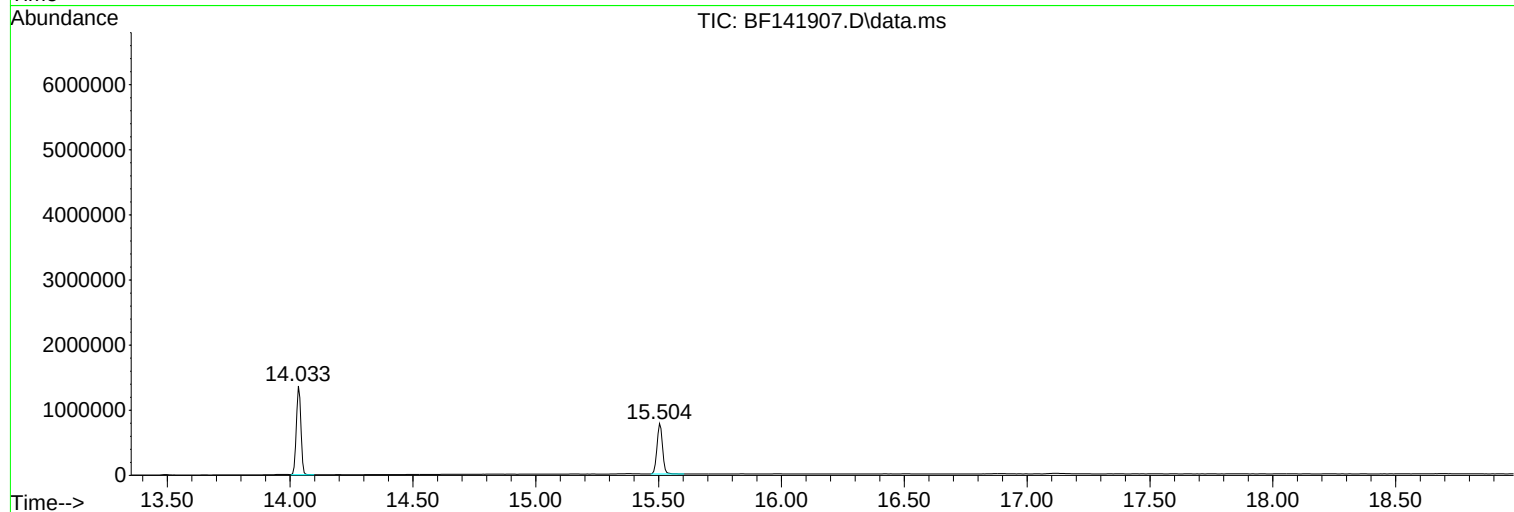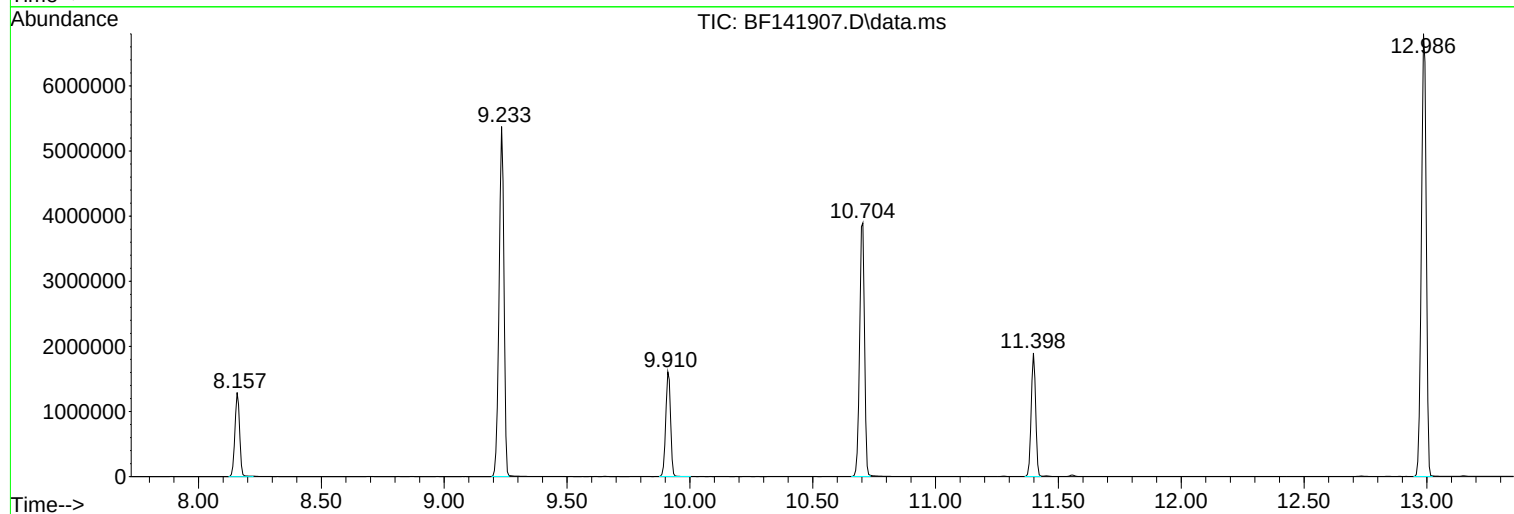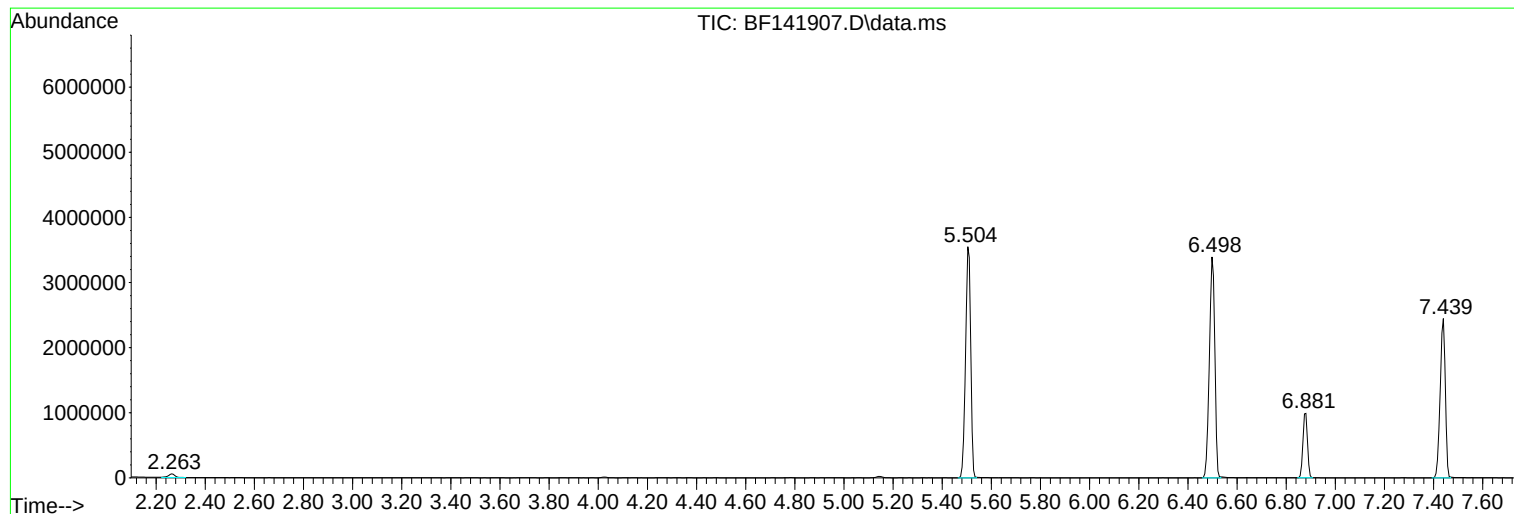

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031025\
Data File : BF141907.D
Acq On : 10 Mar 2025 17:09
Operator : RC/JU
Sample : PB167012BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB167012BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF031025\
Data File : BF141907.D
Acq On : 10 Mar 2025 17:09
Operator : RC/JU
Sample : PB167012BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB167012BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------