


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031115\
 Data File : BF077680.D
 Acq On : 11 Mar 2015 10:41
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 12 02:24:12 2015

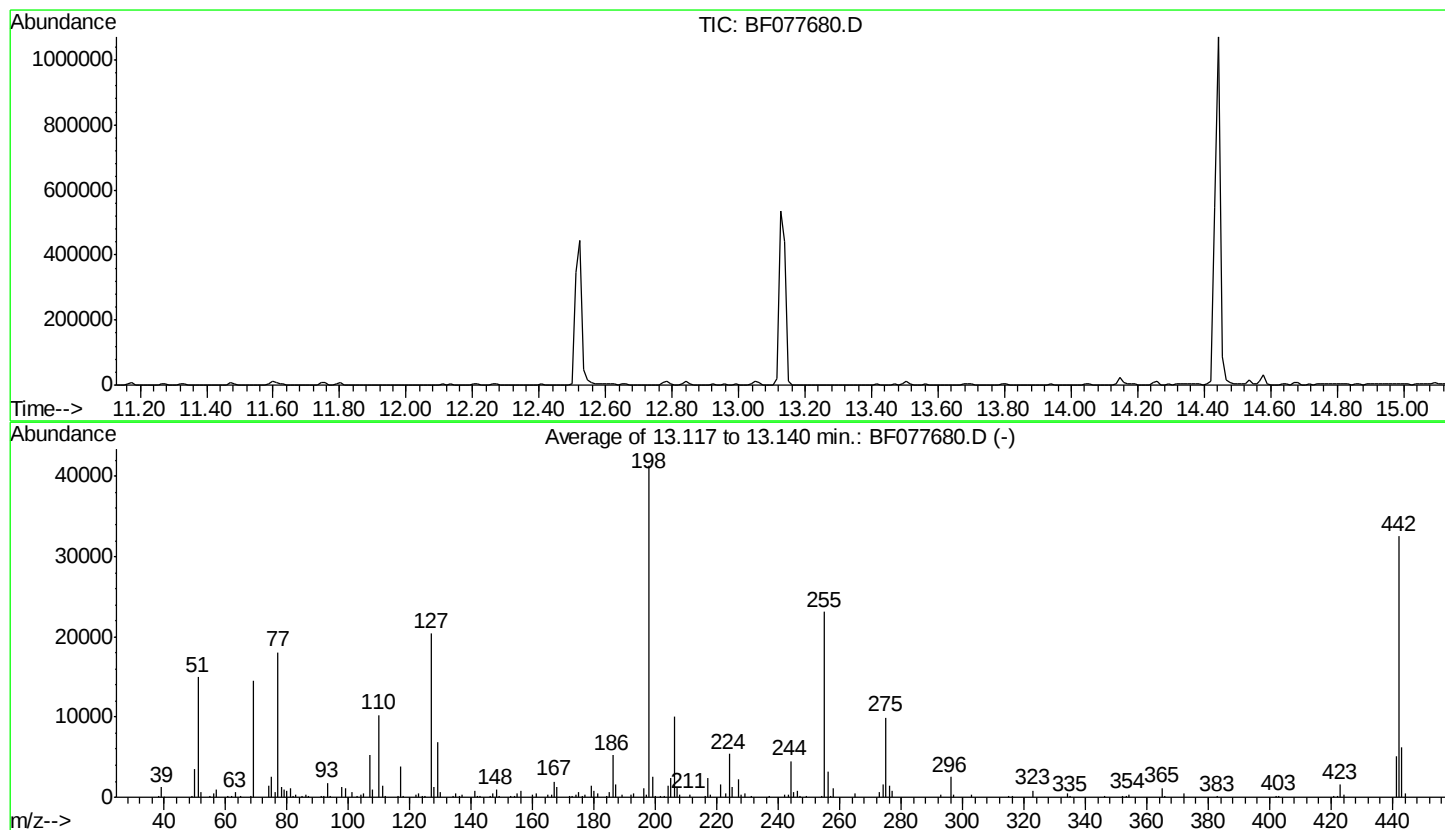

AutoFind: Scans 1070, 1071, 1072; Background Corrected with Scan 1067

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	14950	PASS
68	69	0.00	2	1.2	177	PASS
69	198	0.00	100	35.2	14556	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.3	20378	PASS
197	198	0.00	2	0.7	291	PASS
198	198	100	100	100.0	41348	PASS
199	198	5	9	6.2	2547	PASS
275	198	10	60	24.1	9954	PASS
365	198	1	100	2.7	1123	PASS
441	442	0.01	24	15.5	5044	PASS
442	198	50	100	78.6	32490	PASS
443	442	15	24	19.2	6234	PASS