



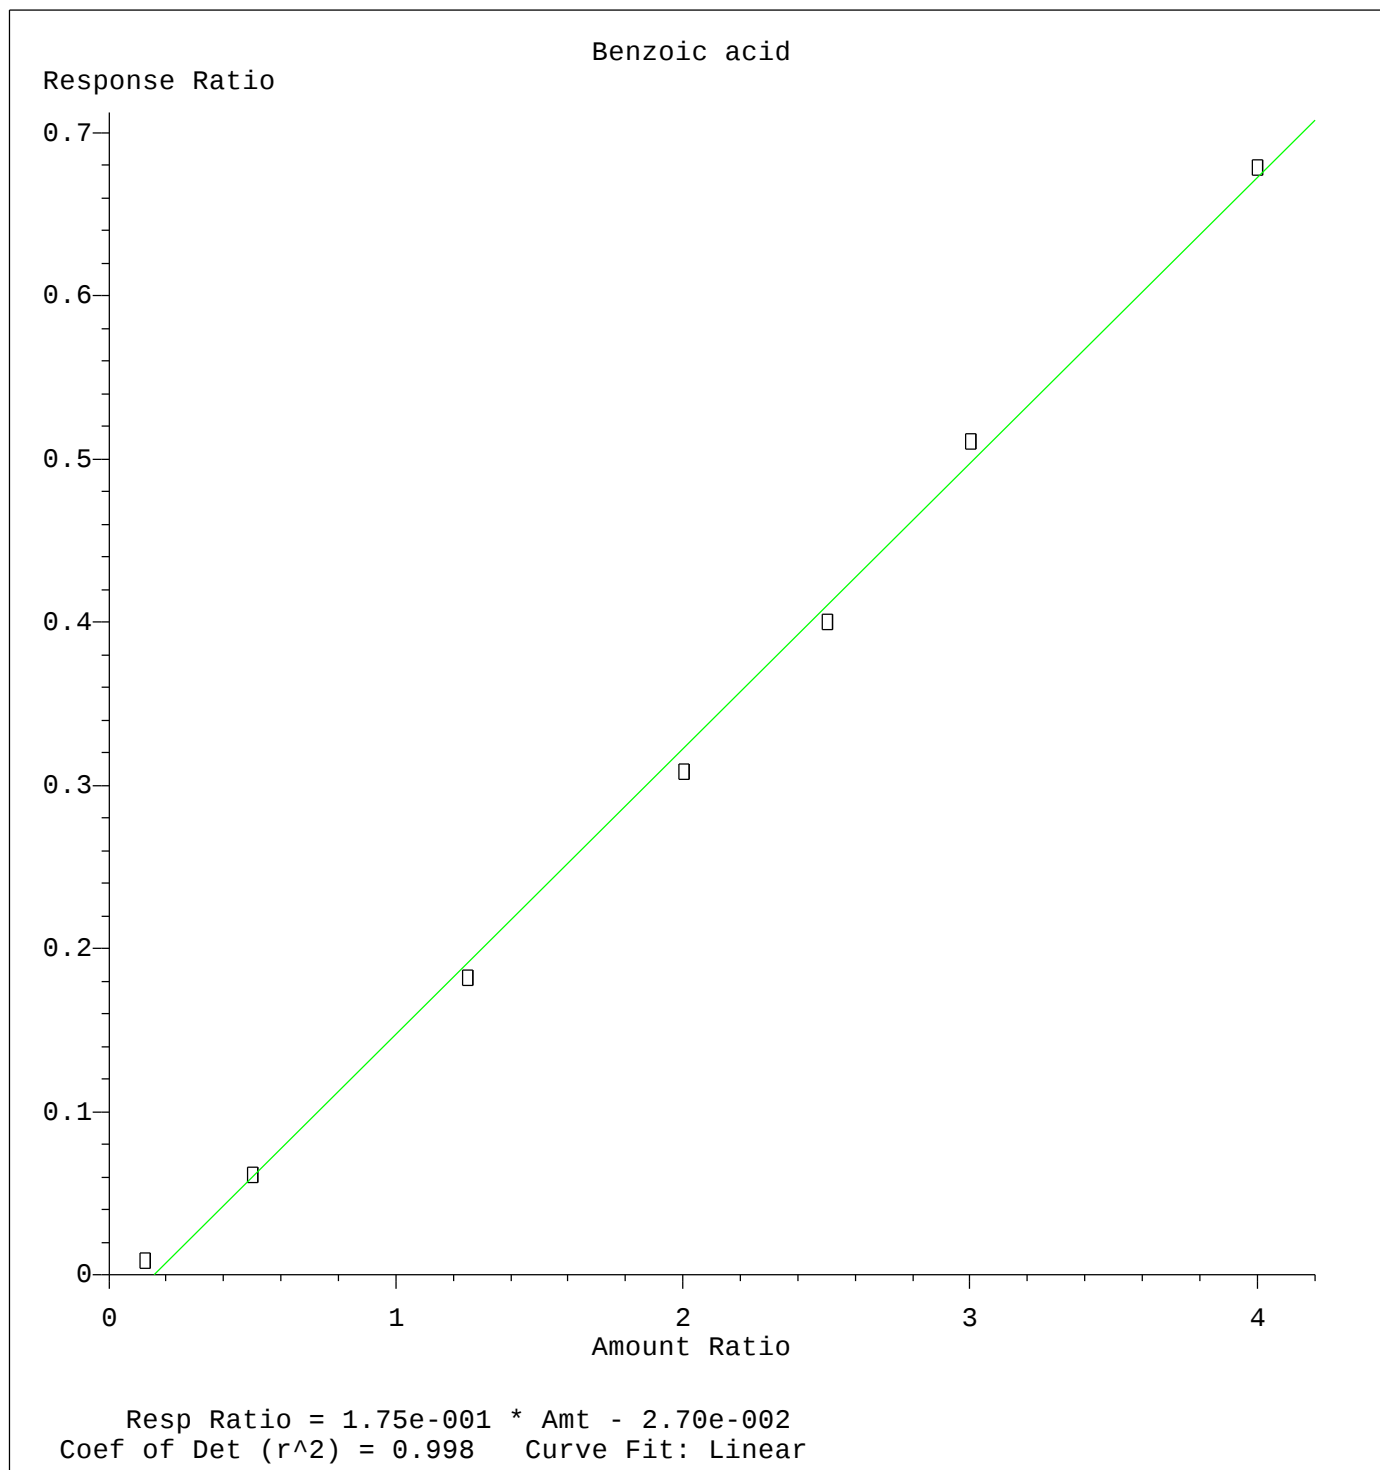

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Calibration Table Last Updated: Thu Mar 12 02:20:25 2015


Hexachlorocyclopentadiene

Response Ratio

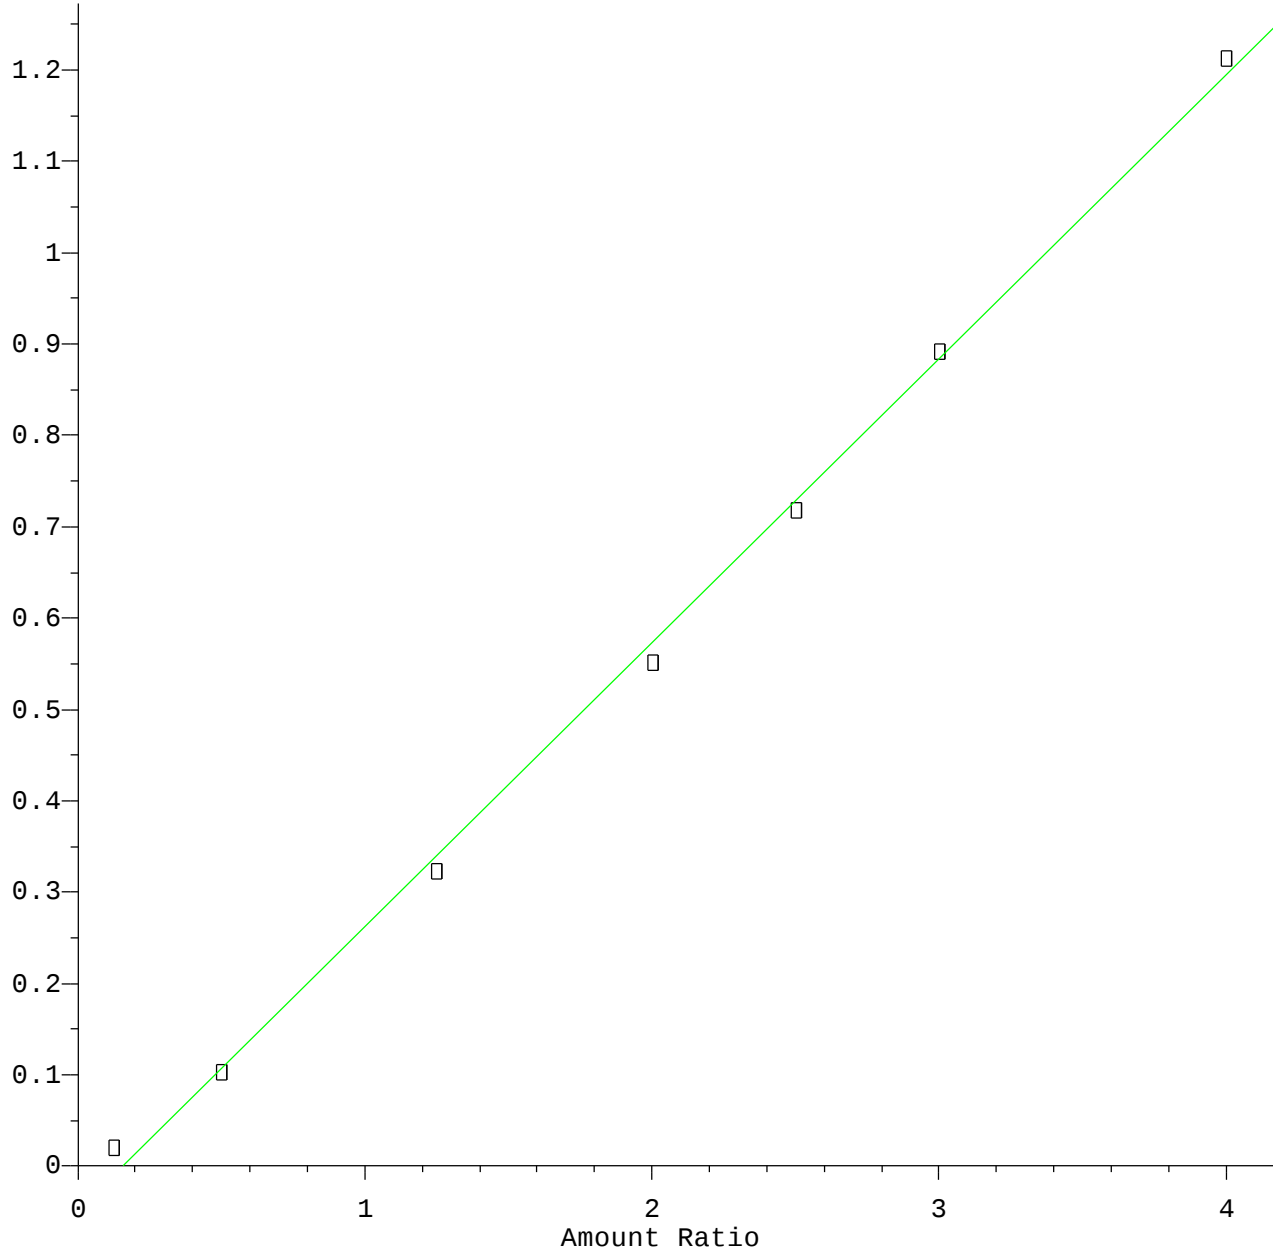


Resp Ratio = $3.11 \times 10^{-1} \times \text{Amt} - 4.92 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Calibration Table Last Updated: Thu Mar 12 02:22:15 2015

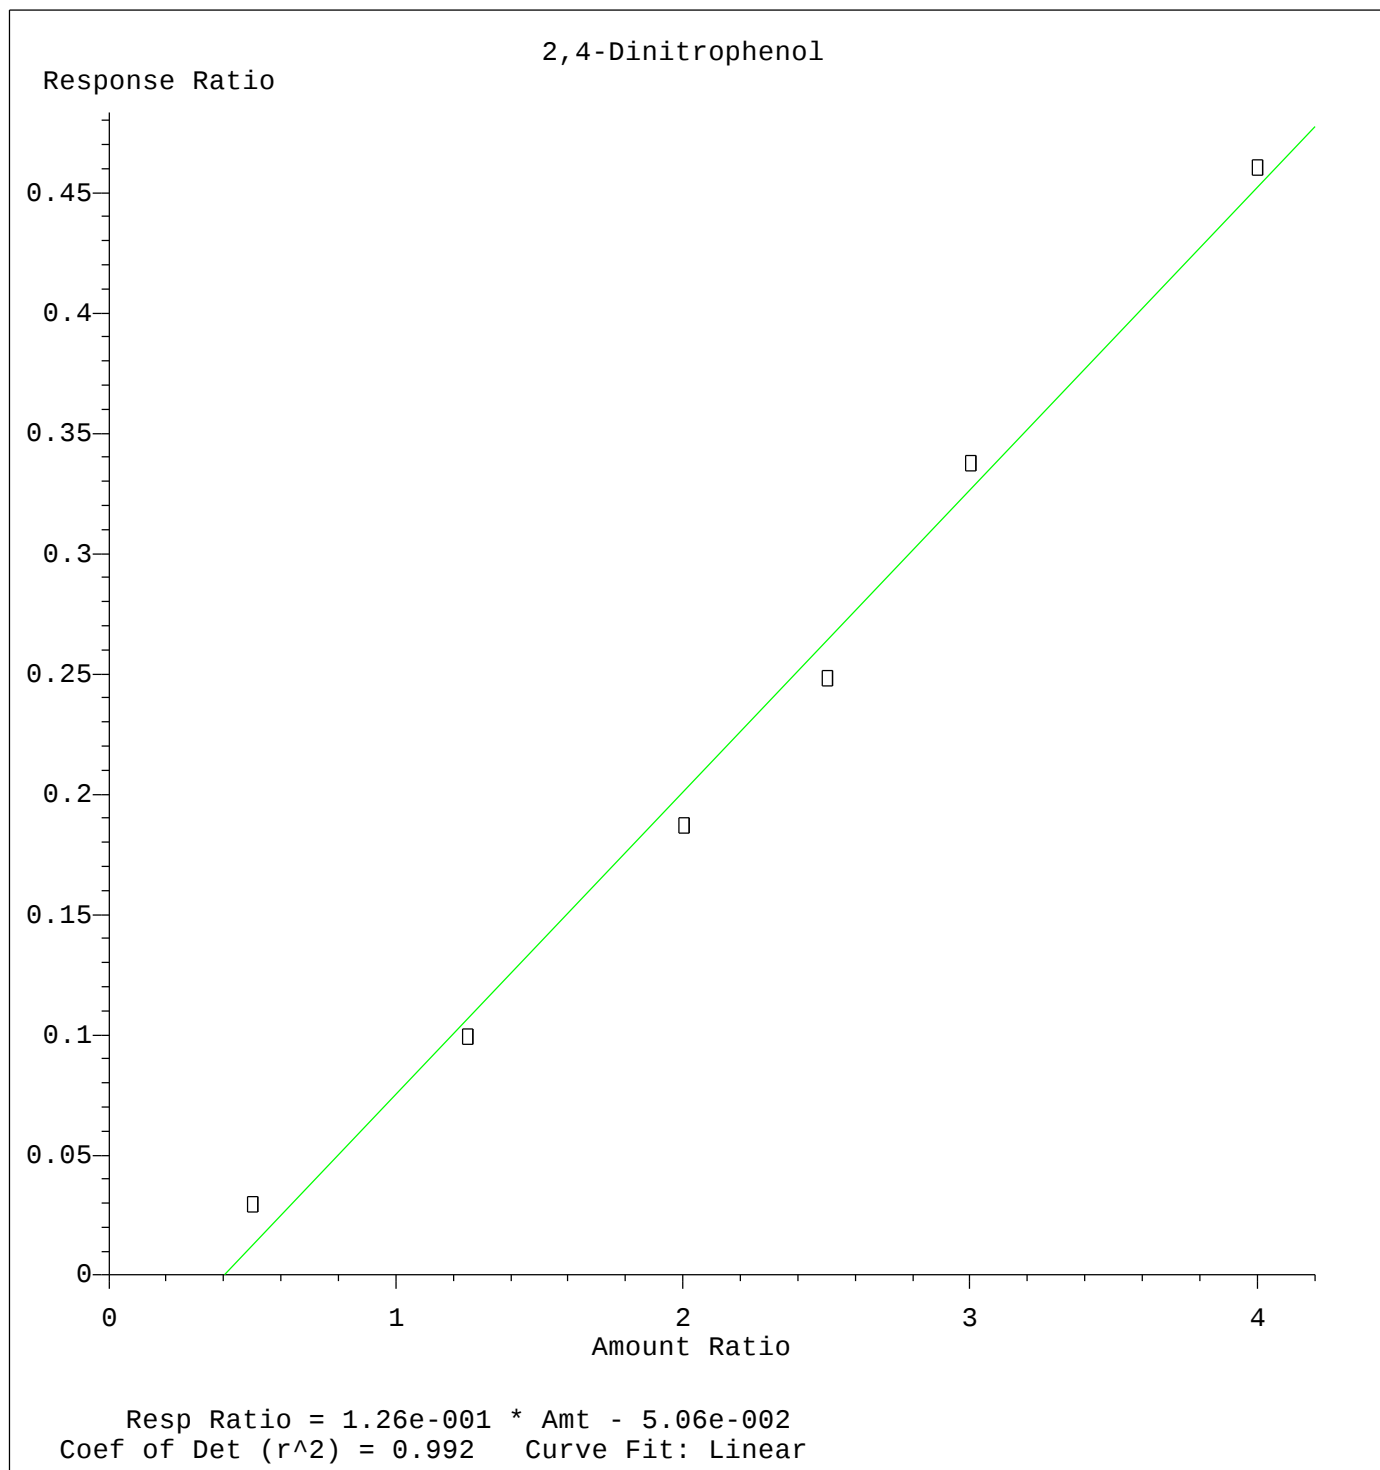


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Calibration Table Last Updated: Thu Mar 12 02:22:40 2015

4,6-Dinitro-2-methylphenol

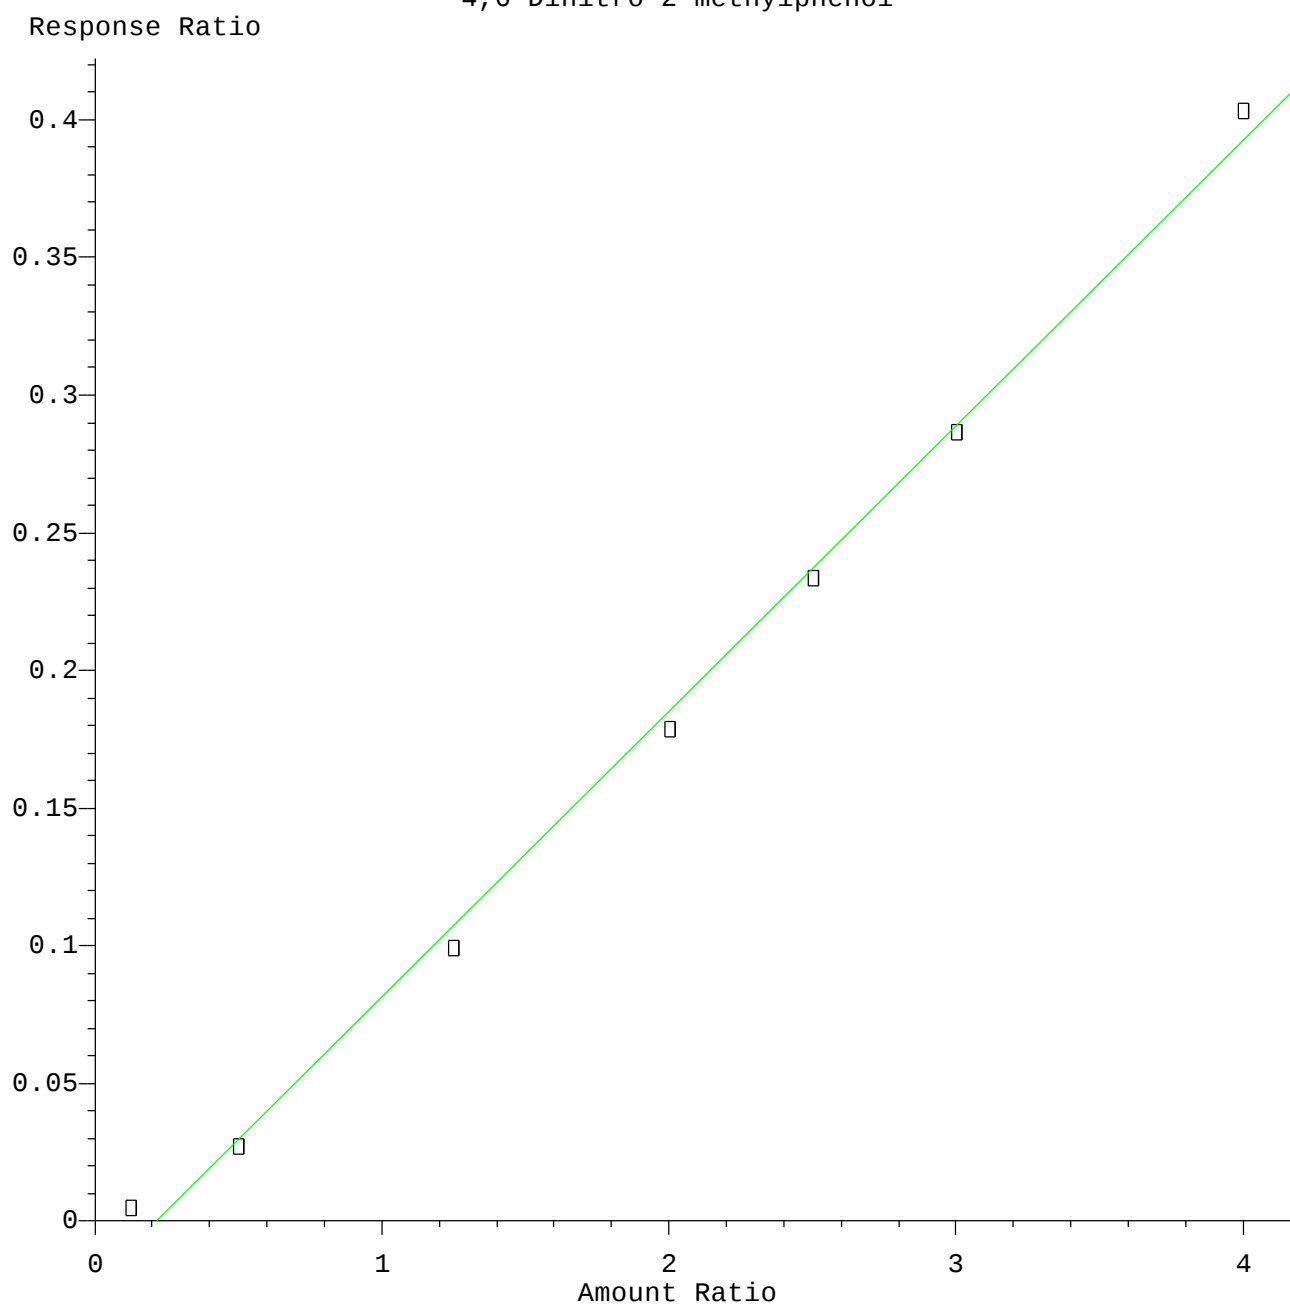


Resp Ratio = $1.04 \times 10^{-1} \times \text{Amt} - 2.23 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Calibration Table Last Updated: Thu Mar 12 02:23:05 2015

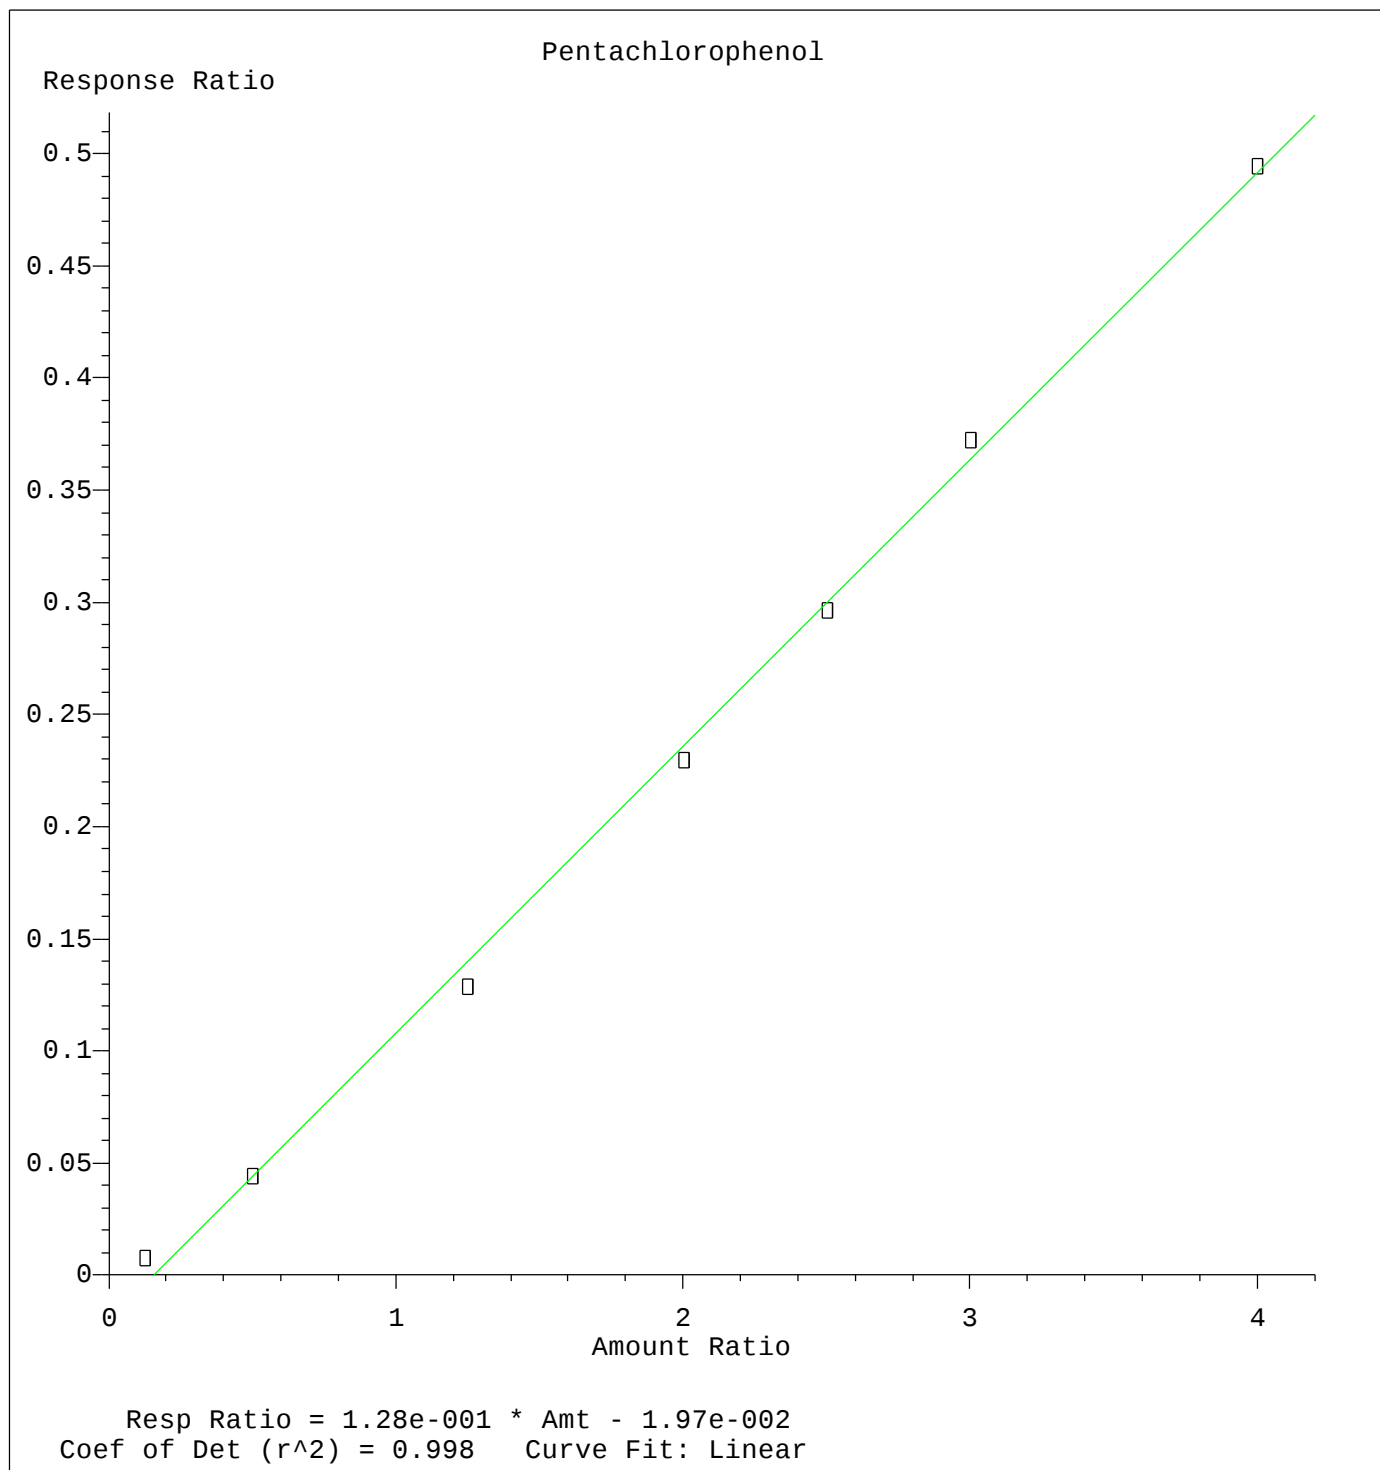

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Calibration Table Last Updated: Thu Mar 12 02:23:31 2015

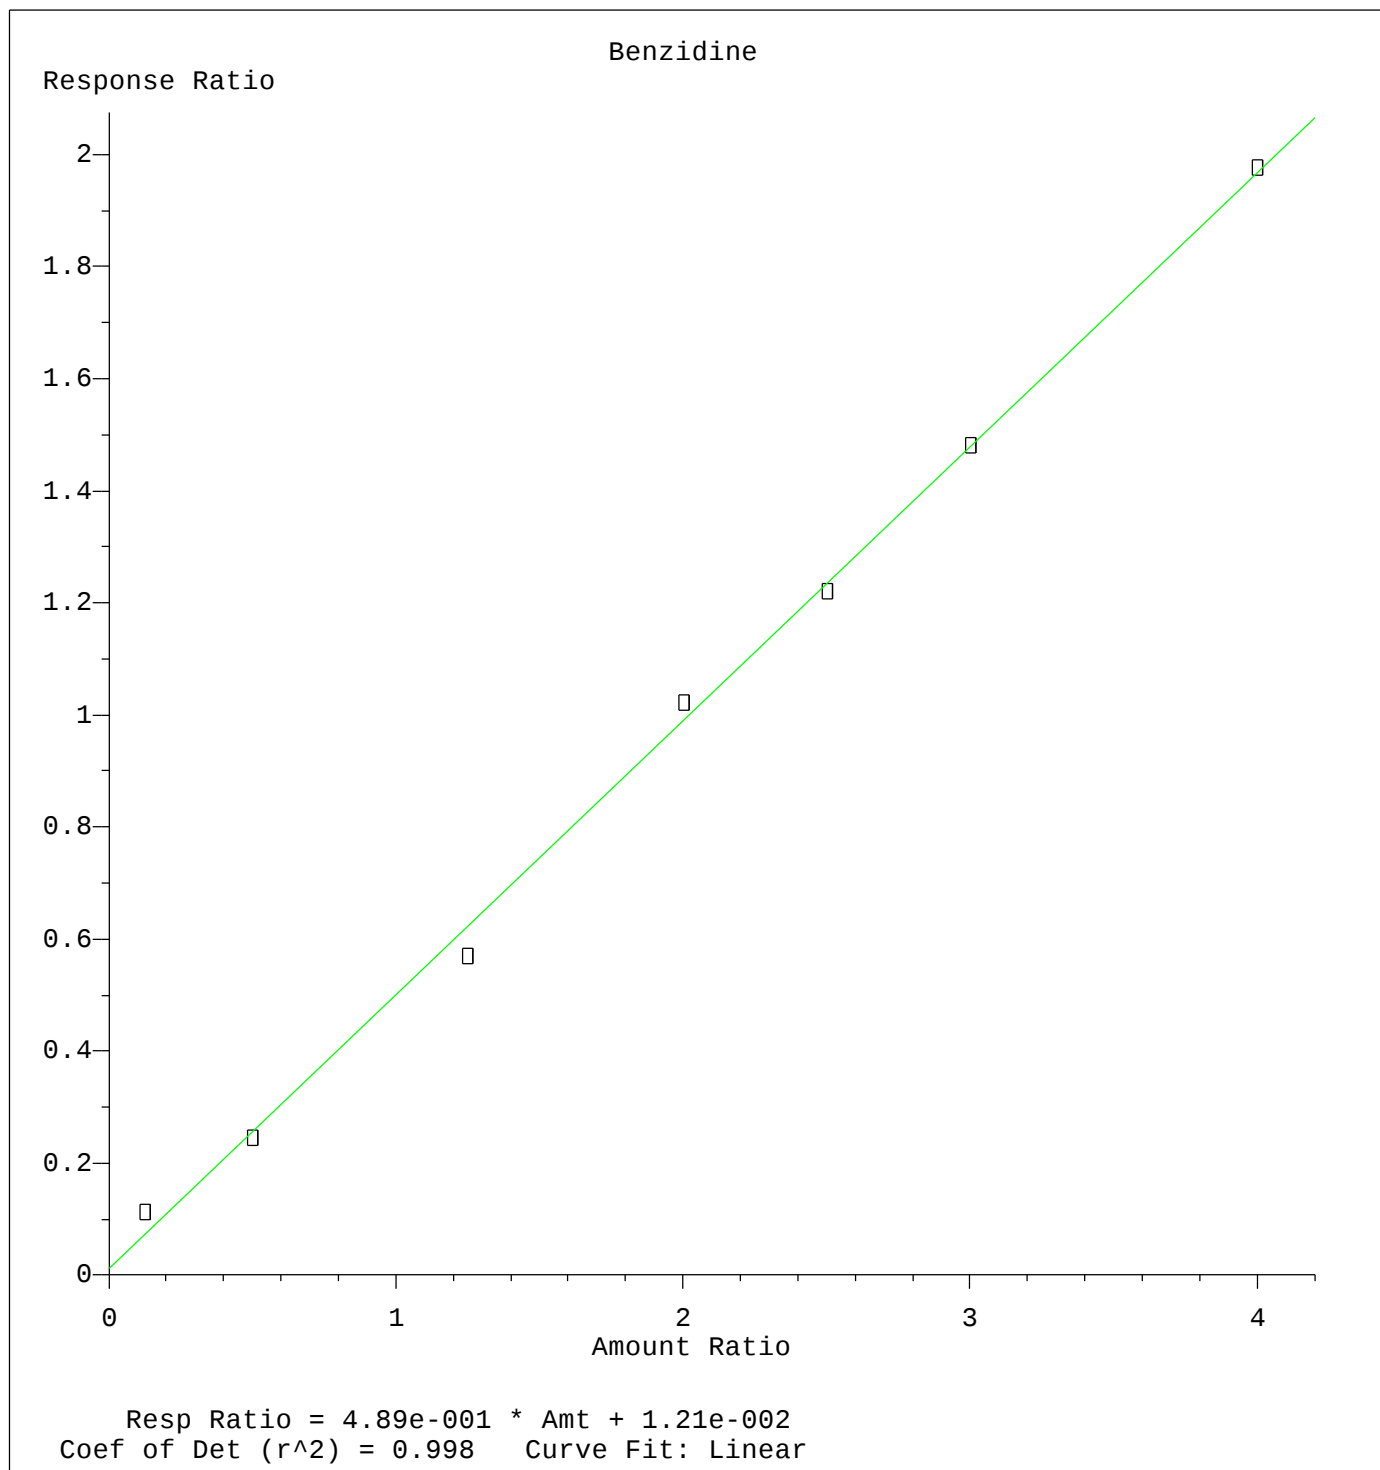

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Calibration Table Last Updated: Thu Mar 12 02:23:52 2015