

Data Path : Z:\HPCHEM1\BNA_F\Data\BF031115\
 Data File : BF077718.D
 Acq On : 12 Mar 2015 6:59
 Operator : TP/IZ
 Sample : G1454-01
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DCW-WW-081-3615

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.458	46	50	53	rVB	321950	481018	20.96%	3.606%
2	1.618	61	64	68	rVB	298451	360157	15.69%	2.700%
3	1.676	68	69	71	rBV	36915	48301	2.10%	0.362%
4	1.790	78	79	96	rBV	328766	546357	23.81%	4.096%
5	4.933	353	354	361	rVB	48656	60247	2.63%	0.452%
6	5.459	397	400	403	rBV	560402	571783	24.92%	4.287%
7	6.739	510	512	514	rBV	363024	352606	15.37%	2.644%
8	6.876	522	524	527	rBV	1071656	1130454	49.26%	8.475%
9	7.173	548	550	552	rBV	235791	268451	11.70%	2.013%
10	7.356	563	566	568	rBV	1246590	1114614	48.57%	8.356%
11	7.859	608	610	613	rBV	809114	822181	35.83%	6.164%
12	8.739	685	687	690	rBV	287950	370242	16.13%	2.776%
13	10.088	803	805	808	rBV	2056102	1848474	80.55%	13.858%
14	10.911	875	877	880	rBV	464994	447424	19.50%	3.354%
15	11.894	960	963	965	rBV	1046524	1099143	47.90%	8.240%
16	12.751	1036	1038	1041	rBV	507400	476034	20.74%	3.569%
17	14.751	1210	1213	1215	rBV	1619290	2294781	100.00%	17.204%
18	15.917	1312	1315	1317	rBV2	15033	24311	1.06%	0.182%
19	16.031	1322	1325	1327	rBV	378903	512084	22.32%	3.839%
20	17.734	1471	1474	1477	rBV	391322	509857	22.22%	3.822%


Sum of corrected areas: 13338519

Data Path : Z:\HPCHEM1\BNA_F\Data\BF031115\
Data File : BF077718.D
Acq On : 12 Mar 2015 6:59
Operator : TP/IZ
Sample : G1454-01
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DCW-WW-081-3615

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

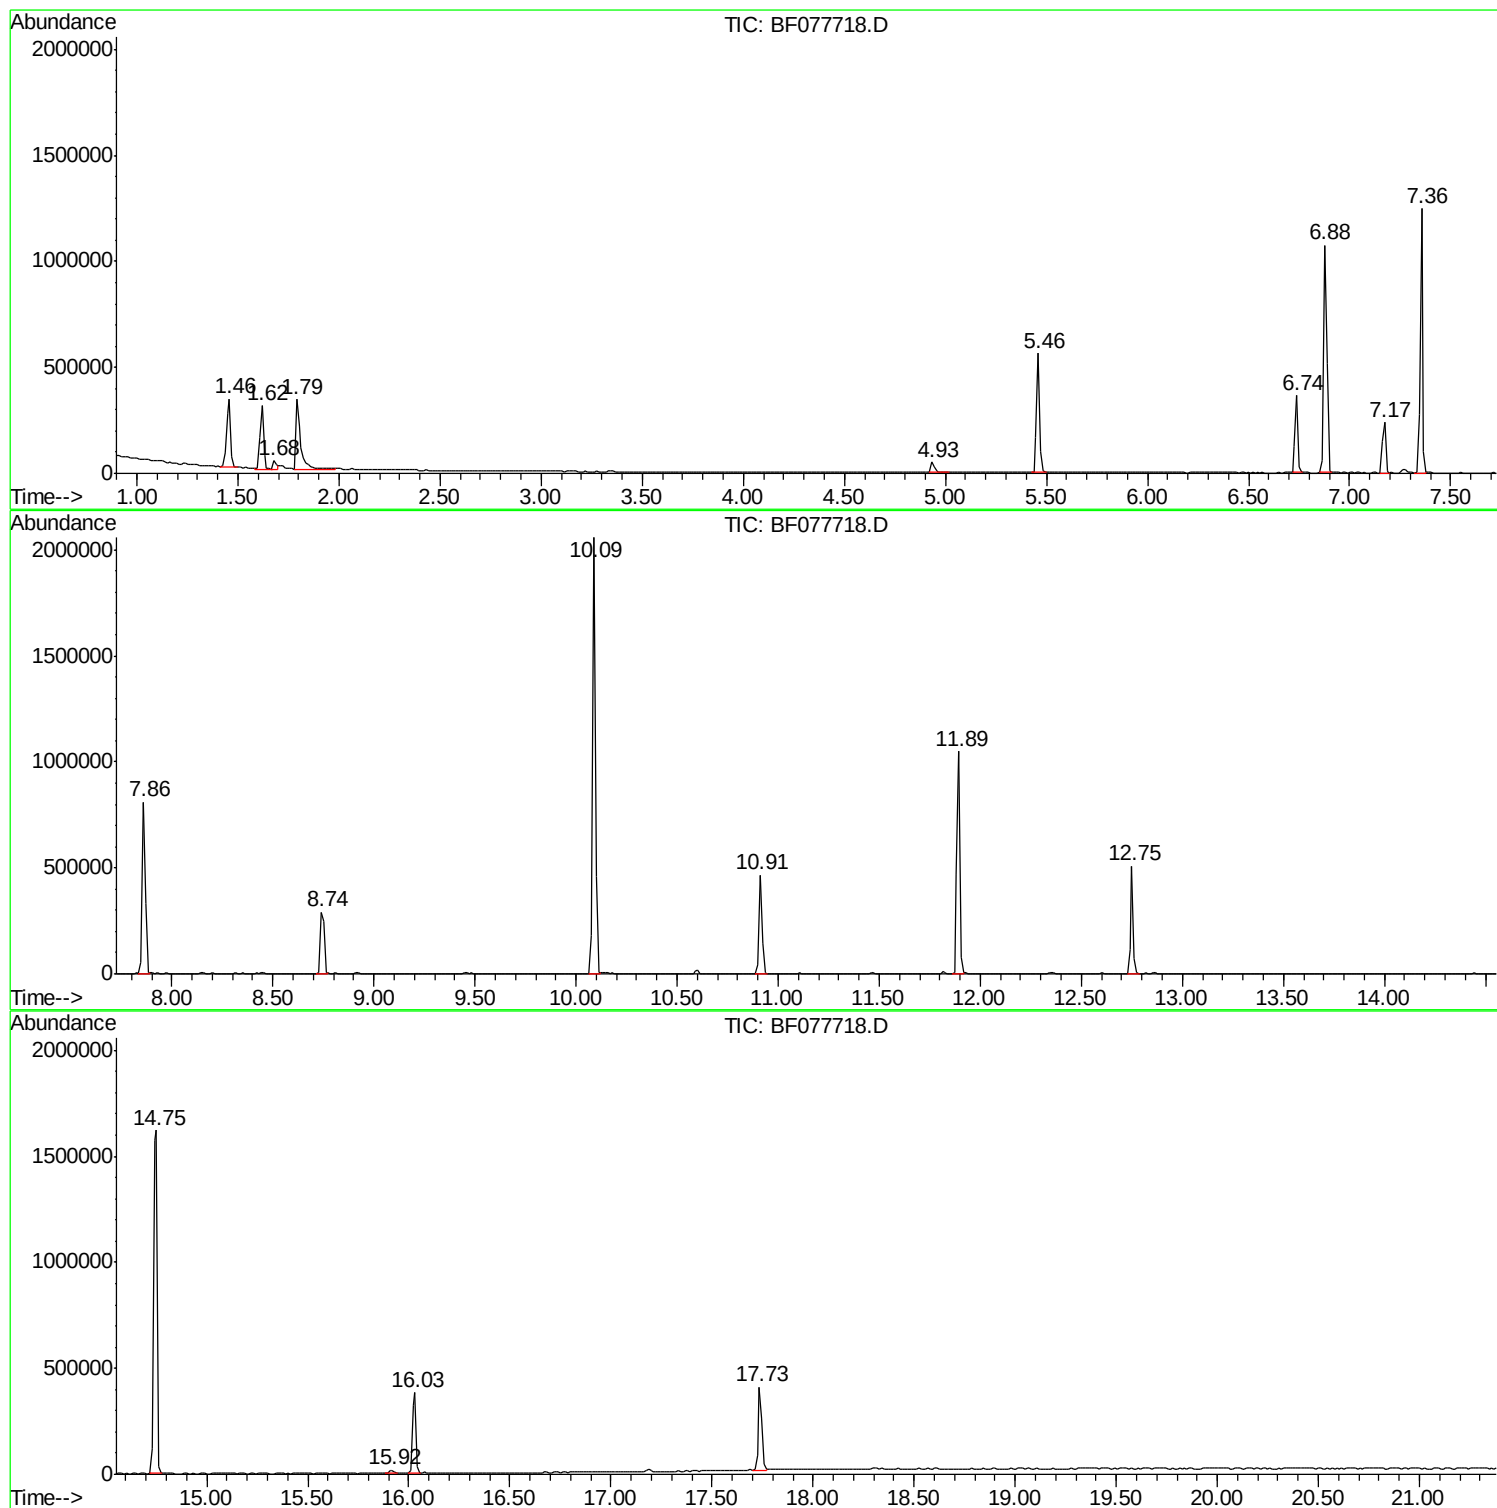

Data Path : Z:\HPCHEM1\BNA_F\Data\BF031115\
Data File : BF077718.D
Acq On : 12 Mar 2015 6:59
Operator : TP/IZ
Sample : G1454-01
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DCW-WW-081-3615

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_F\Data\BF031115\
Data File : BF077718.D
Acq On : 12 Mar 2015 6:59
Operator : TP/IZ
Sample : G1454-01
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DCW-WW-081-3615

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc