
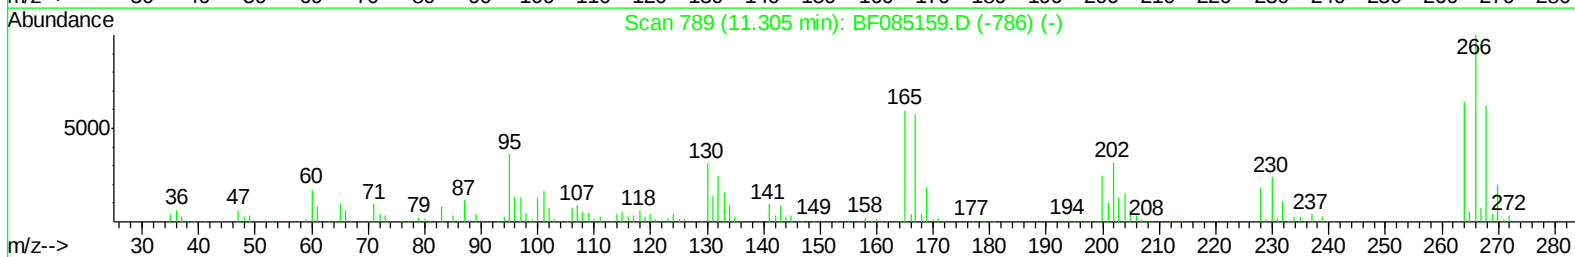
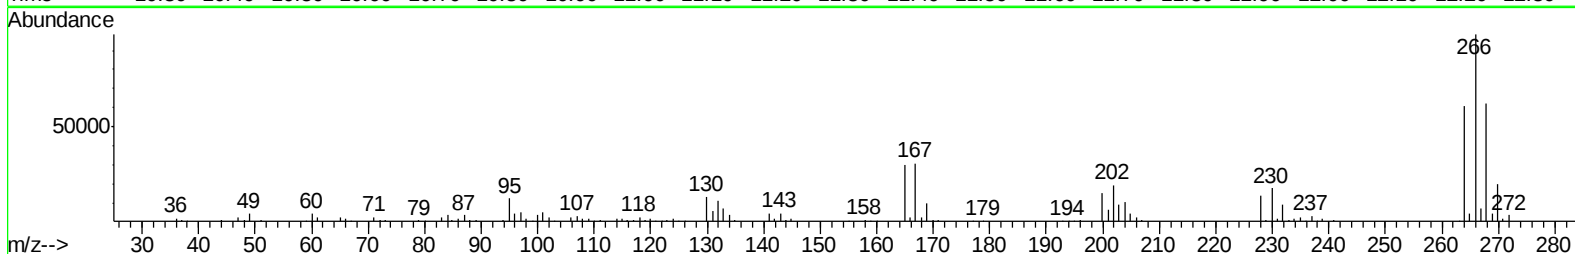


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031116\
Data File : BF085368.D
Acq On : 11 Mar 2016 13:19
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 12 00:09:07 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 04 00:54:58 2016
Response via : Initial Calibration

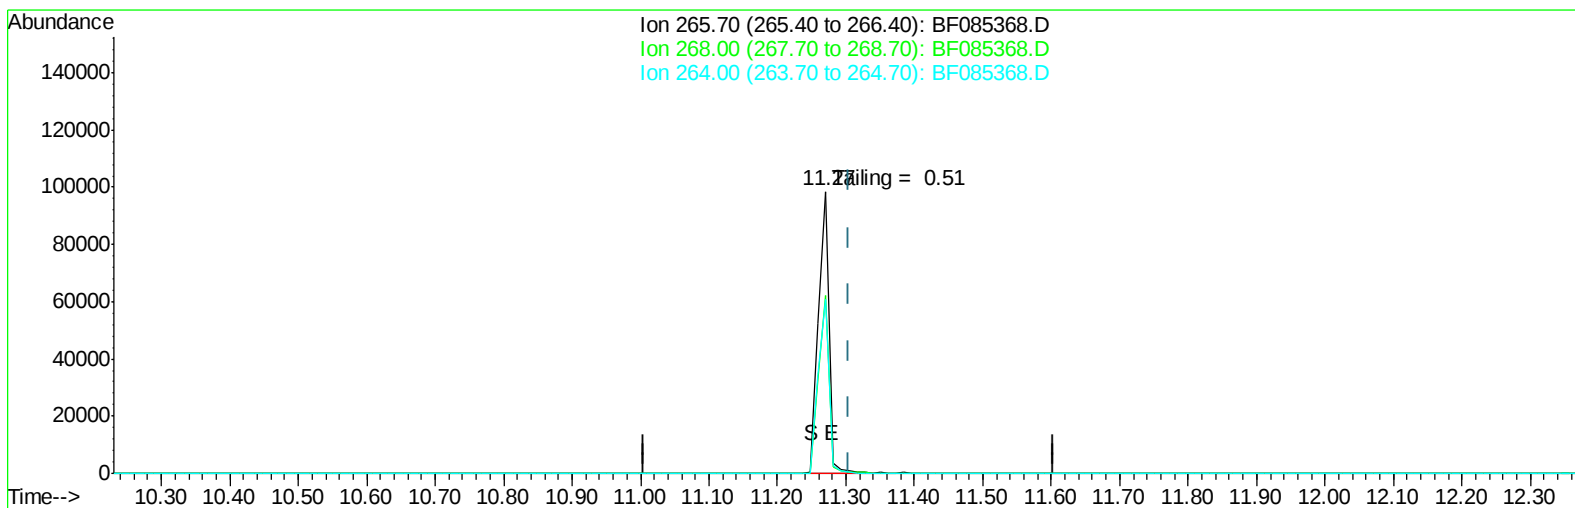

TIC: BF085368.D

(69) Pentachlorophenol (C)




11.271min (-0.034) 55774.48ng

response 108716

Ion	Exp%	Act%
265.70	100	100
268.00	62.50	63.38
264.00	64.30	61.65
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF031116\
Data File : BF085368.D
Acq On : 11 Mar 2016 13:19
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 12 00:09:07 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 04 00:54:58 2016
Response via : Initial Calibration

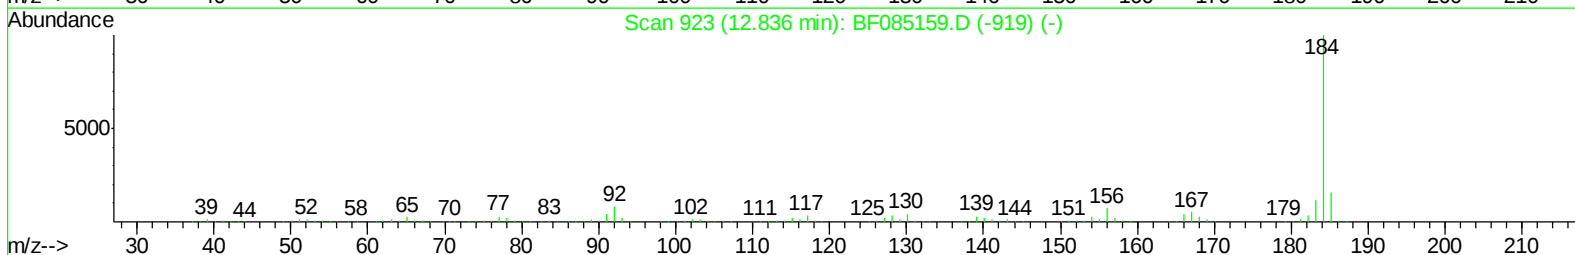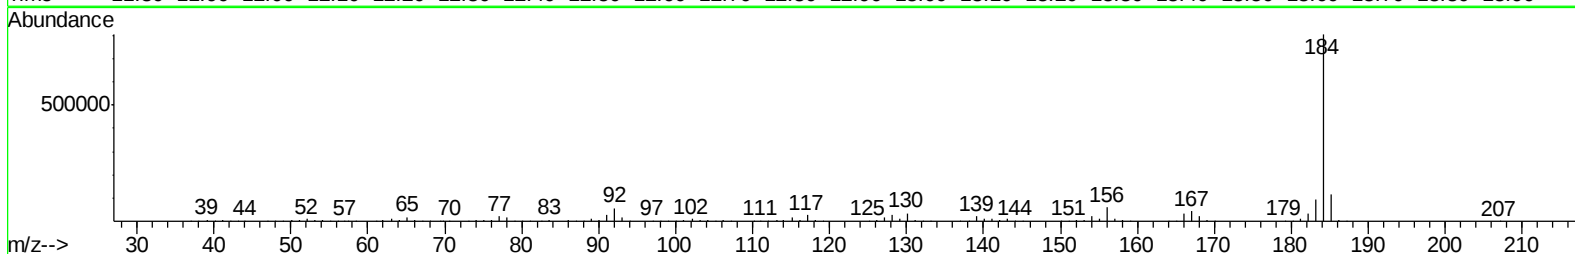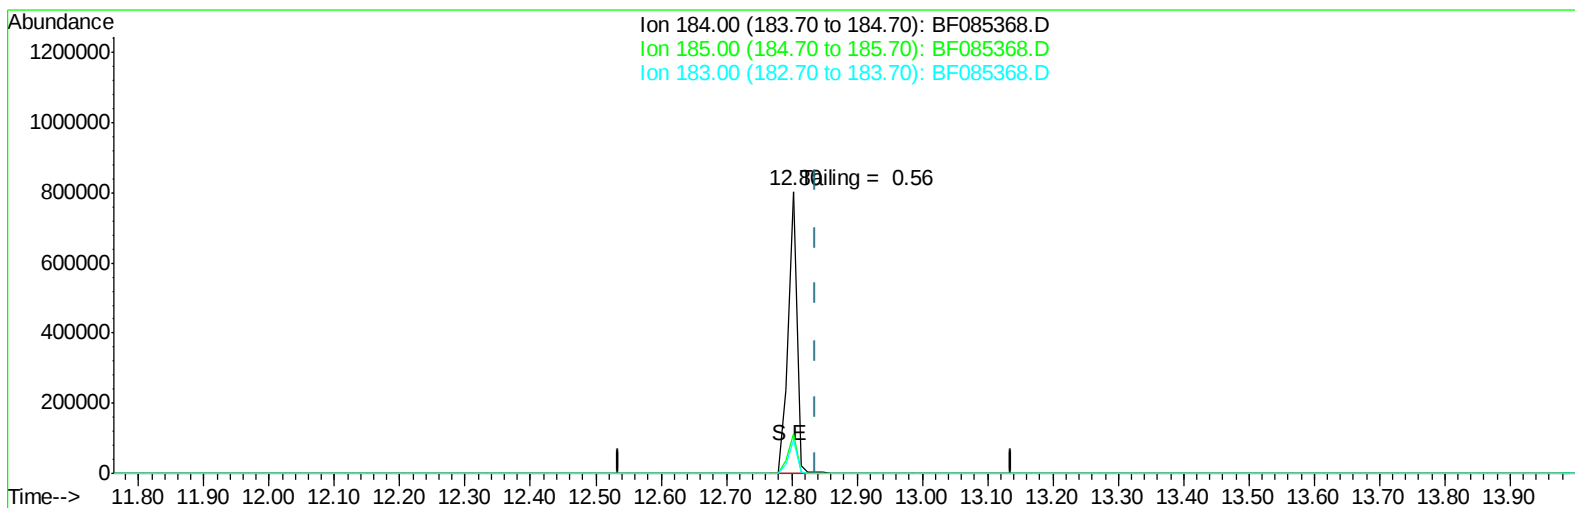

TIC: BF085368.D

(76) Benzidine

12.802min (-0.034) 68998.83ng

response 743383

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.25
183.00	11.80	11.75
0.00	0.00	0.00